

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036234.D
 Acq On : 12 Aug 2022 17:32
 Operator : CG/JU
 Sample : N4095-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GBJM8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036234.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	11	16	33	rVB	1083301	1463692	31.25%	3.648%
2	3.657	94	97	111	rBV	116323	188795	4.03%	0.471%
3	3.875	130	134	139	rVB	20806	29613	0.63%	0.074%
4	3.969	147	150	155	rVB	16090	20557	0.44%	0.051%
5	4.416	222	226	231	rVB	34958	44609	0.95%	0.111%
6	4.499	235	240	249	rBV	61238	85645	1.83%	0.213%
7	4.904	306	309	312	rVB4	4597	5047	0.11%	0.013%
8	5.022	326	329	333	rVB4	4574	5827	0.12%	0.015%
9	6.934	649	654	660	rVB2	22838	32132	0.69%	0.080%
10	7.010	661	667	677	rBV	127129	232273	4.96%	0.579%
11	7.151	685	691	704	rBV	589924	940868	20.09%	2.345%
12	7.351	718	725	735	rBV	552203	894191	19.09%	2.229%
13	7.816	797	804	813	rBV	665254	1040342	22.21%	2.593%
14	7.875	813	814	819	rVB5	4448	6260	0.13%	0.016%
15	8.551	922	929	943	rBV	379013	668440	14.27%	1.666%
16	8.986	996	1003	1013	rBV	653344	1079123	23.04%	2.690%
17	9.381	1065	1070	1076	rVB	38935	56743	1.21%	0.141%
18	9.704	1118	1125	1136	rBV	463398	810101	17.29%	2.019%
19	10.251	1210	1218	1235	rBV	602358	1156345	24.69%	2.882%
20	10.469	1250	1255	1257	rBV5	4395	5525	0.12%	0.014%
21	10.616	1273	1280	1288	rBV	843895	1428535	30.50%	3.560%
22	10.769	1298	1306	1327	rBV	491893	1020730	21.79%	2.544%
23	11.875	1487	1494	1499	rVB2	19445	30302	0.65%	0.076%
24	12.227	1546	1554	1560	rBV3	9859	22656	0.48%	0.056%
25	13.074	1694	1698	1703	rVB8	3400	5231	0.11%	0.013%
26	13.433	1753	1759	1764	rBV6	4235	7478	0.16%	0.019%
27	13.880	1829	1835	1849	rBV	1273536	1790447	38.22%	4.463%
28	14.157	1871	1882	1897	rBV	1539250	2292593	48.94%	5.714%
29	14.463	1927	1934	1948	rBV	1160220	1732685	36.99%	4.319%
30	14.716	1969	1977	1992	rBV2	49465	156744	3.35%	0.391%
31	14.863	1999	2002	2004	rBV3	4754	5106	0.11%	0.013%
32	14.904	2004	2009	2015	rVB10	6983	16958	0.36%	0.042%
33	14.992	2021	2024	2026	rVB3	5363	5943	0.13%	0.015%
34	15.216	2057	2062	2064	rBV4	5901	10605	0.23%	0.026%
35	15.257	2064	2069	2072	rVV	15958	22019	0.47%	0.055%
36	15.292	2072	2075	2077	rVB3	4948	5143	0.11%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036234.D
 Acq On : 12 Aug 2022 17:32
 Operator : CG/JU
 Sample : N4095-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GBJM8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	15.451	2090	2102	2111	rBV	2056734	2903481	61.99%	7.237%
38	15.510	2111	2112	2116	rVV4	8873	9575	0.20%	0.024%
39	15.580	2118	2124	2138	rVV	538097	803580	17.16%	2.003%
40	15.692	2139	2143	2149	rVB2	20086	32362	0.69%	0.081%
41	16.168	2221	2224	2232	rVB9	5067	9768	0.21%	0.024%
42	16.239	2232	2236	2240	rVB6	5819	8873	0.19%	0.022%
43	16.515	2279	2283	2288	rBV8	4586	9325	0.20%	0.023%
44	16.668	2304	2309	2314	rBV5	10417	15989	0.34%	0.040%
45	16.962	2355	2359	2362	rBV5	7851	12486	0.27%	0.031%
46	17.204	2394	2400	2410	rBV	1431116	1924537	41.09%	4.797%
47	17.304	2410	2417	2427	rBV	2345392	3331301	71.12%	8.303%
48	17.739	2487	2491	2497	rVB4	8513	12967	0.28%	0.032%
49	17.815	2501	2504	2510	rVV6	7342	10936	0.23%	0.027%
50	18.104	2549	2553	2560	rBV3	26563	43016	0.92%	0.107%
51	18.180	2562	2566	2573	rVB	13445	24678	0.53%	0.062%
52	19.162	2729	2733	2739	rBV2	31148	45949	0.98%	0.115%
53	19.233	2741	2745	2749	rBV	29258	40057	0.86%	0.100%
54	19.592	2801	2806	2823	rBV	2903871	3980949	84.99%	9.922%
55	20.598	2974	2977	2981	rVB	95518	99636	2.13%	0.248%
56	21.386	3106	3111	3117	rBV	1702409	2288031	48.85%	5.703%
57	23.574	3476	3483	3494	rVB	2493366	4684121	100.00%	11.675%
58	23.721	3502	3508	3519	rVB2	1314977	2510835	53.60%	6.258%




Sum of corrected areas: 40121755

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036234.D
Acq On : 12 Aug 2022 17:32
Operator : CG/JU
Sample : N4095-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBJM8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

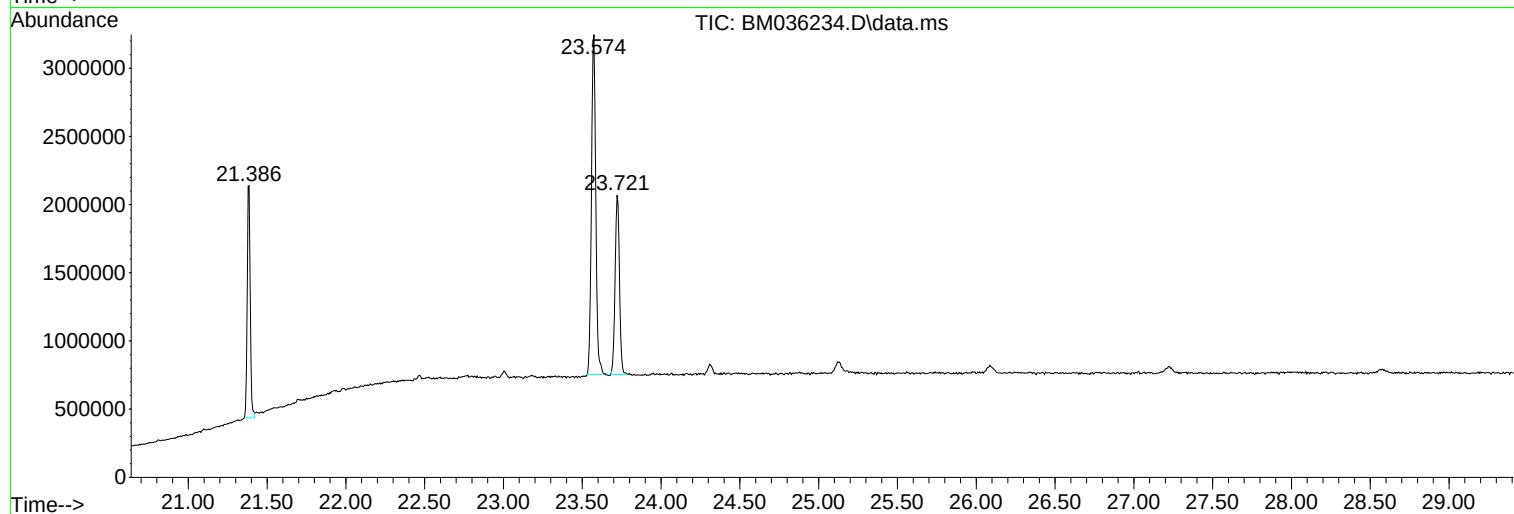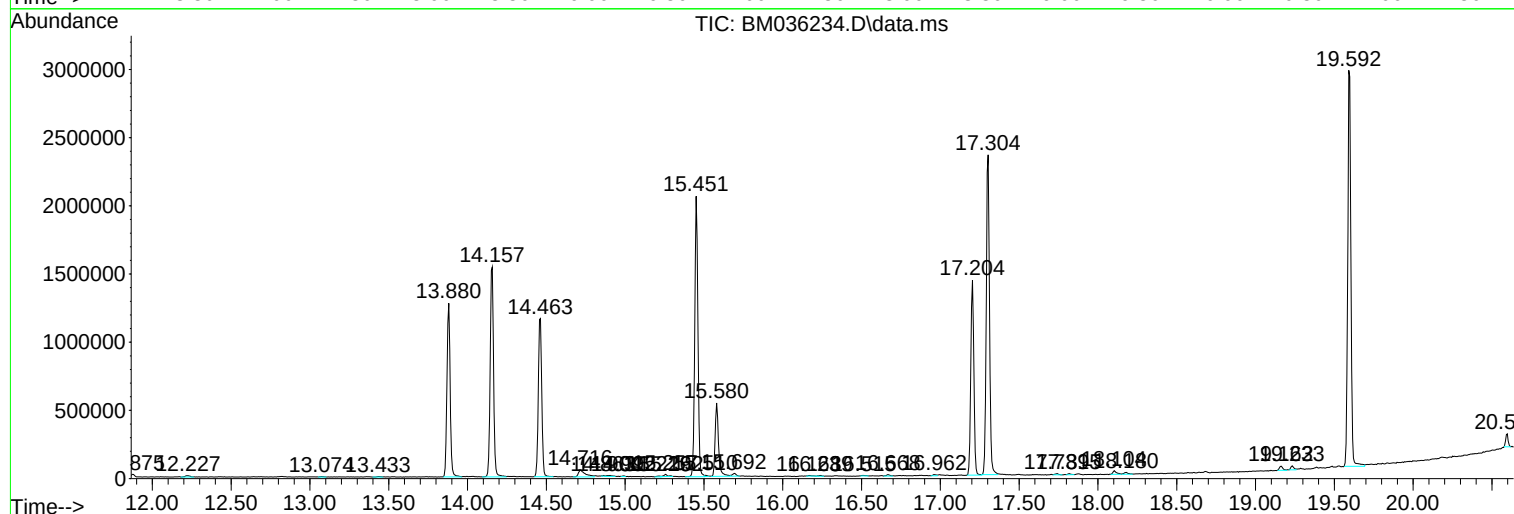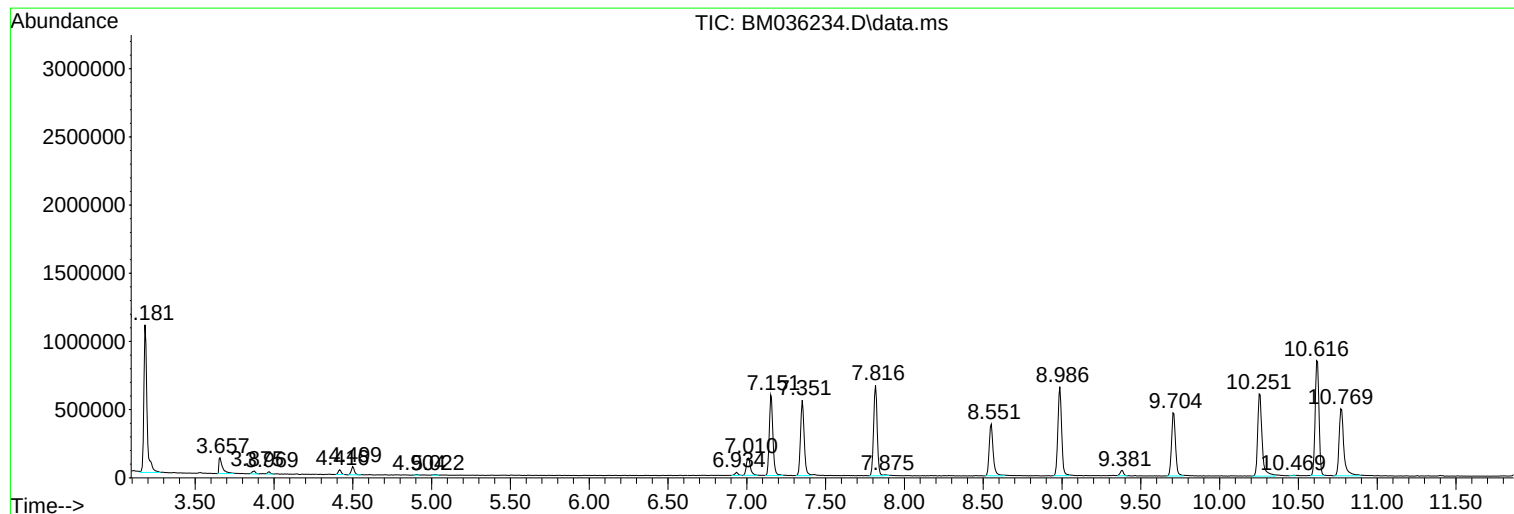

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036234.D
Acq On : 12 Aug 2022 17:32
Operator : CG/JU
Sample : N4095-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBJM8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036234.D
Acq On : 12 Aug 2022 17:32
Operator : CG/JU
Sample : N4095-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBJM8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc