

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036238.D
 Acq On : 12 Aug 2022 19:59
 Operator : CG/JU
 Sample : N4069-18
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GBJM2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036238.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	19	22	27	rVB	45364	55591	1.08%	0.132%
2	3.652	94	96	112	rBV	203604	322293	6.26%	0.767%
3	3.869	129	133	139	rBV	20299	33169	0.64%	0.079%
4	3.969	147	150	154	rVB	15557	18085	0.35%	0.043%
5	4.416	222	226	230	rVB	31780	38870	0.76%	0.093%
6	5.028	324	330	335	rVB9	6434	12822	0.25%	0.031%
7	6.934	649	654	659	rBV	19137	28947	0.56%	0.069%
8	7.004	659	666	678	rVV	147894	260622	5.06%	0.620%
9	7.151	685	691	701	rBV	661639	1029360	20.00%	2.450%
10	7.351	718	725	735	rBV	634103	999316	19.41%	2.378%
11	7.422	735	737	743	rVB7	7728	12392	0.24%	0.029%
12	7.816	797	804	813	rBV	658137	1023927	19.89%	2.437%
13	7.887	813	816	823	rVB4	14096	22655	0.44%	0.054%
14	8.551	920	929	940	rBV	419557	739324	14.36%	1.760%
15	8.987	995	1003	1014	rBV	740296	1211821	23.54%	2.884%
16	9.128	1023	1027	1034	rBV6	5597	9112	0.18%	0.022%
17	9.381	1064	1070	1077	rVB	29800	49463	0.96%	0.118%
18	9.704	1115	1125	1137	rBV	549017	929865	18.06%	2.213%
19	10.251	1210	1218	1236	rBV	738945	1350033	26.23%	3.213%
20	10.616	1273	1280	1288	rBV	866439	1434777	27.87%	3.415%
21	10.769	1299	1306	1329	rBV	524815	1093689	21.25%	2.603%
22	11.451	1417	1422	1429	rBV7	7047	15089	0.29%	0.036%
23	11.875	1490	1494	1499	rVB	18992	26773	0.52%	0.064%
24	12.216	1547	1552	1559	rVV3	12030	22087	0.43%	0.053%
25	12.822	1650	1655	1659	rVB6	6480	9681	0.19%	0.023%
26	13.075	1694	1698	1701	rVV4	4723	7449	0.14%	0.018%
27	13.204	1715	1720	1722	rBV5	2731	5696	0.11%	0.014%
28	13.363	1743	1747	1754	rVB7	8044	12831	0.25%	0.031%
29	13.439	1754	1760	1762	rBV7	4224	6781	0.13%	0.016%
30	13.880	1828	1835	1848	rBV	1470101	2020641	39.26%	4.809%
31	14.004	1851	1856	1863	rVV2	14967	27936	0.54%	0.066%
32	14.151	1870	1881	1896	rBV	1714129	2531176	49.17%	6.024%
33	14.351	1911	1915	1924	rVB2	17465	32044	0.62%	0.076%
34	14.457	1927	1933	1945	rBV	1187772	1734574	33.70%	4.128%
35	14.710	1969	1976	1991	rBV2	63564	175295	3.41%	0.417%
36	14.851	1996	2000	2004	rVV4	14978	30656	0.60%	0.073%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036238.D
 Acq On : 12 Aug 2022 19:59
 Operator : CG/JU
 Sample : N4069-18
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GBJM2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	14.892	2004	2007	2017	rVV9	11219	28451	0.55%	0.068%
38	14.986	2019	2023	2029	rVB	14565	22080	0.43%	0.053%
39	15.257	2064	2069	2071	rBV	10133	13270	0.26%	0.032%
40	15.292	2071	2075	2080	rVB3	8314	14243	0.28%	0.034%
41	15.451	2093	2102	2116	rBV	2221055	3207368	62.31%	7.634%
42	15.580	2118	2124	2135	rVV	644837	936770	18.20%	2.230%
43	15.692	2139	2143	2148	rVB2	22997	37503	0.73%	0.089%
44	16.110	2210	2214	2215	rBV4	6071	6584	0.13%	0.016%
45	16.168	2221	2224	2226	rBV3	6858	7675	0.15%	0.018%
46	16.233	2232	2235	2240	rVB7	7878	11333	0.22%	0.027%
47	16.345	2247	2254	2257	rBV8	5286	11569	0.22%	0.028%
48	16.504	2279	2281	2288	rBV8	3826	7413	0.14%	0.018%
49	16.627	2298	2302	2305	rVB6	5629	9357	0.18%	0.022%
50	16.668	2305	2309	2315	rBV4	14344	25843	0.50%	0.062%
51	16.804	2324	2332	2334	rBV9	4196	9031	0.18%	0.021%
52	16.957	2355	2358	2362	rBV5	10189	14475	0.28%	0.034%
53	17.204	2394	2400	2408	rBV	1376488	1889327	36.70%	4.497%
54	17.304	2410	2417	2428	rVV	2609673	3751504	72.88%	8.929%
55	17.492	2447	2449	2454	rVB2	10947	12972	0.25%	0.031%
56	18.104	2548	2553	2559	rBV4	34566	61262	1.19%	0.146%
57	18.174	2561	2565	2570	rVB	30661	43072	0.84%	0.103%
58	19.156	2729	2732	2740	rBV2	35175	47834	0.93%	0.114%
59	19.233	2741	2745	2752	rBV2	32458	61229	1.19%	0.146%
60	19.592	2801	2806	2813	rBV	3306208	4440235	86.26%	10.568%
61	20.592	2973	2976	2980	rBV	95626	108113	2.10%	0.257%
62	21.098	3059	3062	3066	rBV4	79060	101767	1.98%	0.242%
63	21.380	3106	3110	3120	rBV	1764796	2239175	43.50%	5.329%
64	23.574	3476	3483	3498	rVB2	2608881	5147438	100.00%	12.251%
65	23.721	3502	3508	3519	rVB2	1243089	2413656	46.89%	5.745%




Sum of corrected areas: 42015391

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036238.D
Acq On : 12 Aug 2022 19:59
Operator : CG/JU
Sample : N4069-18
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBJM2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

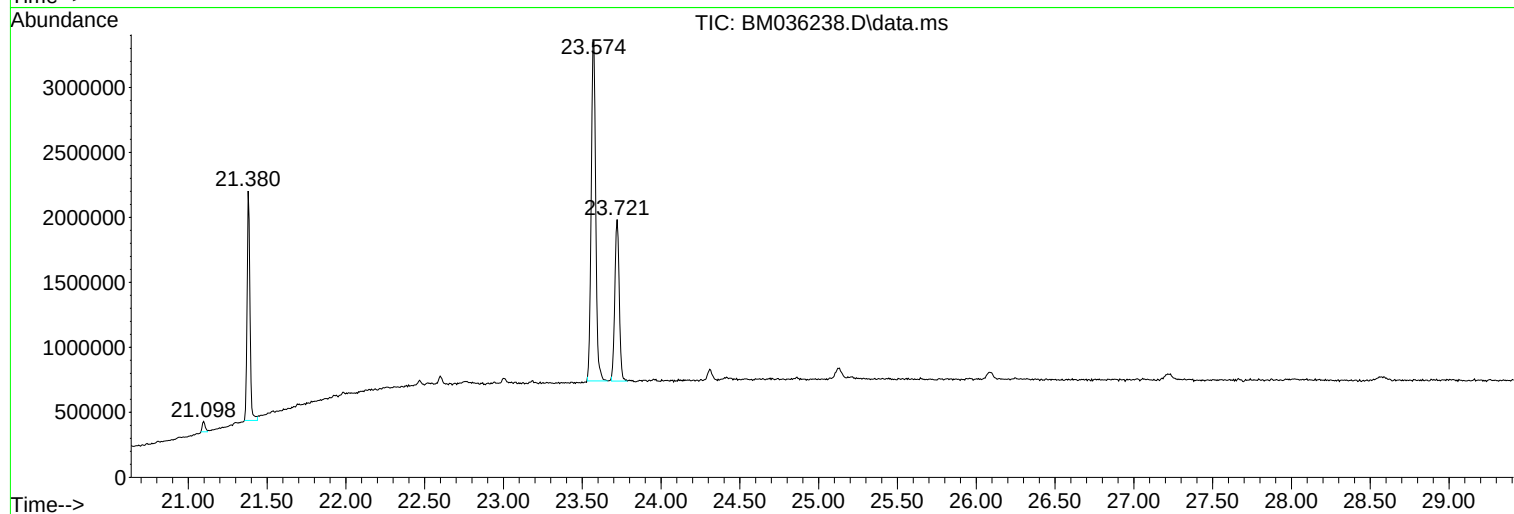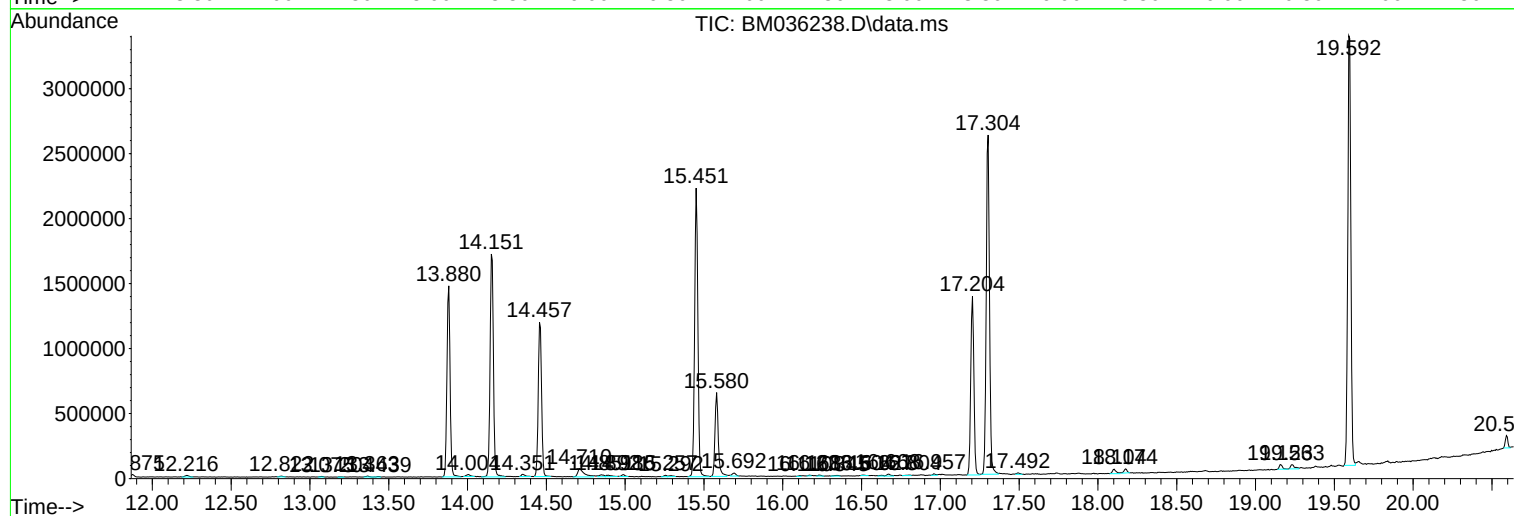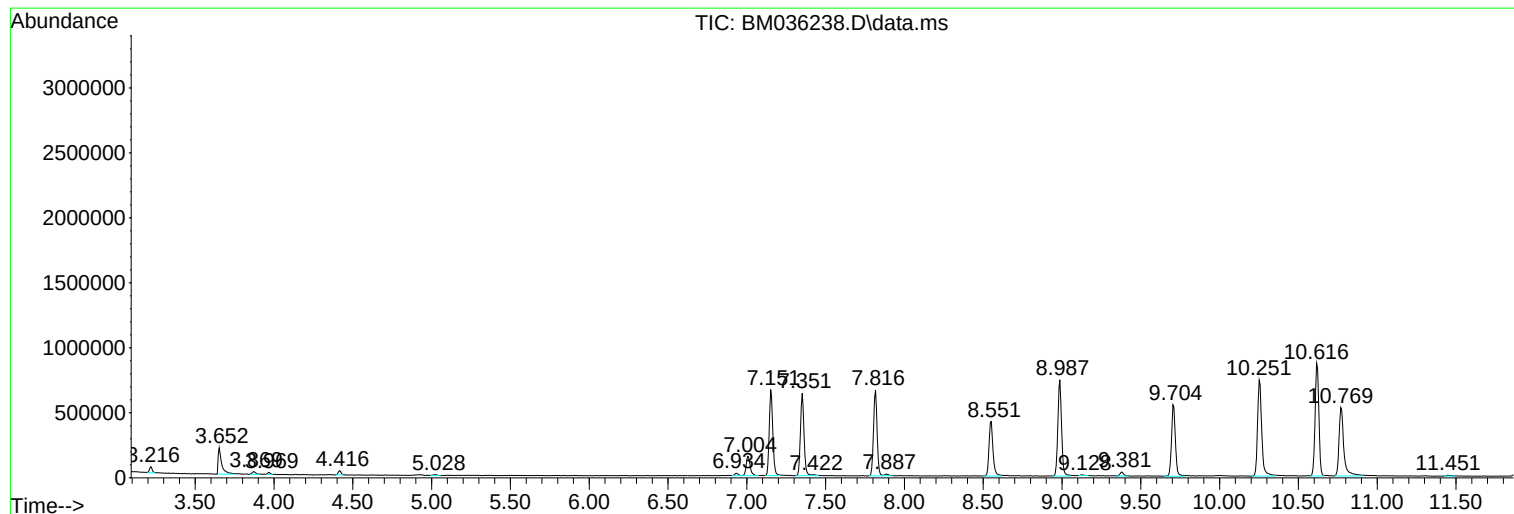

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036238.D
Acq On : 12 Aug 2022 19:59
Operator : CG/JU
Sample : N4069-18
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBJM2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036238.D
Acq On : 12 Aug 2022 19:59
Operator : CG/JU
Sample : N4069-18
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBJM2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
