

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036239.D
 Acq On : 12 Aug 2022 20:35
 Operator : CG/JU
 Sample : N4069-16
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GBJM0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036239.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	13	16	19	rBV	37565	43862	0.80%	0.108%
2	3.216	19	22	28	rVB	44592	50166	0.91%	0.124%
3	3.522	72	74	78	rBV	8119	10273	0.19%	0.025%
4	3.651	94	96	110	rBV	111309	182446	3.31%	0.451%
5	3.869	129	133	140	rBV2	19226	32119	0.58%	0.079%
6	3.963	146	149	155	rVB	14558	17446	0.32%	0.043%
7	4.416	221	226	238	rVB	32711	46747	0.85%	0.116%
8	4.910	305	310	316	rBV10	3671	7082	0.13%	0.018%
9	6.934	650	654	658	rVB	15741	22494	0.41%	0.056%
10	7.004	660	666	678	rVB	143697	254324	4.61%	0.629%
11	7.151	685	691	703	rBV	570604	917833	16.65%	2.269%
12	7.245	703	707	713	rVB	5456	10182	0.18%	0.025%
13	7.351	718	725	735	rBV	557713	899748	16.32%	2.224%
14	7.428	735	738	742	rVB6	4978	7217	0.13%	0.018%
15	7.816	796	804	812	rBV	581150	932793	16.92%	2.306%
16	7.892	812	817	824	rVB3	12728	25651	0.47%	0.063%
17	8.545	921	928	941	rBV	397454	698744	12.67%	1.727%
18	8.986	993	1003	1017	rBV	644378	1080869	19.60%	2.672%
19	9.380	1064	1070	1074	rBV	18526	31625	0.57%	0.078%
20	9.704	1118	1125	1135	rBV	466795	799754	14.51%	1.977%
21	10.251	1211	1218	1239	rBV	641786	1196292	21.70%	2.958%
22	10.616	1272	1280	1287	rBV	776786	1292229	23.44%	3.195%
23	10.675	1287	1290	1297	rVB3	15827	26788	0.49%	0.066%
24	10.775	1299	1307	1321	rBV	326414	749407	13.59%	1.853%
25	11.874	1490	1494	1499	rVB3	11755	16935	0.31%	0.042%
26	12.210	1547	1551	1558	rBV3	11100	19015	0.34%	0.047%
27	12.816	1651	1654	1660	rVB5	7488	11482	0.21%	0.028%
28	13.074	1693	1698	1703	rBV5	8708	14229	0.26%	0.035%
29	13.433	1754	1759	1762	rBV7	4059	7097	0.13%	0.018%
30	13.880	1828	1835	1849	rBV	1293850	1863824	33.80%	4.608%
31	14.151	1873	1881	1896	rBV	1575595	2315533	42.00%	5.725%
32	14.457	1926	1933	1947	rBV	1068453	1570632	28.49%	3.883%
33	14.627	1957	1962	1964	rBV5	3817	5606	0.10%	0.014%
34	14.710	1969	1976	1989	rBV2	67980	185074	3.36%	0.458%
35	14.845	1993	1999	2004	rBV2	19553	37818	0.69%	0.093%
36	15.251	2062	2068	2072	rBV	16140	28937	0.52%	0.072%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036239.D
 Acq On : 12 Aug 2022 20:35
 Operator : CG/JU
 Sample : N4069-16
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GBJM0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	15.292	2072	2075	2081	rVB4	7847	12672	0.23%	0.031%
38	15.451	2093	2102	2118	rBV	2210953	2990842	54.24%	7.394%
39	15.580	2118	2124	2139	rBV	618132	899134	16.31%	2.223%
40	15.692	2139	2143	2147	rVB2	20563	30517	0.55%	0.075%
41	16.015	2194	2198	2203	rVB8	2973	5516	0.10%	0.014%
42	16.168	2221	2224	2225	rBV3	7225	8636	0.16%	0.021%
43	16.233	2231	2235	2239	rBV6	5657	8271	0.15%	0.020%
44	16.345	2250	2254	2259	rVB7	5002	9440	0.17%	0.023%
45	16.509	2279	2282	2285	rBV4	4832	6966	0.13%	0.017%
46	16.621	2298	2301	2305	rBV6	4410	6561	0.12%	0.016%
47	16.668	2305	2309	2317	rVV5	15688	23414	0.42%	0.058%
48	16.798	2327	2331	2332	rBV3	4823	6125	0.11%	0.015%
49	16.956	2354	2358	2362	rBV6	10338	18251	0.33%	0.045%
50	17.127	2383	2387	2392	rVB7	7345	9968	0.18%	0.025%
51	17.204	2394	2400	2408	rBV	1308920	1836408	33.31%	4.540%
52	17.298	2410	2416	2429	rVV	2441175	3577549	64.89%	8.845%
53	17.498	2446	2450	2455	rVB4	7263	12335	0.22%	0.030%
54	17.739	2489	2491	2496	rVB5	10514	13598	0.25%	0.034%
55	17.815	2501	2504	2507	rVV4	13726	17947	0.33%	0.044%
56	17.874	2511	2514	2519	rVB	23423	26915	0.49%	0.067%
57	18.098	2547	2552	2561	rBV2	52943	89857	1.63%	0.222%
58	18.174	2562	2565	2570	rVB	17342	27015	0.49%	0.067%
59	18.645	2643	2645	2647	rBV3	5647	5719	0.10%	0.014%
60	19.162	2729	2733	2739	rBV3	30650	42500	0.77%	0.105%
61	19.233	2741	2745	2748	rBV	33156	43996	0.80%	0.109%
62	19.380	2768	2770	2774	rVB4	13029	11707	0.21%	0.029%
63	19.592	2801	2806	2813	rBV	3454821	4566846	82.83%	11.290%
64	20.592	2973	2976	2980	rBV	136449	135361	2.46%	0.335%
65	21.097	3059	3062	3066	rVB2	125295	146327	2.65%	0.362%
66	21.380	3106	3110	3116	rBV	1921534	2328173	42.23%	5.756%
67	23.568	3475	3482	3496	rBV2	2770539	5513619	100.00%	13.631%
68	23.721	3502	3508	3516	rVB2	1351127	2604954	47.25%	6.440%




Sum of corrected areas: 40449412

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036239.D
Acq On : 12 Aug 2022 20:35
Operator : CG/JU
Sample : N4069-16
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBJM0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

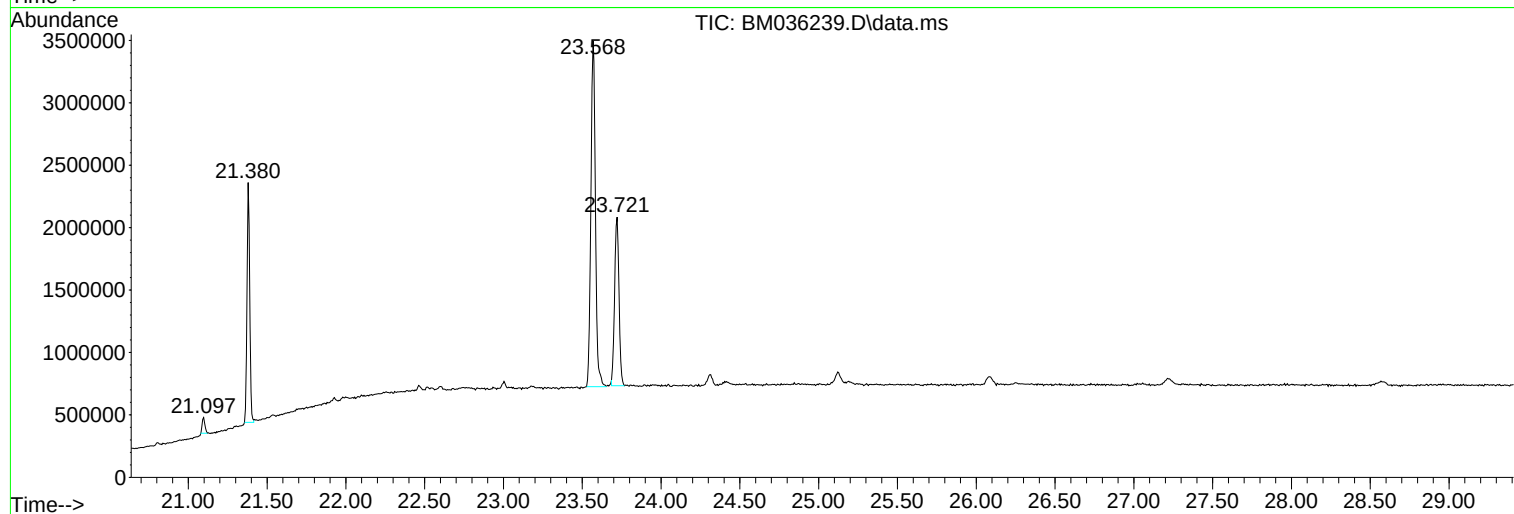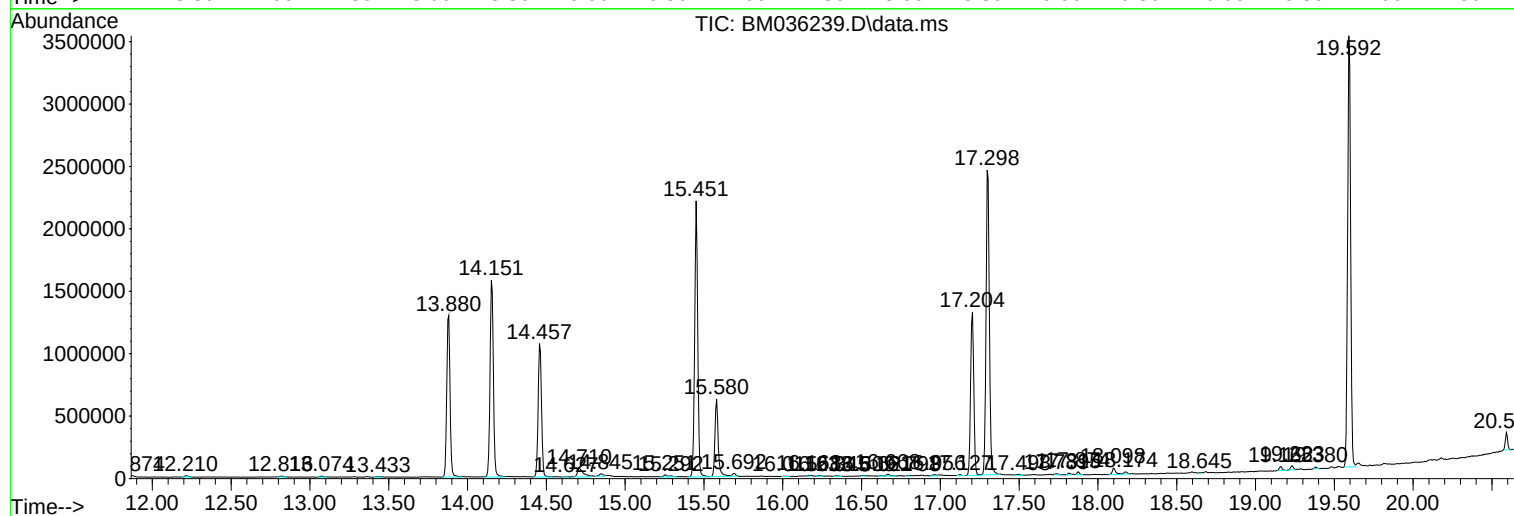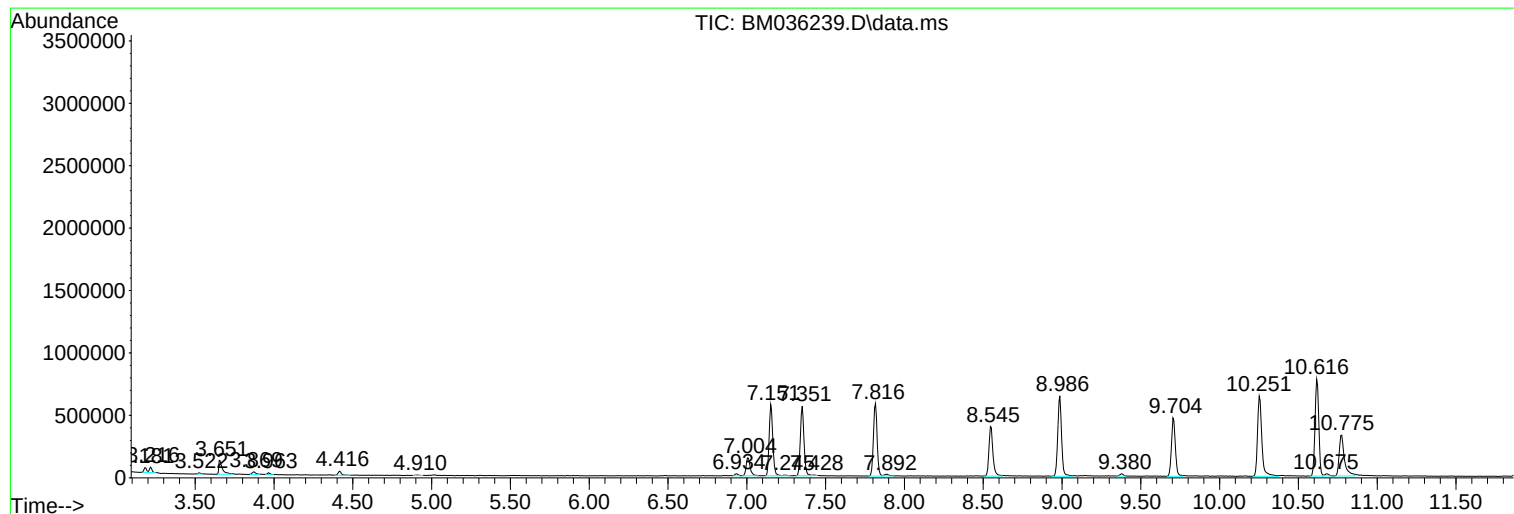

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036239.D
Acq On : 12 Aug 2022 20:35
Operator : CG/JU
Sample : N4069-16
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBJM0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036239.D
Acq On : 12 Aug 2022 20:35
Operator : CG/JU
Sample : N4069-16
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBJM0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc