

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036241.D
 Acq On : 12 Aug 2022 22:24
 Operator : CG/JU
 Sample : PB146838BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK838

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036241.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	18	22	28	rVB	76735	87526	1.76%	0.177%
2	3.640	92	94	116	rBV	815063	1219589	24.51%	2.469%
3	3.963	146	149	153	rVB	17077	21550	0.43%	0.044%
4	7.004	659	666	677	rBV	888030	1438096	28.91%	2.911%
5	7.151	685	691	703	rVB	743951	1168611	23.49%	2.366%
6	7.351	718	725	739	rBV	936970	1500019	30.15%	3.036%
7	7.816	797	804	813	rBV	754030	1196592	24.05%	2.422%
8	8.440	905	910	914	rVB6	2743	5106	0.10%	0.010%
9	8.545	920	928	946	rBV	1031737	1749683	35.17%	3.542%
10	8.987	995	1003	1017	rBV	802195	1353473	27.20%	2.740%
11	9.704	1118	1125	1137	rBV	655325	1092349	21.96%	2.211%
12	10.251	1211	1218	1233	rBV	926496	1621222	32.59%	3.282%
13	10.616	1272	1280	1289	rBV	1042052	1695145	34.07%	3.431%
14	10.769	1296	1306	1322	rBV	954083	1741741	35.01%	3.526%
15	12.222	1548	1553	1563	rVB2	13828	30344	0.61%	0.061%
16	13.880	1828	1835	1847	rBV	1472365	2165023	43.52%	4.383%
17	14.151	1874	1881	1898	rVV	1966170	2802027	56.32%	5.672%
18	14.457	1926	1933	1944	rBV	1430654	2052136	41.25%	4.154%
19	14.692	1967	1973	1994	rBV	492191	1041465	20.93%	2.108%
20	15.286	2071	2074	2078	rBV3	5356	7928	0.16%	0.016%
21	15.451	2095	2102	2118	rBV	2465215	3401604	68.37%	6.886%
22	15.580	2118	2124	2138	rBV	572367	924315	18.58%	1.871%
23	15.692	2138	2143	2151	rVB2	25589	46527	0.94%	0.094%
24	16.169	2221	2224	2227	rBV5	3095	5064	0.10%	0.010%
25	16.227	2231	2234	2239	rVB6	7246	12109	0.24%	0.025%
26	16.339	2249	2253	2258	rVB7	3072	5118	0.10%	0.010%
27	16.504	2277	2281	2283	rBV5	3652	5675	0.11%	0.011%
28	16.668	2307	2309	2312	rVB3	5376	5586	0.11%	0.011%
29	16.963	2355	2359	2360	rBV4	5797	6772	0.14%	0.014%
30	17.198	2393	2399	2409	rVV	1596975	2277352	45.77%	4.610%
31	17.298	2410	2416	2436	rVB	2502274	3629939	72.96%	7.348%
32	17.739	2487	2491	2496	rVB8	4013	8248	0.17%	0.017%
33	18.110	2551	2554	2561	rVB9	7223	11414	0.23%	0.023%
34	18.186	2563	2567	2569	rBV5	4730	6520	0.13%	0.013%
35	19.157	2728	2732	2739	rBV2	30740	51665	1.04%	0.105%
36	19.233	2741	2745	2750	rVB	26290	39214	0.79%	0.079%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036241.D
Acq On : 12 Aug 2022 22:24
Operator : CG/JU
Sample : PB146838BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK838

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Title : SVOA CALIBRATION

37	19.592	2800	2806	2814	rBV	3217766	4280458	86.04%	8.665%
38	20.592	2973	2976	2980	rBV	79865	89319	1.80%	0.181%
39	21.380	3105	3110	3119	rBV	2062012	2726471	54.80%	5.519%
40	23.568	3475	3482	3495	rVB2	2560605	4975136	100.00%	10.071%
41	23.715	3501	3507	3516	rVB2	1530154	2903037	58.35%	5.876%




Sum of corrected areas: 49401168

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036241.D
Acq On : 12 Aug 2022 22:24
Operator : CG/JU
Sample : PB146838BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK838

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

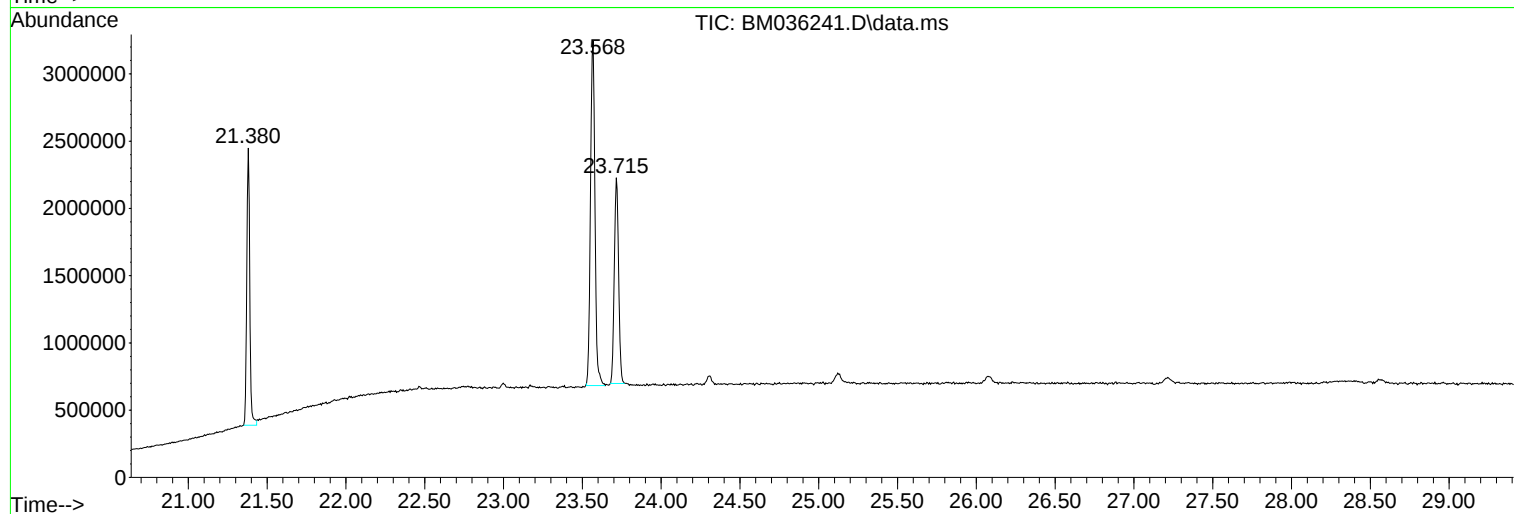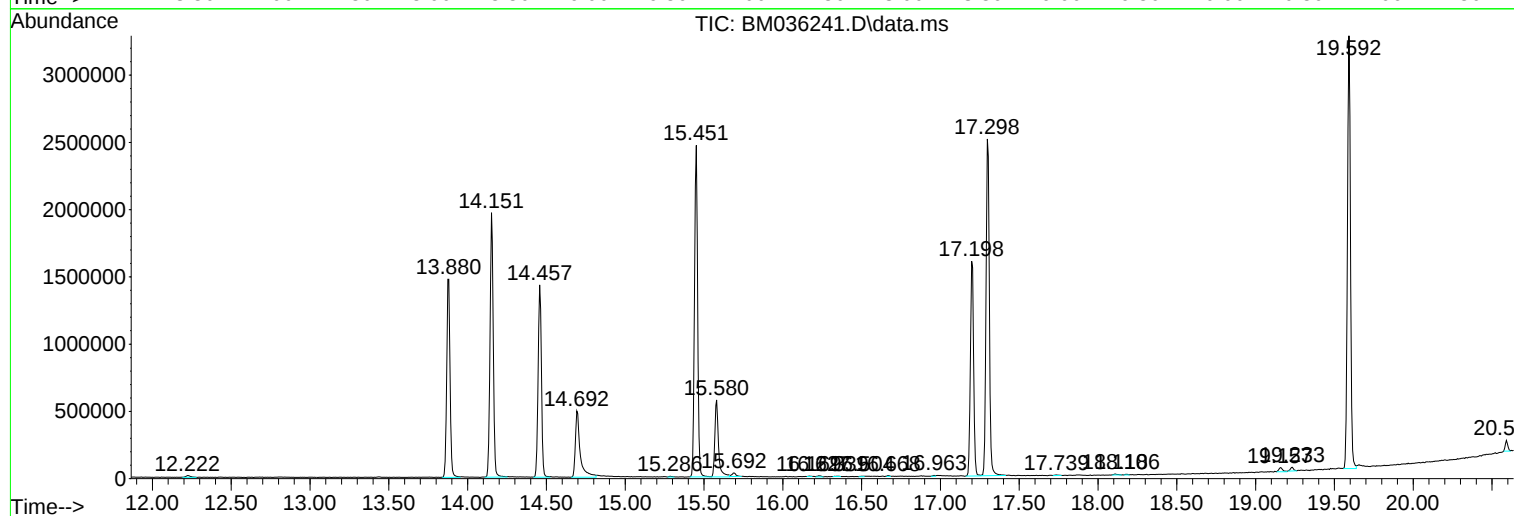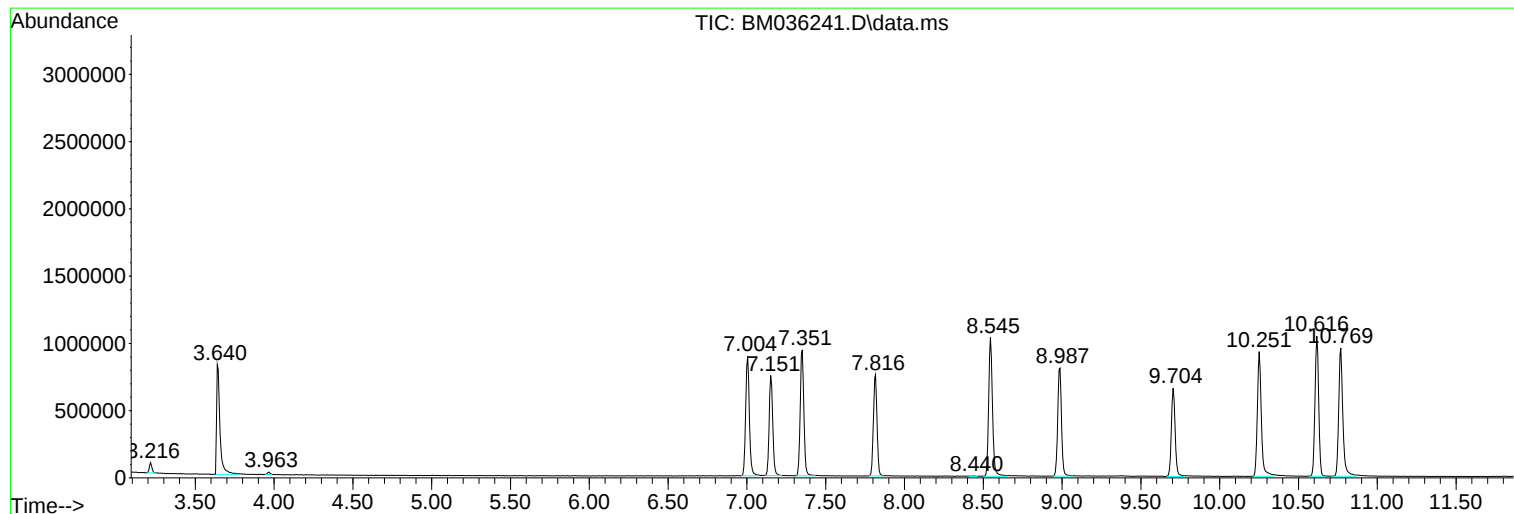

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036241.D
Acq On : 12 Aug 2022 22:24
Operator : CG/JU
Sample : PB146838BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK838

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036241.D
Acq On : 12 Aug 2022 22:24
Operator : CG/JU
Sample : PB146838BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK838

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------