

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036242.D
 Acq On : 12 Aug 2022 23:00
 Operator : CG/JU
 Sample : PB146854BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK854

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036242.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	19	22	34	rVB	72905	102400	1.85%	0.209%
2	3.646	92	95	121	rBV	748846	1140808	20.57%	2.323%
3	3.963	146	149	153	rVB	13802	16949	0.31%	0.035%
4	7.004	659	666	678	rBV	850708	1352275	24.39%	2.754%
5	7.151	685	691	704	rVV	707280	1107421	19.97%	2.255%
6	7.351	718	725	734	rBV	861431	1389783	25.07%	2.830%
7	7.816	797	804	817	rBV	653695	1060526	19.13%	2.160%
8	8.545	921	928	941	rBV	983033	1627534	29.35%	3.314%
9	8.986	993	1003	1016	rBV	763962	1286004	23.19%	2.619%
10	9.704	1117	1125	1137	rBV	615688	1022625	18.44%	2.082%
11	10.251	1211	1218	1236	rBV	834286	1525134	27.51%	3.106%
12	10.616	1272	1280	1290	rBV	916108	1502207	27.09%	3.059%
13	10.769	1298	1306	1330	rBV	868772	1648735	29.74%	3.357%
14	12.221	1547	1553	1558	rBV2	13469	27680	0.50%	0.056%
15	13.880	1828	1835	1845	rBV	1473965	2141316	38.62%	4.360%
16	14.151	1874	1881	1896	rBV	1897768	2720680	49.07%	5.540%
17	14.280	1901	1903	1908	rVV6	3434	5710	0.10%	0.012%
18	14.457	1925	1933	1946	rBV	1305131	1864547	33.63%	3.797%
19	14.692	1967	1973	1989	rBV	532029	1065333	19.21%	2.169%
20	15.280	2071	2073	2083	rVB6	4930	9105	0.16%	0.019%
21	15.451	2095	2102	2112	rBV	2377506	3363662	60.66%	6.849%
22	15.580	2118	2124	2138	rBV	620250	962020	17.35%	1.959%
23	15.692	2138	2143	2153	rVB	25962	50747	0.92%	0.103%
24	16.227	2230	2234	2240	rVB8	7512	12527	0.23%	0.026%
25	16.339	2248	2253	2257	rBV8	3830	6434	0.12%	0.013%
26	16.509	2277	2282	2285	rBV7	4402	8617	0.16%	0.018%
27	16.668	2306	2309	2315	rBV6	4354	6642	0.12%	0.014%
28	16.956	2355	2358	2361	rBV5	6694	10849	0.20%	0.022%
29	17.198	2393	2399	2410	rBV	1555866	2202493	39.72%	4.485%
30	17.298	2410	2416	2428	rVV	2647144	3702126	66.77%	7.539%
31	18.103	2549	2553	2556	rBV5	9470	16365	0.30%	0.033%
32	19.162	2729	2733	2740	rVB4	29158	41551	0.75%	0.085%
33	19.233	2741	2745	2749	rBV2	26278	37180	0.67%	0.076%
34	19.592	2800	2806	2815	rBV	3557796	4567162	82.37%	9.300%
35	20.591	2973	2976	2982	rBV2	85008	99750	1.80%	0.203%
36	21.380	3105	3110	3118	rBV	2148151	2781103	50.16%	5.663%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036242.D
Acq On : 12 Aug 2022 23:00
Operator : CG/JU
Sample : PB146854BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK854

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Title : SVOA CALIBRATION

37	23.568	3475	3482	3493	rBV2	2959134	5544676	100.00%	11.291%
38	23.721	3501	3508	3517	rVB2	1523175	3078089	55.51%	6.268%




Sum of corrected areas: 49108765

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036242.D
Acq On : 12 Aug 2022 23:00
Operator : CG/JU
Sample : PB146854BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK854

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

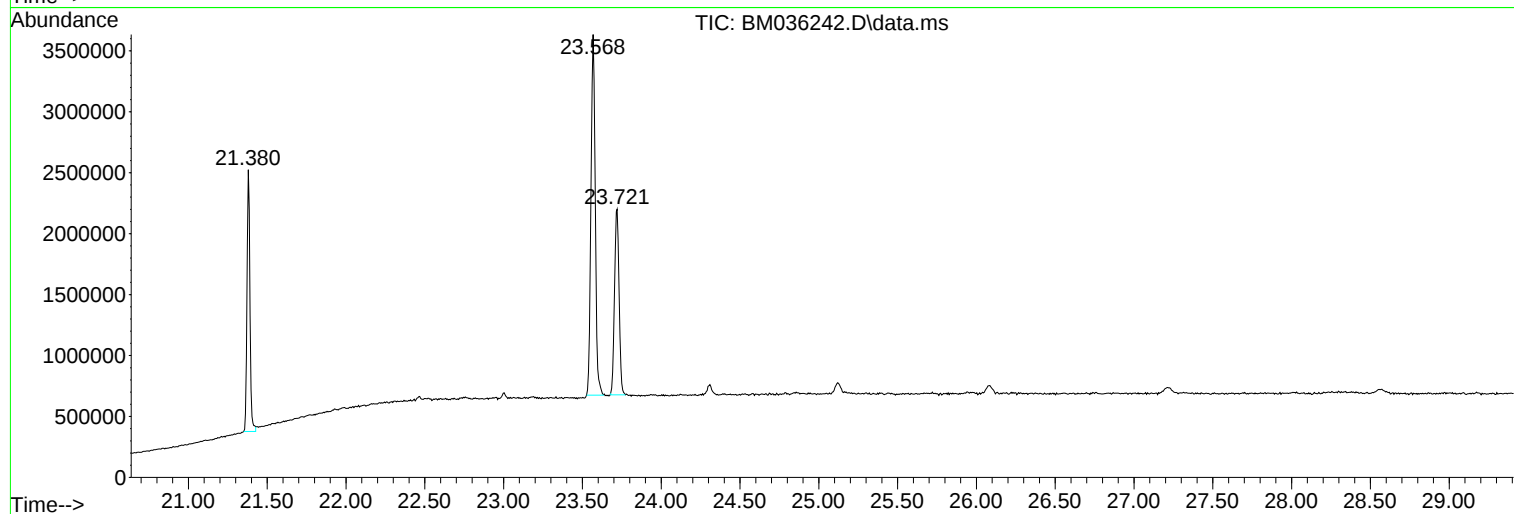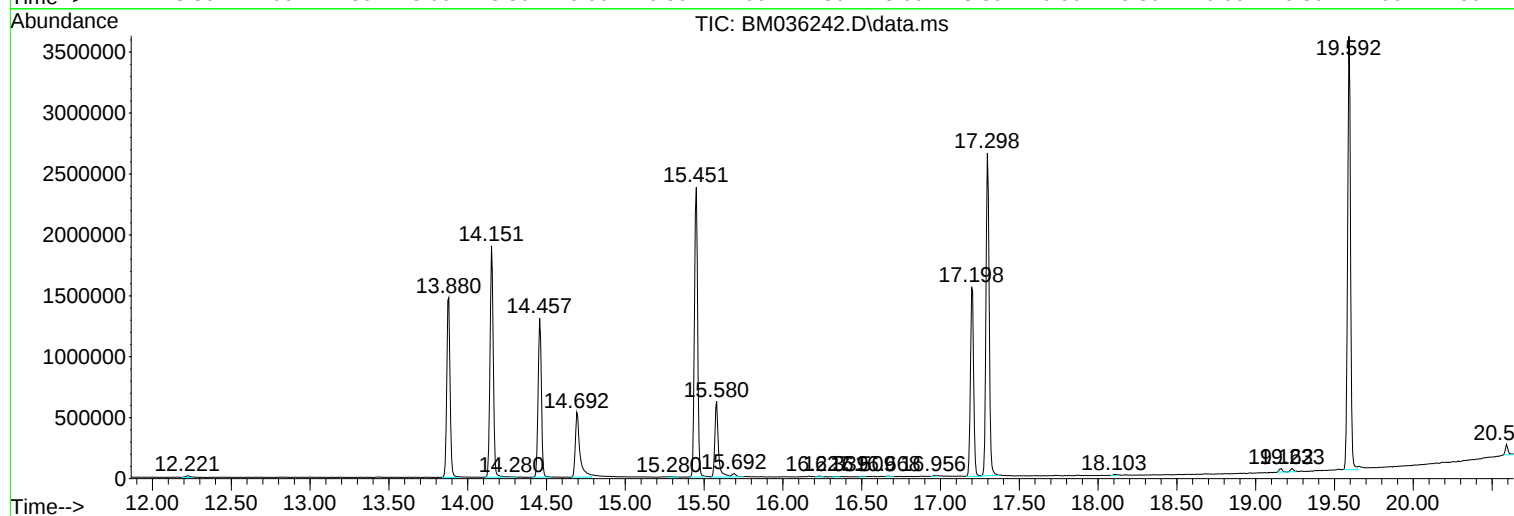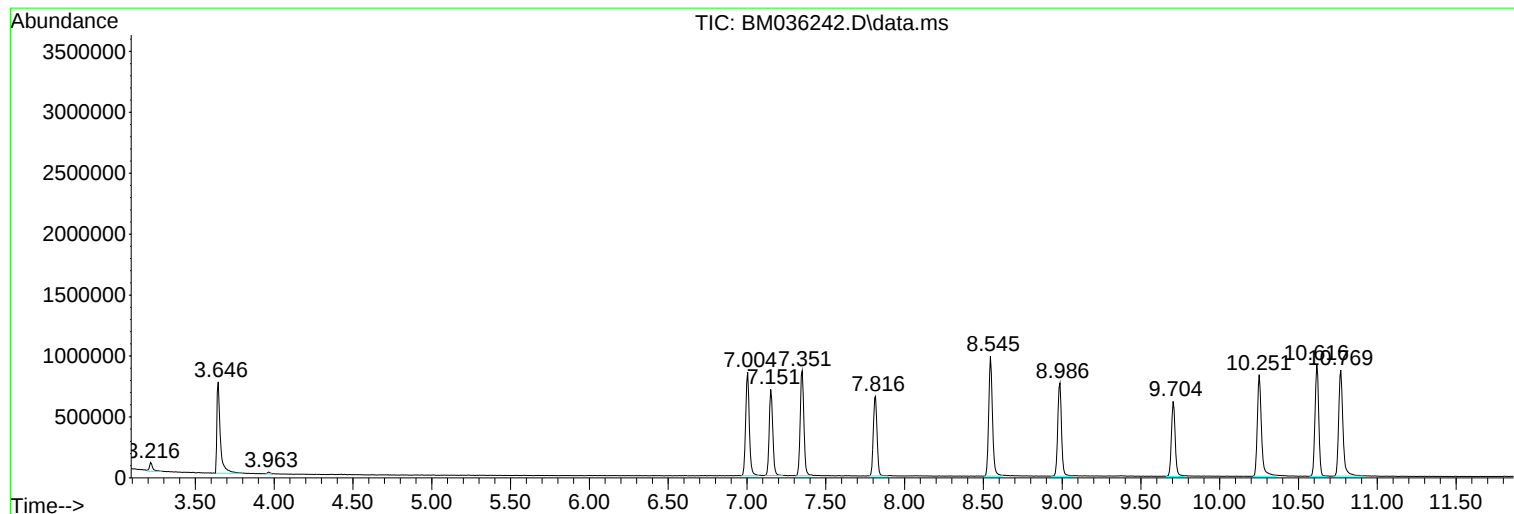

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036242.D
Acq On : 12 Aug 2022 23:00
Operator : CG/JU
Sample : PB146854BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK854

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036242.D
Acq On : 12 Aug 2022 23:00
Operator : CG/JU
Sample : PB146854BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK854

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc