

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036243.D
 Acq On : 12 Aug 2022 23:36
 Operator : CG/JU
 Sample : N4165-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGBX8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036243.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	19	22	28	rVB	50866	59494	1.11%	0.134%
2	3.646	92	95	116	rBV	227812	387166	7.24%	0.869%
3	3.869	129	133	140	rVB	23246	35928	0.67%	0.081%
4	3.963	146	149	154	rVB	16385	23235	0.43%	0.052%
5	4.416	221	226	232	rVB	41153	58806	1.10%	0.132%
6	5.022	326	329	336	rBV7	5979	10159	0.19%	0.023%
7	6.463	570	574	580	rBV7	8229	13920	0.26%	0.031%
8	6.934	650	654	658	rBV	19692	26339	0.49%	0.059%
9	7.004	660	666	674	rBV	132429	232393	4.35%	0.521%
10	7.151	684	691	705	rBV	654555	1028634	19.24%	2.308%
11	7.351	718	725	734	rBV	569163	937856	17.54%	2.105%
12	7.422	735	737	741	rVB4	5976	8469	0.16%	0.019%
13	7.551	754	759	767	rVB8	8382	13590	0.25%	0.030%
14	7.810	796	803	811	rBV	739855	1196791	22.39%	2.686%
15	8.545	920	928	945	rBV	398899	704026	13.17%	1.580%
16	8.981	995	1002	1014	rBV	676605	1162169	21.74%	2.608%
17	9.375	1065	1069	1074	rVB	18694	28388	0.53%	0.064%
18	9.704	1118	1125	1135	rBV	515535	870931	16.29%	1.954%
19	10.251	1210	1218	1234	rBV	679653	1250198	23.38%	2.805%
20	10.616	1272	1280	1290	rBV	998749	1660706	31.06%	3.727%
21	10.769	1297	1306	1327	rBV	691658	1340599	25.08%	3.008%
22	11.874	1489	1494	1499	rVB2	12063	18934	0.35%	0.042%
23	12.221	1547	1553	1559	rBV2	11341	22553	0.42%	0.051%
24	12.810	1648	1653	1665	rBV6	6647	16182	0.30%	0.036%
25	13.074	1693	1698	1703	rVB5	5247	9559	0.18%	0.021%
26	13.363	1743	1747	1752	rVB7	4430	7807	0.15%	0.018%
27	13.433	1755	1759	1767	rVB7	2999	6780	0.13%	0.015%
28	13.874	1827	1834	1850	rBV	1407197	1966656	36.79%	4.413%
29	14.151	1873	1881	1894	rBV	1726306	2498419	46.73%	5.606%
30	14.457	1925	1933	1944	rBV	1430025	2032790	38.02%	4.562%
31	14.680	1966	1971	1975	rBV	150683	244704	4.58%	0.549%
32	15.251	2064	2068	2071	rBV6	4901	6410	0.12%	0.014%
33	15.286	2071	2074	2080	rVB2	8275	11130	0.21%	0.025%
34	15.451	2093	2102	2113	rBV	2250109	3206766	59.98%	7.196%
35	15.580	2118	2124	2140	rVV	531974	852948	15.95%	1.914%
36	15.692	2140	2143	2150	rVB5	13660	24077	0.45%	0.054%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036243.D
 Acq On : 12 Aug 2022 23:36
 Operator : CG/JU
 Sample : N4165-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGBX8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	16.168	2221	2224	2226	rBV3	5270	6883	0.13%	0.015%
38	16.345	2247	2254	2258	rBV9	4645	8502	0.16%	0.019%
39	16.668	2305	2309	2314	rVB5	9097	12156	0.23%	0.027%
40	16.962	2355	2359	2361	rBV5	7235	10969	0.21%	0.025%
41	17.198	2393	2399	2409	rBV	1694767	2358285	44.11%	5.292%
42	17.298	2410	2416	2429	rVV	2619539	3634695	67.98%	8.156%
43	17.733	2487	2490	2494	rVB3	8303	11082	0.21%	0.025%
44	17.874	2510	2514	2519	rVB7	8474	11860	0.22%	0.027%
45	18.103	2547	2553	2560	rBV6	24575	51643	0.97%	0.116%
46	18.174	2562	2565	2569	rVB	11718	14858	0.28%	0.033%
47	18.639	2643	2644	2648	rBV3	4433	6325	0.12%	0.014%
48	19.156	2729	2732	2738	rVB2	31021	40079	0.75%	0.090%
49	19.233	2741	2745	2751	rVV2	28391	43836	0.82%	0.098%
50	19.592	2800	2806	2814	rBV	3463154	4424309	82.75%	9.928%
51	20.592	2973	2976	2980	rVB	76015	76368	1.43%	0.171%
52	21.097	3059	3062	3067	rBV5	79166	107170	2.00%	0.240%
53	21.297	3093	3096	3101	rBV2	112339	123623	2.31%	0.277%
54	21.380	3105	3110	3119	rBV	2398881	3004843	56.20%	6.743%
55	23.568	3475	3482	3494	rVB2	2713424	5346353	100.00%	11.997%
56	23.715	3501	3507	3518	rVB2	1715785	3293804	61.61%	7.391%




Sum of corrected areas: 44563155

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036243.D
Acq On : 12 Aug 2022 23:36
Operator : CG/JU
Sample : N4165-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBX8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

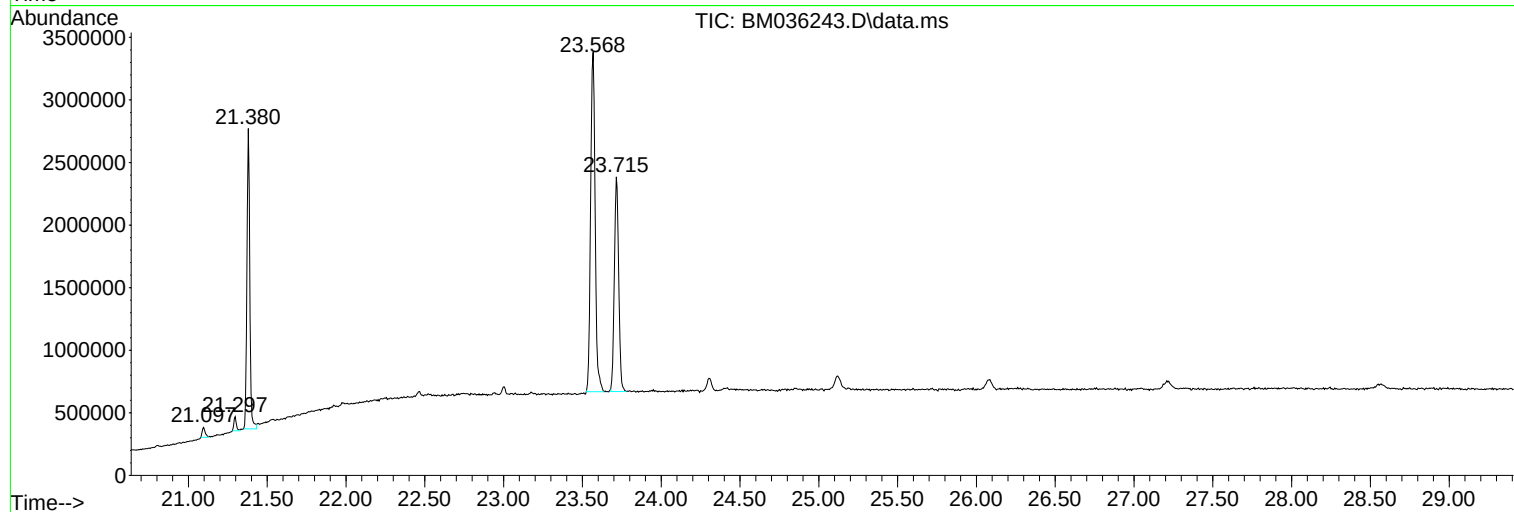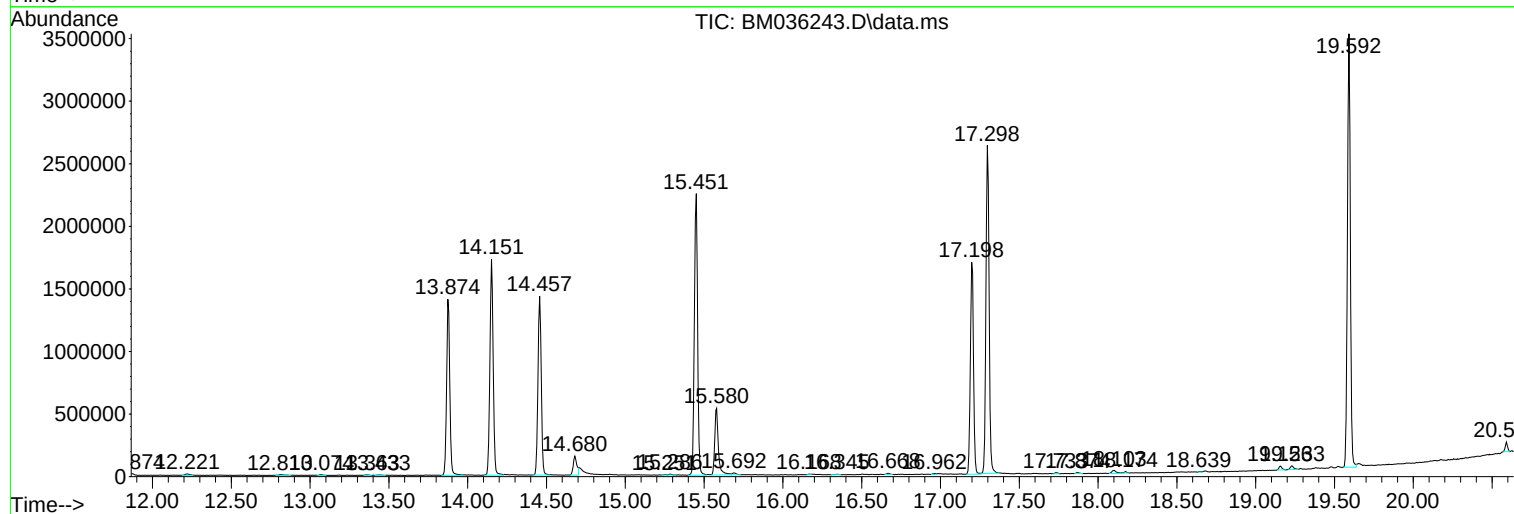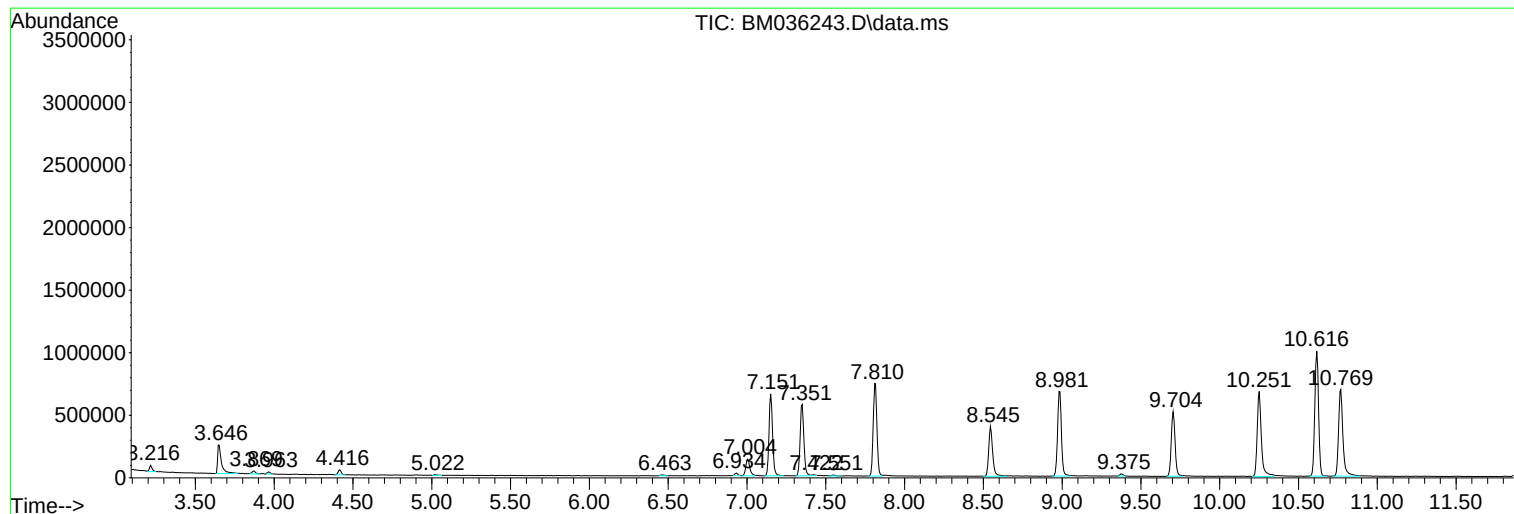

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036243.D
Acq On : 12 Aug 2022 23:36
Operator : CG/JU
Sample : N4165-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBX8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036243.D
Acq On : 12 Aug 2022 23:36
Operator : CG/JU
Sample : N4165-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBX8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc