

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036246.D
 Acq On : 13 Aug 2022 01:24
 Operator : CG/JU
 Sample : N4069-17
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GBJM1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036246.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	13	16	19	rBV	55413	62456	1.12%	0.139%
2	3.216	19	22	31	rVB	54890	69759	1.25%	0.155%
3	3.652	93	96	113	rBV	201179	326375	5.85%	0.727%
4	3.869	129	133	141	rVB	25610	37392	0.67%	0.083%
5	3.969	146	150	158	rVB	19153	28227	0.51%	0.063%
6	4.416	221	226	231	rVV	39577	51014	0.91%	0.114%
7	4.905	304	309	313	rBV5	3616	6073	0.11%	0.014%
8	5.022	324	329	334	rVB8	6751	10392	0.19%	0.023%
9	6.934	647	654	658	rBV	20177	29737	0.53%	0.066%
10	7.004	660	666	678	rVB	156842	270556	4.85%	0.603%
11	7.151	684	691	704	rBV	690193	1082004	19.39%	2.412%
12	7.346	718	724	735	rBV	625196	1038303	18.61%	2.314%
13	7.428	735	738	747	rVB8	7767	15977	0.29%	0.036%
14	7.810	797	803	813	rBV	734887	1172485	21.01%	2.613%
15	7.887	813	816	820	rVB5	5359	7715	0.14%	0.017%
16	8.546	920	928	943	rBV	455958	785173	14.07%	1.750%
17	8.981	995	1002	1011	rBV	762850	1254947	22.49%	2.797%
18	9.375	1064	1069	1077	rVB	19676	35167	0.63%	0.078%
19	9.704	1118	1125	1134	rBV	559898	937540	16.80%	2.090%
20	10.251	1209	1218	1240	rBV	739498	1366674	24.49%	3.046%
21	10.616	1273	1280	1287	rBV	1008264	1638521	29.37%	3.652%
22	10.675	1287	1290	1296	rVB7	8948	14097	0.25%	0.031%
23	10.769	1297	1306	1328	rBV	692200	1360961	24.39%	3.034%
24	11.451	1415	1422	1426	rBV7	5321	9657	0.17%	0.022%
25	11.869	1486	1493	1499	rVB3	14218	23957	0.43%	0.053%
26	12.216	1546	1552	1558	rBV2	11940	25376	0.45%	0.057%
27	12.816	1650	1654	1663	rVB6	6662	12780	0.23%	0.028%
28	13.069	1693	1697	1703	rVB4	7246	12140	0.22%	0.027%
29	13.363	1743	1747	1751	rVB5	7536	11317	0.20%	0.025%
30	13.433	1756	1759	1765	rVB7	5022	6896	0.12%	0.015%
31	13.875	1827	1834	1847	rBV	1490823	2073266	37.16%	4.621%
32	14.010	1854	1857	1864	rVB8	2710	5676	0.10%	0.013%
33	14.151	1871	1881	1890	rBV	1780827	2567539	46.02%	5.723%
34	14.457	1926	1933	1944	rBV	1383085	1949201	34.93%	4.345%
35	14.710	1969	1976	1989	rBV2	60038	172681	3.09%	0.385%
36	14.886	2001	2006	2014	rVB2	6161	14968	0.27%	0.033%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036246.D
 Acq On : 13 Aug 2022 01:24
 Operator : CG/JU
 Sample : N4069-17
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GBJM1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	15.251	2063	2068	2071	rBV2	12023	14858	0.27%	0.033%
38	15.286	2072	2074	2079	rVB5	5578	6558	0.12%	0.015%
39	15.445	2093	2101	2115	rBV	2260365	3307062	59.27%	7.371%
40	15.574	2117	2123	2136	rBV	643154	971906	17.42%	2.166%
41	15.686	2138	2142	2148	rVB	24289	38156	0.68%	0.085%
42	16.122	2210	2216	2218	rBV7	3893	7364	0.13%	0.016%
43	16.163	2220	2223	2225	rBV4	4849	5633	0.10%	0.013%
44	16.233	2231	2235	2238	rVB6	6943	9430	0.17%	0.021%
45	16.674	2306	2310	2314	rVB6	8910	14394	0.26%	0.032%
46	16.957	2355	2358	2361	rBV5	7026	9934	0.18%	0.022%
47	17.121	2383	2386	2390	rVB6	6587	7334	0.13%	0.016%
48	17.198	2393	2399	2409	rBV	1550395	2168202	38.86%	4.833%
49	17.298	2410	2416	2429	rVV	2817322	3832001	68.68%	8.541%
50	17.492	2445	2449	2452	rVB2	9718	11730	0.21%	0.026%
51	17.739	2487	2491	2496	rVB5	7399	11222	0.20%	0.025%
52	17.868	2511	2513	2518	rVB6	7339	11706	0.21%	0.026%
53	18.098	2548	2552	2557	rBV7	12399	22412	0.40%	0.050%
54	18.174	2561	2565	2568	rVV	31799	39966	0.72%	0.089%
55	18.680	2647	2651	2654	rBV5	9891	15680	0.28%	0.035%
56	19.157	2728	2732	2739	rBV4	30415	45823	0.82%	0.102%
57	19.227	2740	2744	2747	rBV	31611	44013	0.79%	0.098%
58	19.592	2800	2806	2813	rBV	3613866	4649817	83.33%	10.364%
59	20.592	2973	2976	2981	rVB	69337	78338	1.40%	0.175%
60	21.380	3105	3110	3118	rBV	2066100	2633846	47.20%	5.871%
61	23.568	3475	3482	3493	rVB	2929104	5579686	100.00%	12.437%
62	23.715	3501	3507	3517	rVB2	1492312	2839444	50.89%	6.329%




Sum of corrected areas: 44863514

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036246.D
Acq On : 13 Aug 2022 01:24
Operator : CG/JU
Sample : N4069-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBJM1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

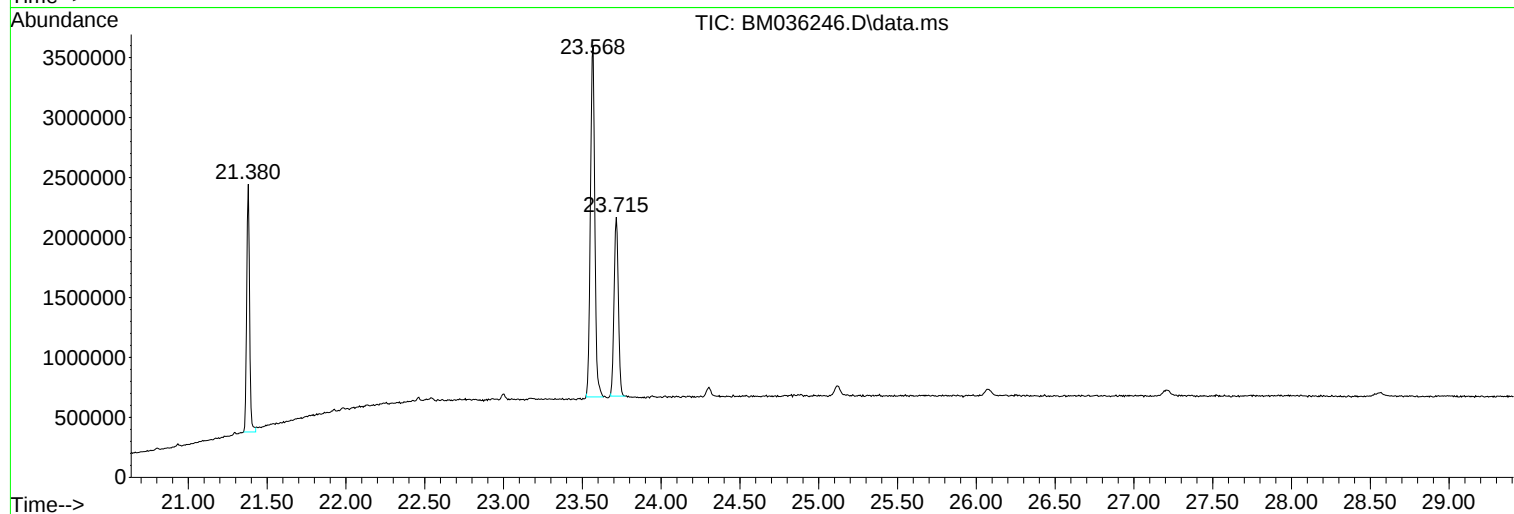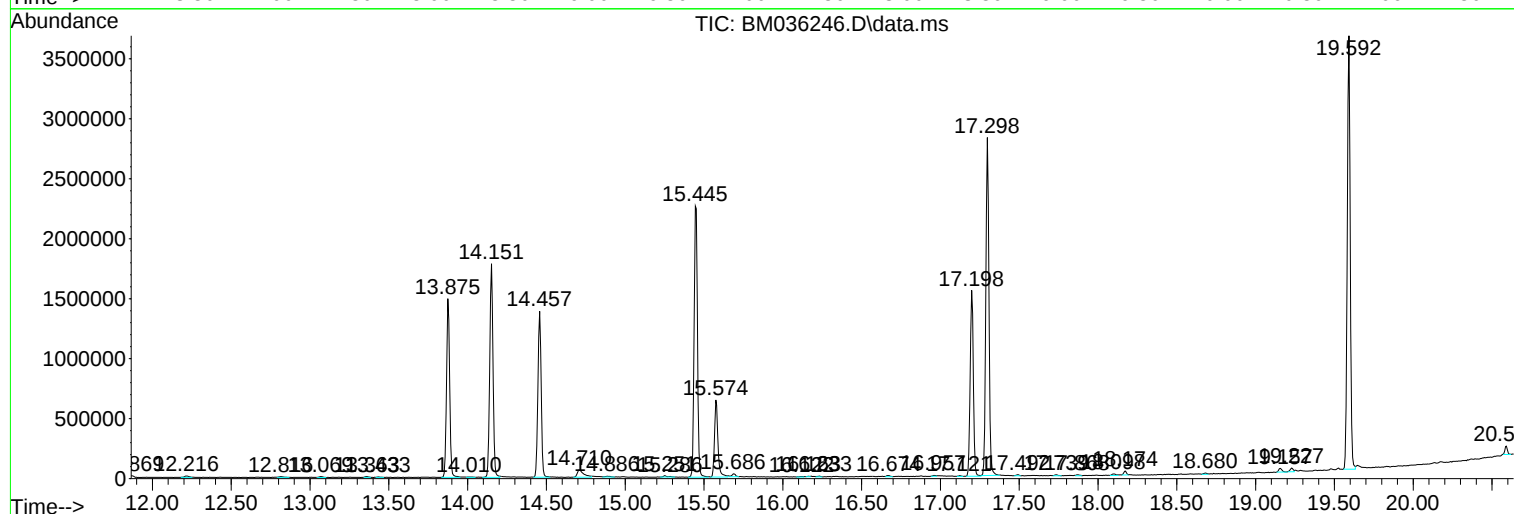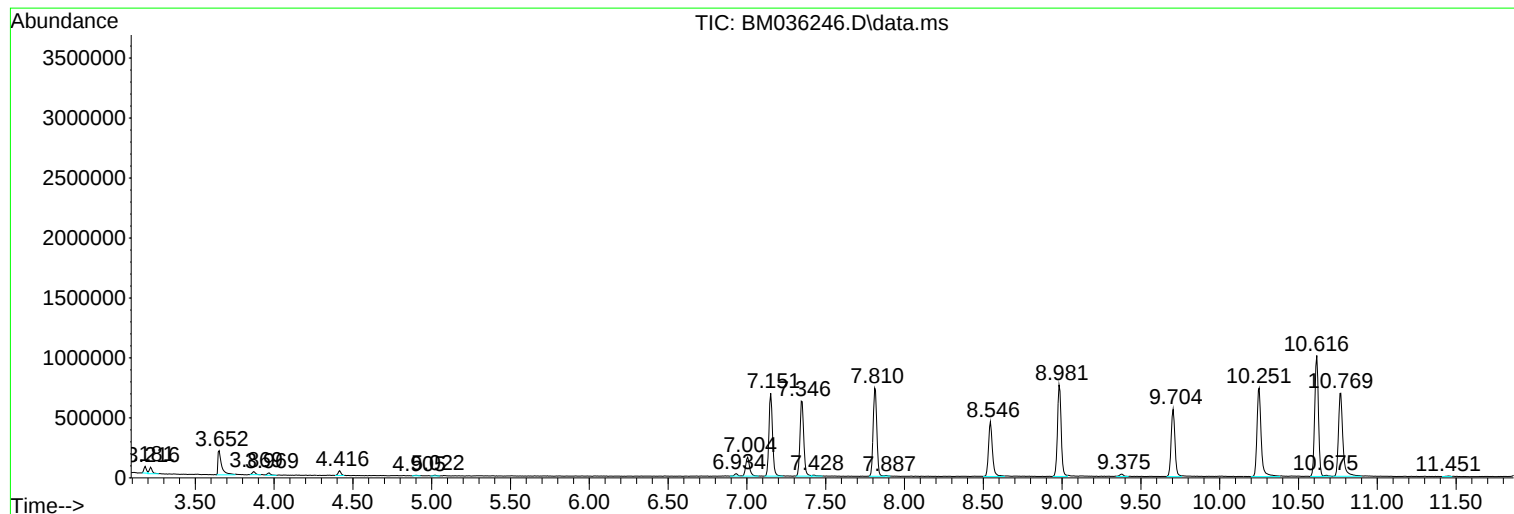

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036246.D
Acq On : 13 Aug 2022 01:24
Operator : CG/JU
Sample : N4069-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBJM1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036246.D
Acq On : 13 Aug 2022 01:24
Operator : CG/JU
Sample : N4069-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBJM1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc