

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036247.D
 Acq On : 13 Aug 2022 02:00
 Operator : CG/JU
 Sample : N4165-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGBX7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036247.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	13	15	18	rVV3	8033	9320	0.19%	0.021%
2	3.216	18	22	32	rVB	53563	70915	1.42%	0.158%
3	3.652	93	96	118	rBV	159855	258460	5.16%	0.575%
4	3.869	129	133	138	rBV	26381	39107	0.78%	0.087%
5	3.963	146	149	154	rVB	17619	22957	0.46%	0.051%
6	4.416	221	226	230	rBV	42866	59486	1.19%	0.132%
7	4.899	305	308	313	rBV4	5422	6627	0.13%	0.015%
8	5.022	324	329	333	rBV3	8224	12440	0.25%	0.028%
9	6.934	647	654	659	rVV	23208	34328	0.69%	0.076%
10	7.004	660	666	681	rVB	174680	306261	6.12%	0.682%
11	7.151	684	691	703	rVV	741520	1151054	23.00%	2.563%
12	7.346	718	724	734	rBV	688702	1114553	22.27%	2.481%
13	7.422	734	737	741	rVB4	7072	10310	0.21%	0.023%
14	7.810	790	803	813	rBV	747252	1198390	23.94%	2.668%
15	7.881	813	815	818	rVB4	4947	5434	0.11%	0.012%
16	8.545	921	928	941	rBV	498971	853595	17.05%	1.900%
17	8.981	994	1002	1016	rBV	826327	1357453	27.12%	3.022%
18	9.128	1024	1027	1034	rVB8	5253	8290	0.17%	0.018%
19	9.375	1065	1069	1076	rVB2	23521	35467	0.71%	0.079%
20	9.704	1116	1125	1139	rBV	612333	1038169	20.74%	2.311%
21	10.251	1210	1218	1240	rBV	808555	1489705	29.76%	3.316%
22	10.616	1272	1280	1289	rBV	1016584	1688174	33.73%	3.758%
23	10.769	1298	1306	1327	rBV	733599	1411324	28.20%	3.142%
24	11.869	1485	1493	1501	rVB2	13935	26059	0.52%	0.058%
25	12.216	1547	1552	1563	rVB2	13556	29884	0.60%	0.067%
26	12.816	1649	1654	1660	rBV6	5222	8494	0.17%	0.019%
27	13.069	1692	1697	1701	rBV6	6160	9784	0.20%	0.022%
28	13.875	1826	1834	1848	rBV	1563866	2150191	42.96%	4.787%
29	14.151	1874	1881	1894	rBV	1959011	2792641	55.79%	6.217%
30	14.280	1900	1903	1908	rVB7	3030	5235	0.10%	0.012%
31	14.457	1926	1933	1943	rBV	1387518	2003634	40.03%	4.461%
32	14.704	1967	1975	1989	rBV2	66112	204480	4.09%	0.455%
33	14.886	2001	2006	2013	rVB9	6850	15749	0.31%	0.035%
34	15.251	2064	2068	2071	rBV4	3903	6084	0.12%	0.014%
35	15.286	2071	2074	2079	rVB2	6357	10385	0.21%	0.023%
36	15.445	2093	2101	2116	rBV	2391271	3504602	70.02%	7.802%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036247.D
 Acq On : 13 Aug 2022 02:00
 Operator : CG/JU
 Sample : N4165-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGBX7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	15.574	2118	2123	2138	rVV	617987	928427	18.55%	2.067%
38	15.692	2138	2143	2147	rVB3	13572	23886	0.48%	0.053%
39	16.174	2220	2225	2229	rVV7	6772	15101	0.30%	0.034%
40	16.233	2231	2235	2239	rVB7	3508	6029	0.12%	0.013%
41	16.668	2304	2309	2312	rBV4	10225	14748	0.29%	0.033%
42	16.957	2355	2358	2362	rBV6	8650	12666	0.25%	0.028%
43	17.198	2393	2399	2409	rBV	1591402	2193503	43.82%	4.883%
44	17.298	2409	2416	2433	rVV	2779106	3855111	77.02%	8.583%
45	17.492	2446	2449	2454	rVB6	5218	7177	0.14%	0.016%
46	17.733	2487	2490	2496	rBV5	8343	10816	0.22%	0.024%
47	17.874	2511	2514	2518	rVB6	7846	9073	0.18%	0.020%
48	18.098	2548	2552	2558	rBV6	15678	25435	0.51%	0.057%
49	18.174	2562	2565	2573	rVB	9658	15525	0.31%	0.035%
50	18.392	2598	2602	2604	rBV5	5145	8683	0.17%	0.019%
51	19.157	2728	2732	2737	rBV3	31853	43148	0.86%	0.096%
52	19.227	2741	2744	2749	rVV	27209	39772	0.79%	0.089%
53	19.592	2800	2806	2814	rBV	3323648	4381927	87.54%	9.755%
54	20.592	2973	2976	2980	rVB2	69204	74798	1.49%	0.167%
55	21.380	3105	3110	3119	rBV	2014369	2585943	51.66%	5.757%
56	23.568	3475	3482	3493	rVB2	2678508	5005431	100.00%	11.143%
57	23.715	3501	3507	3516	rVB2	1378117	2711788	54.18%	6.037%




Sum of corrected areas: 44918028

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036247.D
Acq On : 13 Aug 2022 02:00
Operator : CG/JU
Sample : N4165-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBX7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

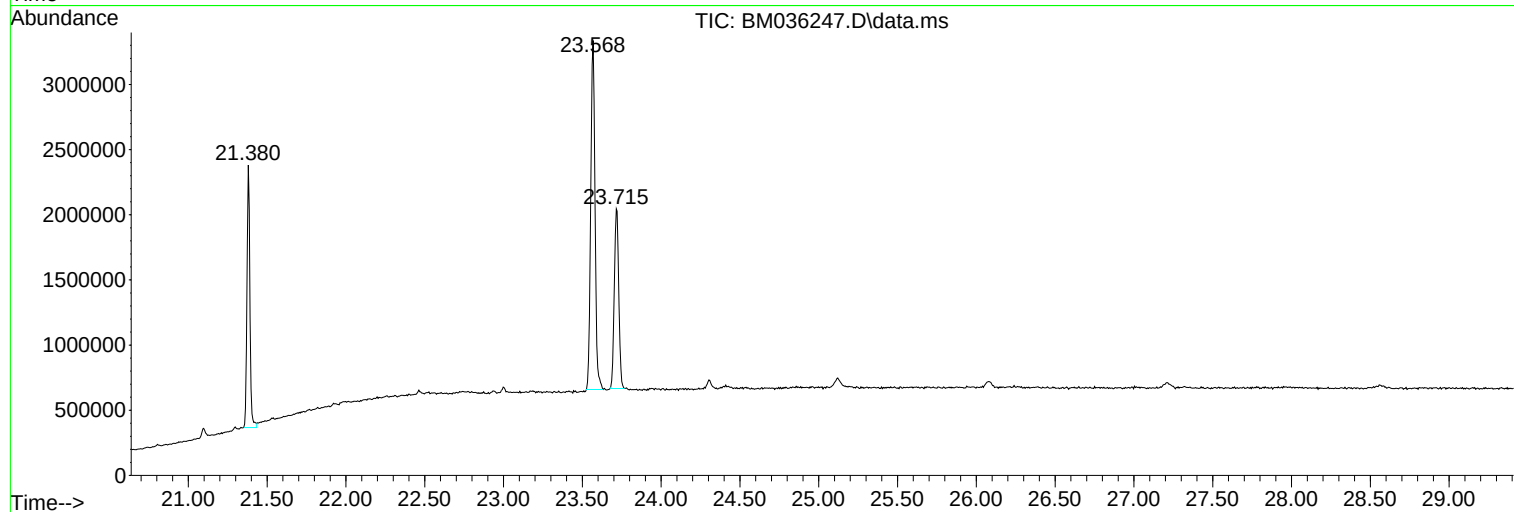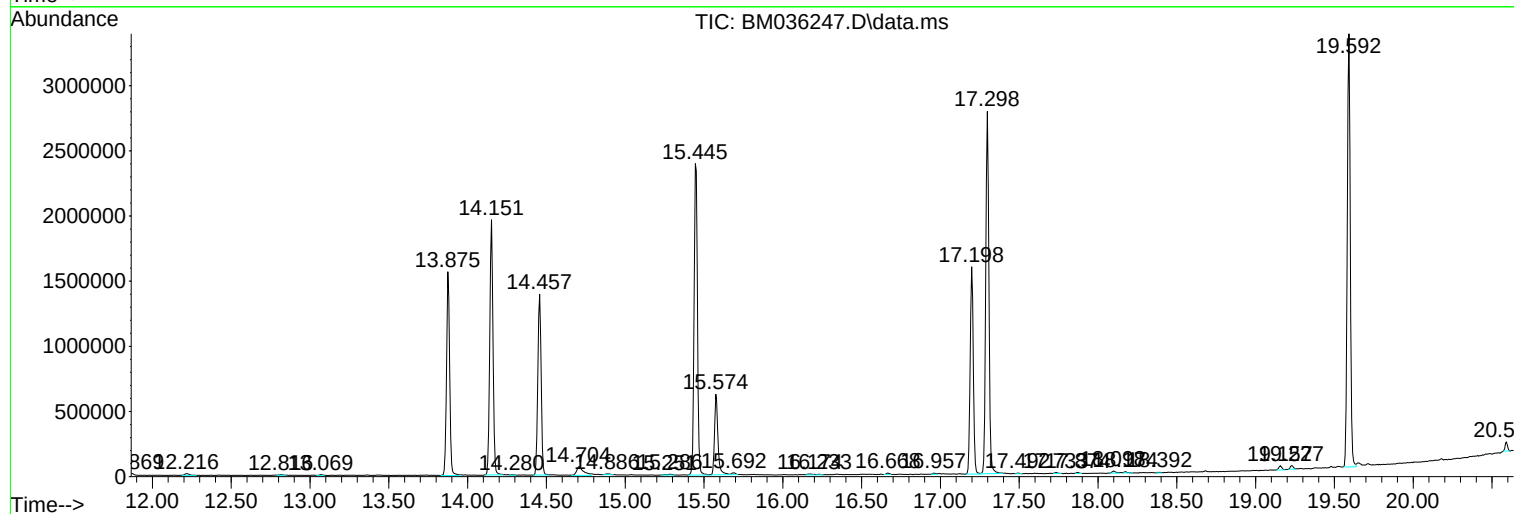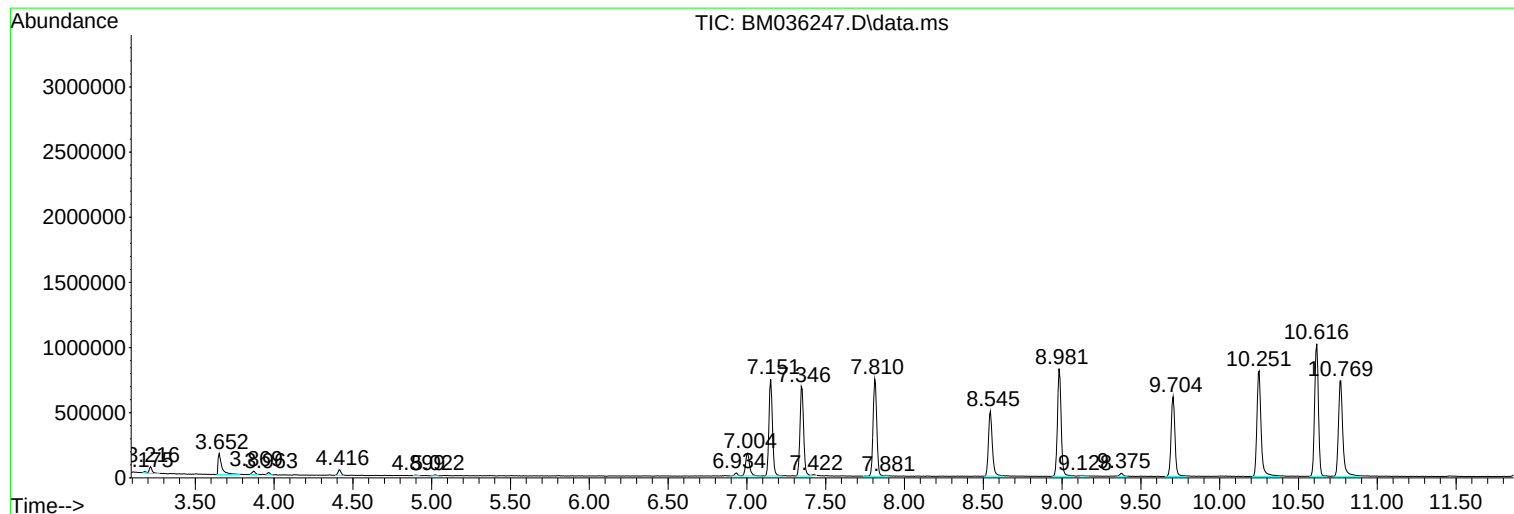

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036247.D
Acq On : 13 Aug 2022 02:00
Operator : CG/JU
Sample : N4165-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBX7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036247.D
Acq On : 13 Aug 2022 02:00
Operator : CG/JU
Sample : N4165-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBX7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------