

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036248.D
 Acq On : 13 Aug 2022 02:36
 Operator : CG/JU
 Sample : N4165-13
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGC17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036248.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	18	22	31	rVB	44391	59133	1.09%	0.152%
2	3.658	95	97	111	rBV	84848	141362	2.60%	0.363%
3	3.869	128	133	140	rBV2	22359	37674	0.69%	0.097%
4	3.963	145	149	155	rVB	17839	25320	0.47%	0.065%
5	4.416	221	226	232	rVB	38268	54223	1.00%	0.139%
6	4.899	305	308	313	rBV3	6869	9916	0.18%	0.025%
7	6.934	649	654	659	rVV	18338	25263	0.46%	0.065%
8	7.004	661	666	675	rVB	97049	171127	3.15%	0.439%
9	7.151	684	691	704	rBV	627544	985923	18.14%	2.529%
10	7.345	718	724	735	rBV	317857	535982	9.86%	1.375%
11	7.422	735	737	741	rVB4	7202	9963	0.18%	0.026%
12	7.810	795	803	814	rBV	630580	1007709	18.54%	2.585%
13	8.545	922	928	942	rBV	233425	421419	7.75%	1.081%
14	8.981	994	1002	1022	rBV	681415	1150320	21.16%	2.951%
15	9.375	1063	1069	1076	rVB2	18748	30078	0.55%	0.077%
16	9.704	1117	1125	1138	rBV	294181	514806	9.47%	1.321%
17	10.251	1211	1218	1239	rBV	363070	700495	12.89%	1.797%
18	10.616	1273	1280	1291	rBV	837587	1405427	25.86%	3.606%
19	10.769	1297	1306	1329	rBV	611209	1212634	22.31%	3.111%
20	11.875	1489	1494	1498	rVB3	12132	18821	0.35%	0.048%
21	12.216	1546	1552	1557	rBV4	10388	20924	0.38%	0.054%
22	12.816	1651	1654	1658	rVV6	4194	6481	0.12%	0.017%
23	13.357	1742	1746	1753	rVV7	6004	12128	0.22%	0.031%
24	13.874	1827	1834	1847	rBV	1236917	1689354	31.08%	4.334%
25	14.151	1873	1881	1892	rBV	1651280	2372689	43.65%	6.087%
26	14.457	1926	1933	1944	rBV	1162997	1697537	31.23%	4.355%
27	14.721	1971	1978	1992	rBV3	29589	105032	1.93%	0.269%
28	14.898	2006	2008	2015	rVB8	5356	7112	0.13%	0.018%
29	15.445	2091	2101	2112	rBV	2160222	3082145	56.70%	7.907%
30	15.574	2118	2123	2136	rBV	278862	458945	8.44%	1.177%
31	15.686	2138	2142	2148	rVB6	12942	23685	0.44%	0.061%
32	16.163	2218	2223	2225	rVV4	5577	8353	0.15%	0.021%
33	16.186	2225	2227	2232	rVV6	5866	8615	0.16%	0.022%
34	16.498	2275	2280	2284	rBV8	3515	7338	0.14%	0.019%
35	16.663	2305	2308	2312	rBV3	9211	10551	0.19%	0.027%
36	16.963	2353	2359	2361	rBV5	6228	11338	0.21%	0.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036248.D
 Acq On : 13 Aug 2022 02:36
 Operator : CG/JU
 Sample : N4165-13
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGC17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	17.198	2393	2399	2407	rBV	1426598	1950855	35.89%	5.005%
38	17.298	2409	2416	2434	rVB	2657020	3711054	68.27%	9.521%
39	17.733	2488	2490	2494	rVB3	6329	6419	0.12%	0.016%
40	18.098	2548	2552	2557	rBV8	15048	22577	0.42%	0.058%
41	18.168	2561	2564	2568	rBV2	12444	16140	0.30%	0.041%
42	18.680	2649	2651	2656	rVB5	8813	10362	0.19%	0.027%
43	19.156	2728	2732	2737	rBV3	29428	41594	0.77%	0.107%
44	19.227	2740	2744	2748	rBV	30087	46188	0.85%	0.118%
45	19.592	2800	2806	2813	rBV	3510394	4471401	82.26%	11.471%
46	20.592	2973	2976	2981	rVB	65683	69193	1.27%	0.178%
47	21.380	3105	3110	3117	rBV	1962676	2488009	45.77%	6.383%
48	23.568	3475	3482	3495	rVB2	2751687	5435455	100.00%	13.945%
49	23.715	3501	3507	3517	rVB	1399586	2669950	49.12%	6.850%




Sum of corrected areas: 38979019

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036248.D
Acq On : 13 Aug 2022 02:36
Operator : CG/JU
Sample : N4165-13
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGC17

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

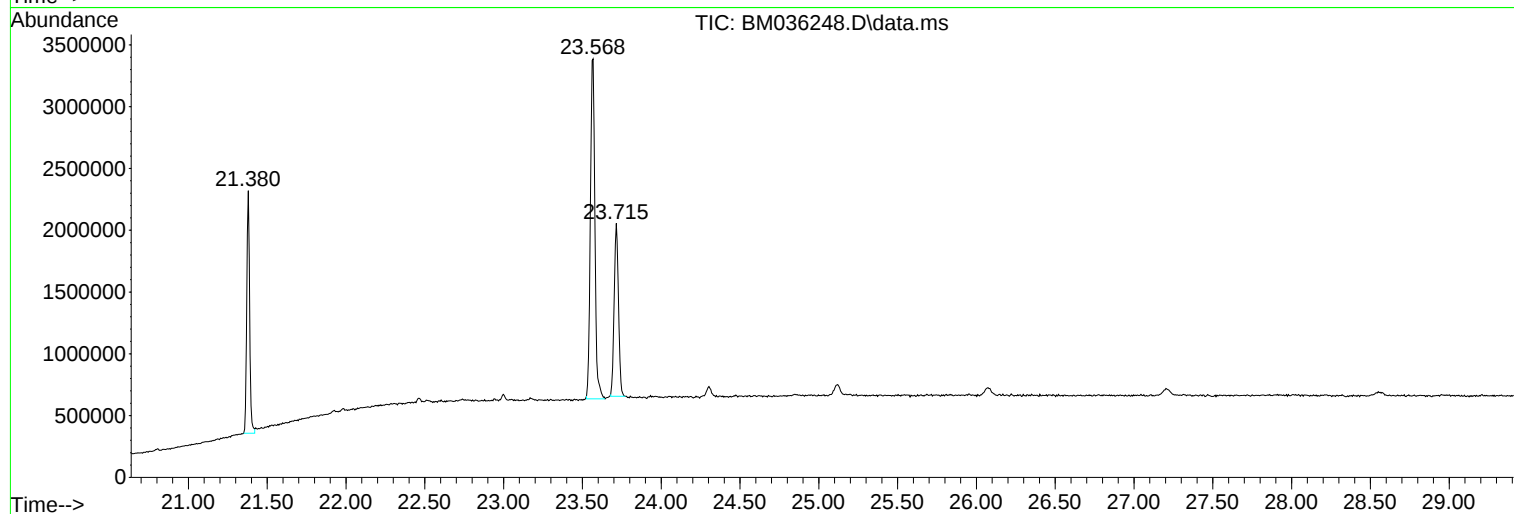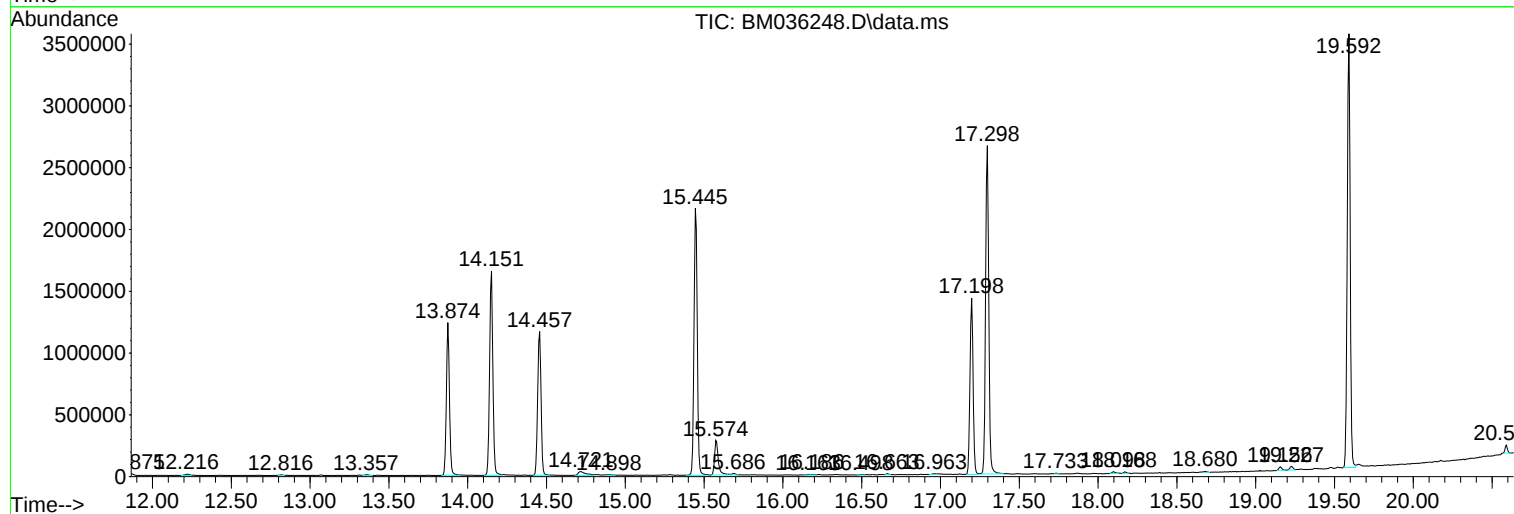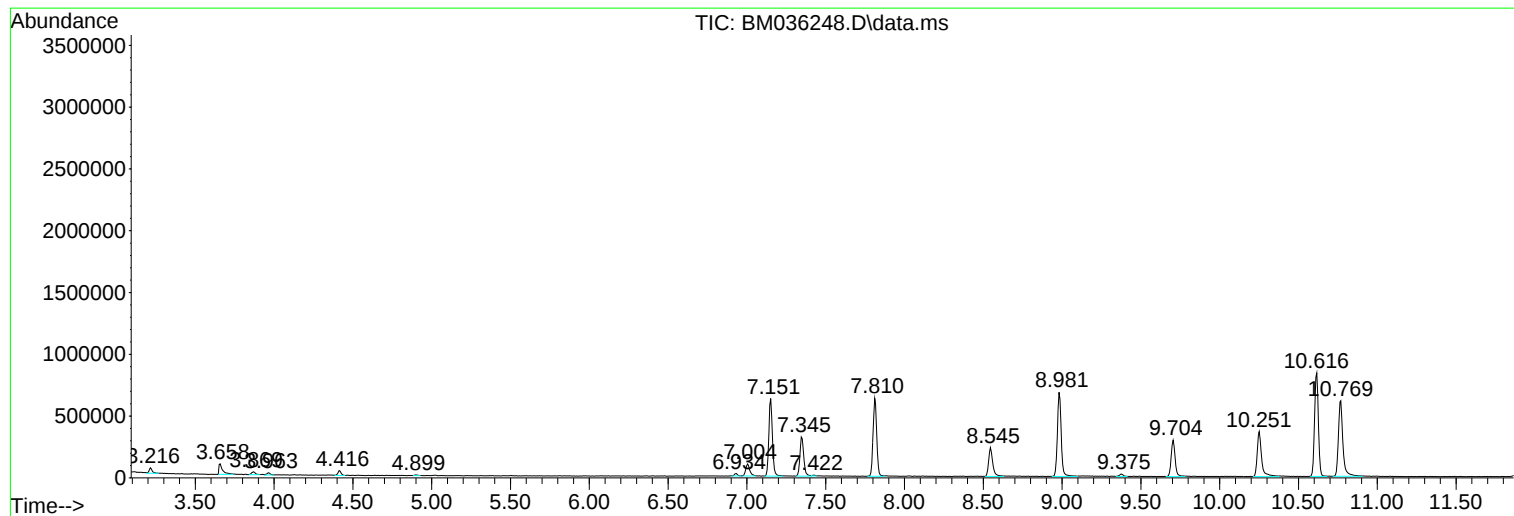

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036248.D
Acq On : 13 Aug 2022 02:36
Operator : CG/JU
Sample : N4165-13
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGC17

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036248.D
Acq On : 13 Aug 2022 02:36
Operator : CG/JU
Sample : N4165-13
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGC17

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc