

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036249.D
 Acq On : 13 Aug 2022 03:11
 Operator : CG/JU
 Sample : N4165-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGBY5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036249.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	18	22	29	rVB	53624	66654	1.24%	0.153%
2	3.646	92	95	107	rBV	205145	322719	6.02%	0.742%
3	3.869	128	133	139	rVB	27128	38579	0.72%	0.089%
4	3.963	145	149	154	rVB	16454	20724	0.39%	0.048%
5	4.416	221	226	231	rVB	40843	56169	1.05%	0.129%
6	4.899	303	308	314	rBV4	5184	8194	0.15%	0.019%
7	5.022	325	329	331	rVB2	6269	5604	0.10%	0.013%
8	6.928	649	653	657	rBV	20104	28007	0.52%	0.064%
9	7.004	660	666	675	rVV	148150	261172	4.87%	0.601%
10	7.151	683	691	701	rBV	682638	1077538	20.09%	2.478%
11	7.345	717	724	734	rBV	628857	1017422	18.97%	2.340%
12	7.428	734	738	746	rVB	8926	18915	0.35%	0.043%
13	7.810	796	803	813	rBV	657603	1039985	19.39%	2.392%
14	8.545	920	928	943	rBV	424688	763030	14.22%	1.755%
15	8.981	993	1002	1015	rBV	755440	1246556	23.24%	2.867%
16	9.128	1022	1027	1029	rBV7	3099	5587	0.10%	0.013%
17	9.375	1064	1069	1074	rBV2	18934	29916	0.56%	0.069%
18	9.704	1117	1125	1137	rBV	539195	939994	17.52%	2.162%
19	10.245	1208	1217	1240	rBV	726434	1350460	25.17%	3.106%
20	10.616	1272	1280	1289	rBV	857056	1450332	27.04%	3.335%
21	10.763	1297	1305	1321	rBV	734838	1383352	25.79%	3.181%
22	11.869	1489	1493	1499	rVB2	11828	20088	0.37%	0.046%
23	12.222	1547	1553	1559	rBV4	11108	23719	0.44%	0.055%
24	12.810	1651	1653	1659	rVB6	5007	7763	0.14%	0.018%
25	13.069	1693	1697	1701	rVB7	4115	6930	0.13%	0.016%
26	13.357	1741	1746	1751	rBV4	3434	6141	0.11%	0.014%
27	13.874	1827	1834	1847	rBV	1484785	2042408	38.07%	4.697%
28	14.151	1872	1881	1898	rBV	1817210	2621194	48.86%	6.028%
29	14.457	1925	1933	1944	rVB	1205952	1756207	32.74%	4.039%
30	14.710	1969	1976	1992	rBV2	54756	174403	3.25%	0.401%
31	15.280	2070	2073	2079	rVB3	4927	7784	0.15%	0.018%
32	15.445	2093	2101	2117	rBV	2368284	3344482	62.34%	7.691%
33	15.574	2117	2123	2139	rVV	590731	889074	16.57%	2.045%
34	15.686	2139	2142	2152	rVB5	15144	28731	0.54%	0.066%
35	16.010	2193	2197	2205	rVB10	3391	6537	0.12%	0.015%
36	16.168	2220	2224	2232	rBV2	28718	62059	1.16%	0.143%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036249.D
 Acq On : 13 Aug 2022 03:11
 Operator : CG/JU
 Sample : N4165-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGBY5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	16.327	2246	2251	2256	rBV7	3841	7175	0.13%	0.016%
38	16.504	2275	2281	2286	rBV9	4974	11137	0.21%	0.026%
39	16.662	2305	2308	2313	rVB5	8540	13882	0.26%	0.032%
40	16.957	2353	2358	2361	rBV6	6577	11439	0.21%	0.026%
41	17.198	2393	2399	2408	rBV	1495103	2013240	37.53%	4.630%
42	17.298	2410	2416	2433	rVB	2705245	3765614	70.20%	8.660%
43	17.733	2487	2490	2496	rVB5	8314	12464	0.23%	0.029%
44	17.874	2511	2514	2518	rVB5	8147	10457	0.19%	0.024%
45	18.098	2548	2552	2559	rBV4	25937	40034	0.75%	0.092%
46	18.168	2561	2564	2568	rVB	9802	13266	0.25%	0.031%
47	19.156	2728	2732	2739	rBV4	30467	44569	0.83%	0.102%
48	19.227	2741	2744	2748	rVV2	28652	38488	0.72%	0.089%
49	19.592	2800	2806	2813	rBV	3409873	4544065	84.71%	10.450%
50	20.592	2973	2976	2981	rVB	69754	71255	1.33%	0.164%
51	21.092	3058	3061	3067	rBV3	105206	175683	3.27%	0.404%
52	21.380	3105	3110	3118	rBV	2007139	2520144	46.98%	5.795%
53	23.568	3475	3482	3495	rVB2	2739146	5364495	100.00%	12.336%
54	23.715	3501	3507	3516	rVB2	1407200	2699134	50.31%	6.207%




Sum of corrected areas: 43484970

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036249.D
Acq On : 13 Aug 2022 03:11
Operator : CG/JU
Sample : N4165-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBY5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

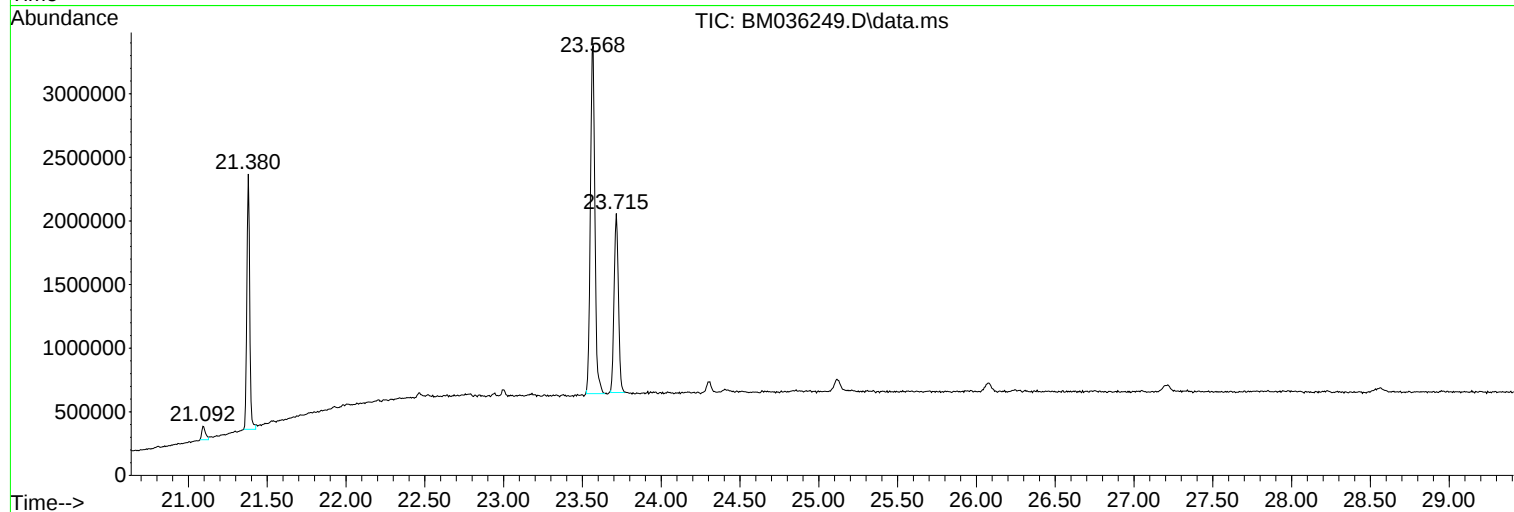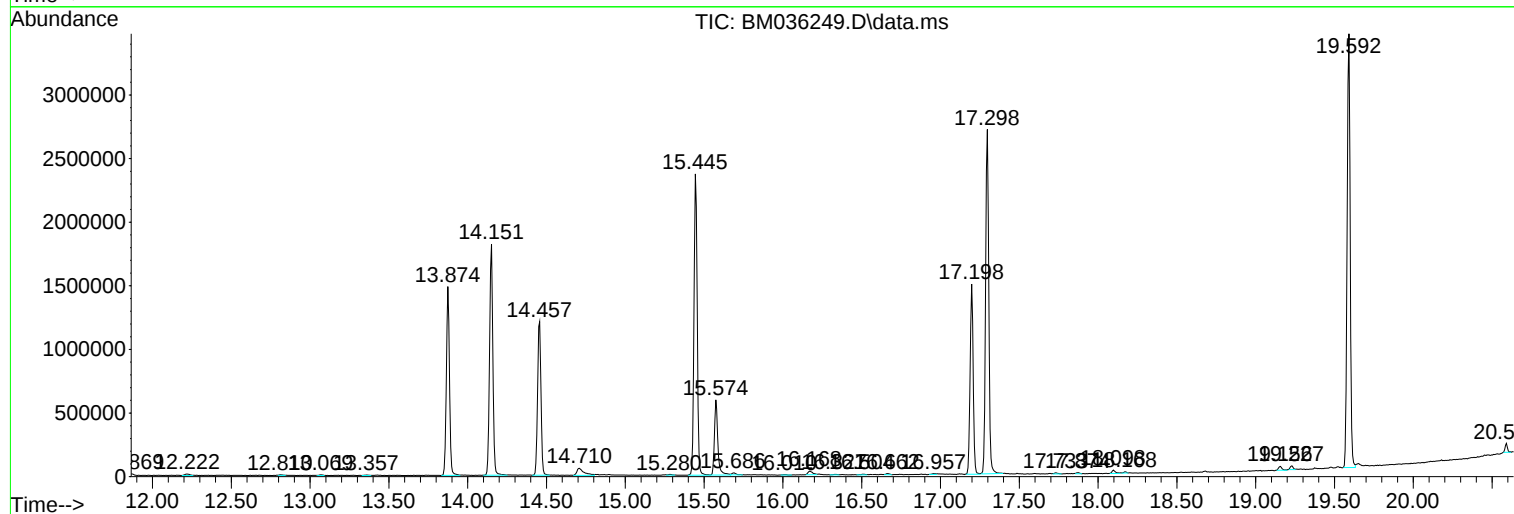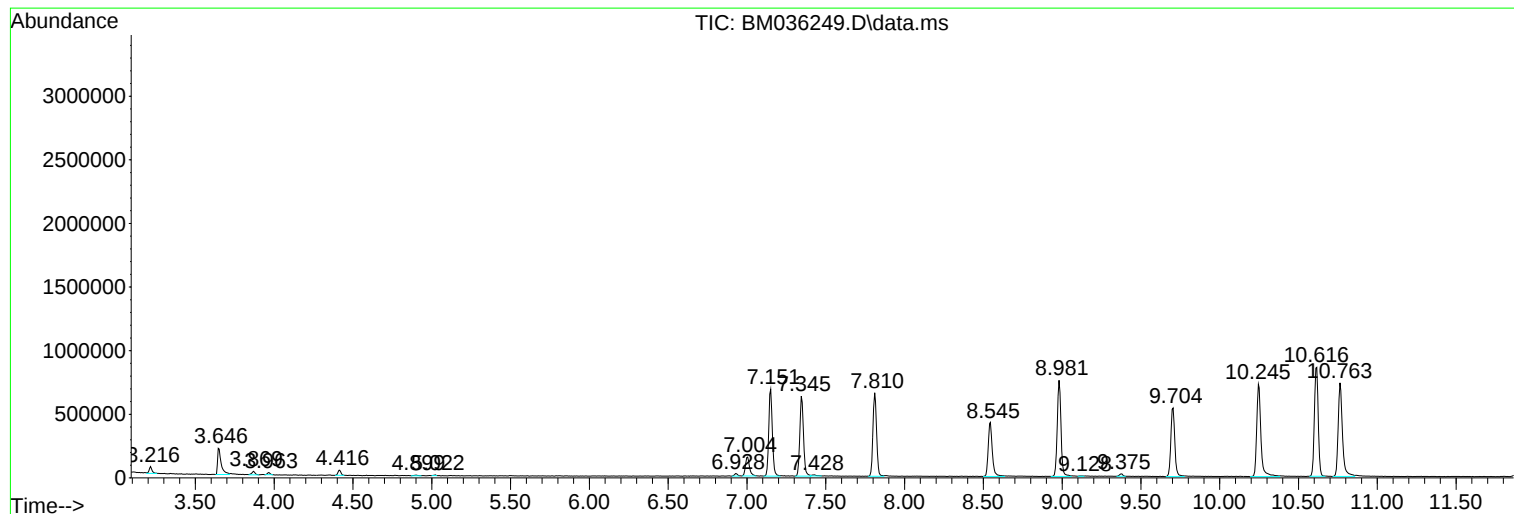

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036249.D
Acq On : 13 Aug 2022 03:11
Operator : CG/JU
Sample : N4165-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBY5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036249.D
Acq On : 13 Aug 2022 03:11
Operator : CG/JU
Sample : N4165-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBY5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc