

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036251.D
 Acq On : 13 Aug 2022 04:23
 Operator : CG/JU
 Sample : N4165-04
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGBX9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036251.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	13	16	19	rBV	21322	24984	0.43%	0.050%
2	3.216	19	22	30	rVB	66682	85753	1.48%	0.170%
3	3.646	93	95	112	rBV	297896	447426	7.73%	0.886%
4	3.869	128	133	138	rBV	29306	45546	0.79%	0.090%
5	3.963	145	149	154	rVB	28473	39131	0.68%	0.078%
6	4.346	212	214	220	rVB7	4440	5878	0.10%	0.012%
7	4.416	221	226	232	rVB	49581	71498	1.24%	0.142%
8	4.904	305	309	314	rVB4	6125	8676	0.15%	0.017%
9	5.016	325	328	334	rVB7	8076	10324	0.18%	0.020%
10	6.934	648	654	660	rVB	25179	36904	0.64%	0.073%
11	6.998	660	665	680	rBV	171135	305972	5.29%	0.606%
12	7.151	684	691	703	rBV	829565	1305674	22.56%	2.587%
13	7.345	717	724	735	rBV	763816	1219100	21.07%	2.415%
14	7.422	735	737	742	rVB6	8478	11731	0.20%	0.023%
15	7.640	770	774	779	rVB7	3555	5878	0.10%	0.012%
16	7.810	795	803	812	rBV	831102	1296211	22.40%	2.568%
17	7.881	812	815	820	rVB7	5460	9397	0.16%	0.019%
18	8.539	918	927	941	rBV	522351	899469	15.54%	1.782%
19	8.981	994	1002	1017	rBV	920539	1516980	26.22%	3.006%
20	9.375	1064	1069	1075	rVB2	24765	36109	0.62%	0.072%
21	9.704	1117	1125	1134	rBV	663993	1121300	19.38%	2.222%
22	10.245	1210	1217	1237	rBV	893868	1600024	27.65%	3.170%
23	10.610	1272	1279	1294	rVB	1089347	1833208	31.68%	3.632%
24	10.763	1296	1305	1326	rBV	903032	1655063	28.60%	3.279%
25	11.869	1487	1493	1500	rVB2	15254	24896	0.43%	0.049%
26	12.222	1547	1553	1558	rBV2	13287	26436	0.46%	0.052%
27	12.816	1650	1654	1658	rBV6	4248	7247	0.13%	0.014%
28	13.074	1693	1698	1700	rBV5	4492	6484	0.11%	0.013%
29	13.874	1827	1834	1847	rBV	1708647	2378528	41.10%	4.713%
30	14.151	1871	1881	1892	rBV	2109353	3092870	53.45%	6.128%
31	14.351	1909	1915	1918	rBV5	5753	7970	0.14%	0.016%
32	14.457	1924	1933	1945	rBV	1508684	2213896	38.26%	4.386%
33	14.704	1970	1975	1996	rBV2	67070	206437	3.57%	0.409%
34	14.898	2005	2008	2012	rVB5	6210	9106	0.16%	0.018%
35	15.251	2061	2068	2070	rBV6	4050	7350	0.13%	0.015%
36	15.445	2090	2101	2115	rBV	2738751	3903237	67.45%	7.733%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036251.D
 Acq On : 13 Aug 2022 04:23
 Operator : CG/JU
 Sample : N4165-04
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGBX9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	15.574	2118	2123	2138	rVV	736196	1055286	18.24%	2.091%
38	15.686	2138	2142	2150	rVB6	16011	32415	0.56%	0.064%
39	16.168	2219	2224	2230	rBV3	16614	37374	0.65%	0.074%
40	16.221	2232	2233	2240	rVB7	5960	8454	0.15%	0.017%
41	16.498	2277	2280	2284	rBV6	4171	7930	0.14%	0.016%
42	16.662	2304	2308	2314	rBV2	10979	14304	0.25%	0.028%
43	16.957	2354	2358	2361	rBV5	11403	17318	0.30%	0.034%
44	17.198	2392	2399	2407	rBV	1804507	2454564	42.42%	4.863%
45	17.298	2409	2416	2428	rVV	3008524	4383224	75.75%	8.684%
46	17.692	2479	2483	2486	rBV4	6725	9820	0.17%	0.019%
47	17.733	2487	2490	2496	rVB3	9472	11404	0.20%	0.023%
48	17.868	2510	2513	2519	rVB7	9639	15059	0.26%	0.030%
49	18.098	2546	2552	2559	rBV3	28479	47167	0.82%	0.093%
50	18.174	2561	2565	2568	rVB2	8512	11446	0.20%	0.023%
51	18.674	2648	2650	2655	rBV4	8639	10756	0.19%	0.021%
52	19.156	2728	2732	2739	rBV2	35517	49811	0.86%	0.099%
53	19.227	2740	2744	2748	rVV	35021	49352	0.85%	0.098%
54	19.280	2751	2753	2756	rVV4	8321	7437	0.13%	0.015%
55	19.592	2800	2806	2813	rBV	3838501	5054109	87.34%	10.014%
56	20.592	2973	2976	2979	rBV2	54348	62576	1.08%	0.124%
57	21.092	3059	3061	3068	rVB4	64528	73103	1.26%	0.145%
58	21.380	3105	3110	3117	rBV	2205309	2793570	48.28%	5.535%
59	23.562	3475	3481	3494	rVB2	2989421	5786616	100.00%	11.465%
60	23.715	3501	3507	3516	rVB2	1562948	3002686	51.89%	5.949%




Sum of corrected areas: 50472474

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036251.D
Acq On : 13 Aug 2022 04:23
Operator : CG/JU
Sample : N4165-04
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBX9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

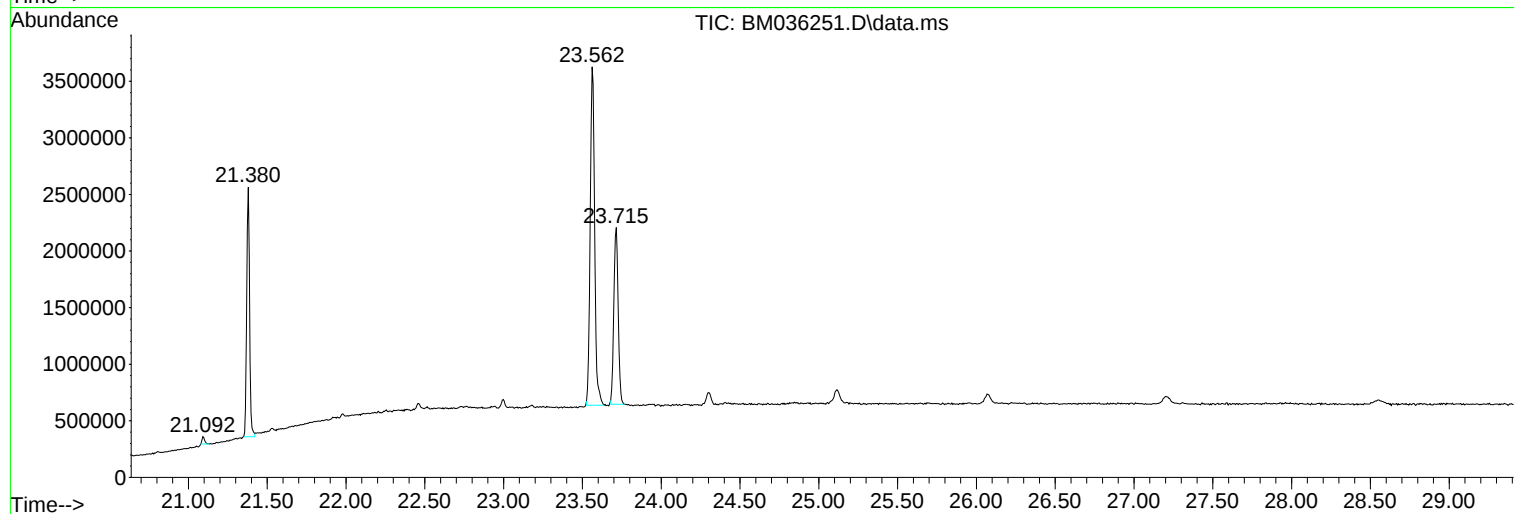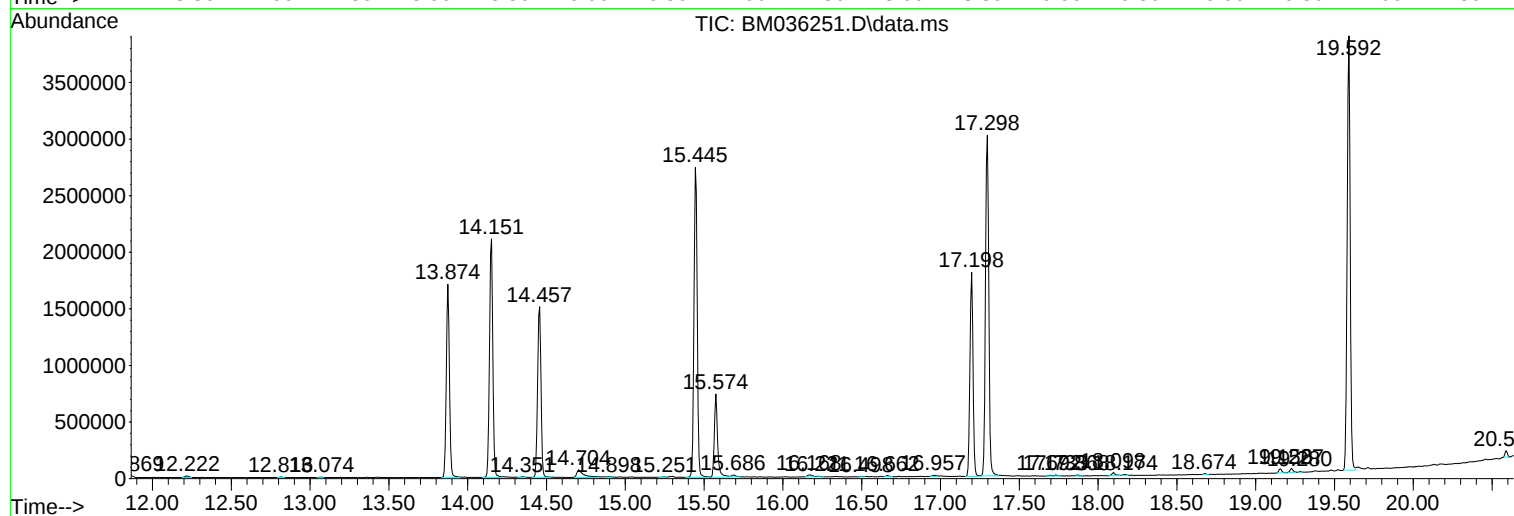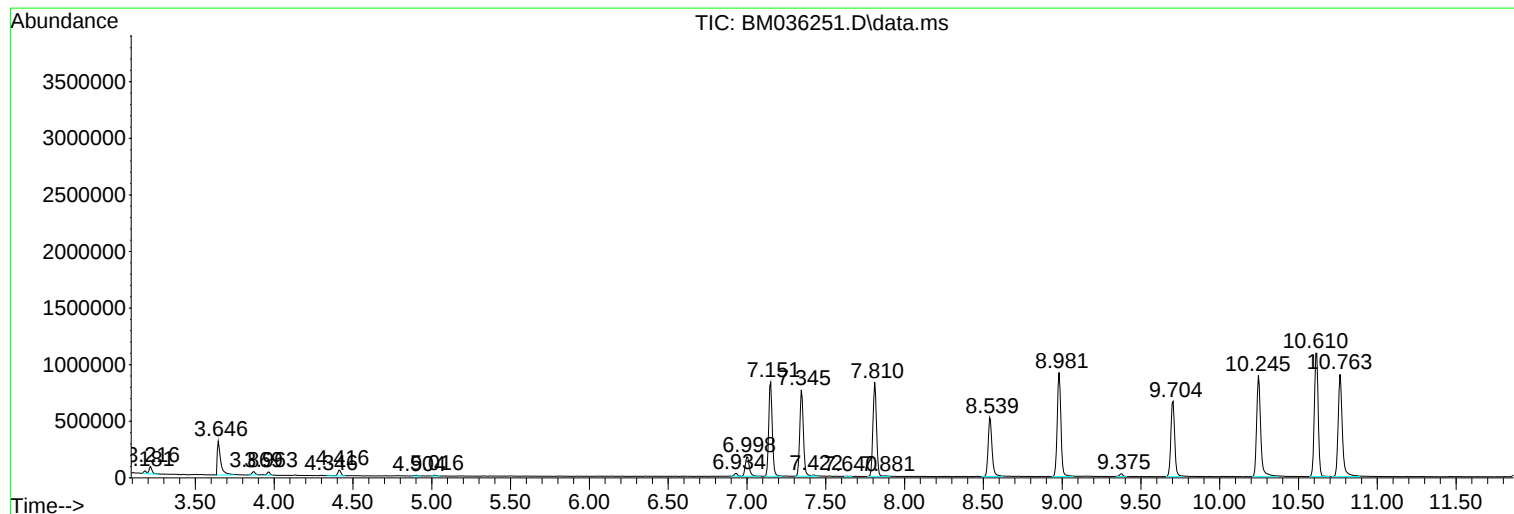

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036251.D
Acq On : 13 Aug 2022 04:23
Operator : CG/JU
Sample : N4165-04
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBX9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036251.D
Acq On : 13 Aug 2022 04:23
Operator : CG/JU
Sample : N4165-04
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBX9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc