

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036252.D
 Acq On : 13 Aug 2022 04:58
 Operator : CG/JU
 Sample : N4165-05
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGBY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036252.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	13	16	19	rBV2	14851	18472	0.32%	0.038%
2	3.216	19	22	28	rVB	62327	75937	1.32%	0.157%
3	3.646	93	95	111	rBV	251988	395560	6.88%	0.817%
4	3.869	128	133	139	rVB	27888	43200	0.75%	0.089%
5	3.963	146	149	154	rVB	19786	25910	0.45%	0.053%
6	4.410	221	225	232	rVB	48570	70652	1.23%	0.146%
7	4.898	305	308	311	rBV5	5299	6434	0.11%	0.013%
8	5.022	325	329	331	rBV4	6124	8207	0.14%	0.017%
9	5.504	408	411	417	rVB7	4360	6370	0.11%	0.013%
10	6.928	645	653	658	rBV	22922	35679	0.62%	0.074%
11	6.998	660	665	678	rVB	163060	284880	4.95%	0.588%
12	7.151	681	691	703	rBV	776288	1249897	21.73%	2.581%
13	7.345	717	724	735	rBV	715989	1145596	19.92%	2.365%
14	7.422	735	737	744	rVB5	9209	14255	0.25%	0.029%
15	7.810	794	803	812	rBV	776364	1232207	21.42%	2.544%
16	8.539	920	927	938	rBV	479965	836725	14.55%	1.728%
17	8.981	995	1002	1015	rBV	874777	1439634	25.03%	2.972%
18	9.375	1064	1069	1076	rVB2	21843	34811	0.61%	0.072%
19	9.704	1117	1125	1139	rBV	619964	1070138	18.61%	2.210%
20	10.245	1210	1217	1237	rBV	839887	1499712	26.08%	3.097%
21	10.610	1271	1279	1292	rBV	1045160	1743214	30.31%	3.599%
22	10.763	1295	1305	1324	rBV	852022	1596009	27.75%	3.295%
23	11.869	1487	1493	1500	rVB2	13092	22683	0.39%	0.047%
24	12.216	1546	1552	1559	rVB4	12768	27081	0.47%	0.056%
25	13.363	1741	1747	1751	rBV6	7127	12957	0.23%	0.027%
26	13.874	1825	1834	1846	rBV	1657617	2253297	39.18%	4.652%
27	14.151	1872	1881	1897	rBV	1999043	2960135	51.47%	6.112%
28	14.457	1925	1933	1943	rBV	1402594	2092999	36.39%	4.322%
29	14.704	1969	1975	1988	rBV2	54588	162924	2.83%	0.336%
30	15.039	2026	2032	2035	rBV8	3628	6640	0.12%	0.014%
31	15.251	2063	2068	2071	rBV6	4462	9504	0.17%	0.020%
32	15.280	2071	2073	2080	rVB4	5731	8936	0.16%	0.018%
33	15.445	2092	2101	2115	rBV	2614700	3703707	64.40%	7.647%
34	15.574	2117	2123	2139	rVV	624118	958339	16.66%	1.979%
35	15.686	2139	2142	2148	rVB3	14153	22910	0.40%	0.047%
36	16.168	2220	2224	2227	rBV6	4313	7485	0.13%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036252.D
 Acq On : 13 Aug 2022 04:58
 Operator : CG/JU
 Sample : N4165-05
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGBY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	16.333	2247	2252	2257	rVB8	2874	6131	0.11%	0.013%
38	16.662	2305	2308	2313	rVB2	9776	10778	0.19%	0.022%
39	16.962	2354	2359	2361	rBV4	7632	11282	0.20%	0.023%
40	17.127	2381	2387	2391	rBV8	3257	7780	0.14%	0.016%
41	17.198	2393	2399	2408	rVV	1709106	2349213	40.85%	4.851%
42	17.298	2409	2416	2431	rVB	2989417	4139370	71.97%	8.547%
43	17.486	2446	2448	2453	rBV6	4904	7244	0.13%	0.015%
44	17.698	2480	2484	2485	rBV4	4803	6158	0.11%	0.013%
45	17.733	2487	2490	2494	rVB4	8463	9438	0.16%	0.019%
46	17.868	2510	2513	2519	rVB6	8235	13157	0.23%	0.027%
47	18.109	2549	2554	2557	rBV7	5294	10291	0.18%	0.021%
48	18.174	2561	2565	2570	rVV2	7307	11349	0.20%	0.023%
49	18.674	2648	2650	2654	rVB3	10577	12476	0.22%	0.026%
50	19.156	2728	2732	2736	rBV3	31665	43646	0.76%	0.090%
51	19.227	2740	2744	2750	rBV	35981	52521	0.91%	0.108%
52	19.592	2800	2806	2814	rBV	3595262	4866221	84.61%	10.048%
53	20.592	2973	2976	2980	rVB2	57596	63164	1.10%	0.130%
54	21.380	3105	3110	3119	rBV	2255762	2871233	49.92%	5.928%
55	23.562	3474	3481	3494	rBV2	2930538	5751264	100.00%	11.875%
56	23.715	3501	3507	3519	rVB2	1581093	3106293	54.01%	6.414%




Sum of corrected areas: 48432105

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036252.D
Acq On : 13 Aug 2022 04:58
Operator : CG/JU
Sample : N4165-05
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBY0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

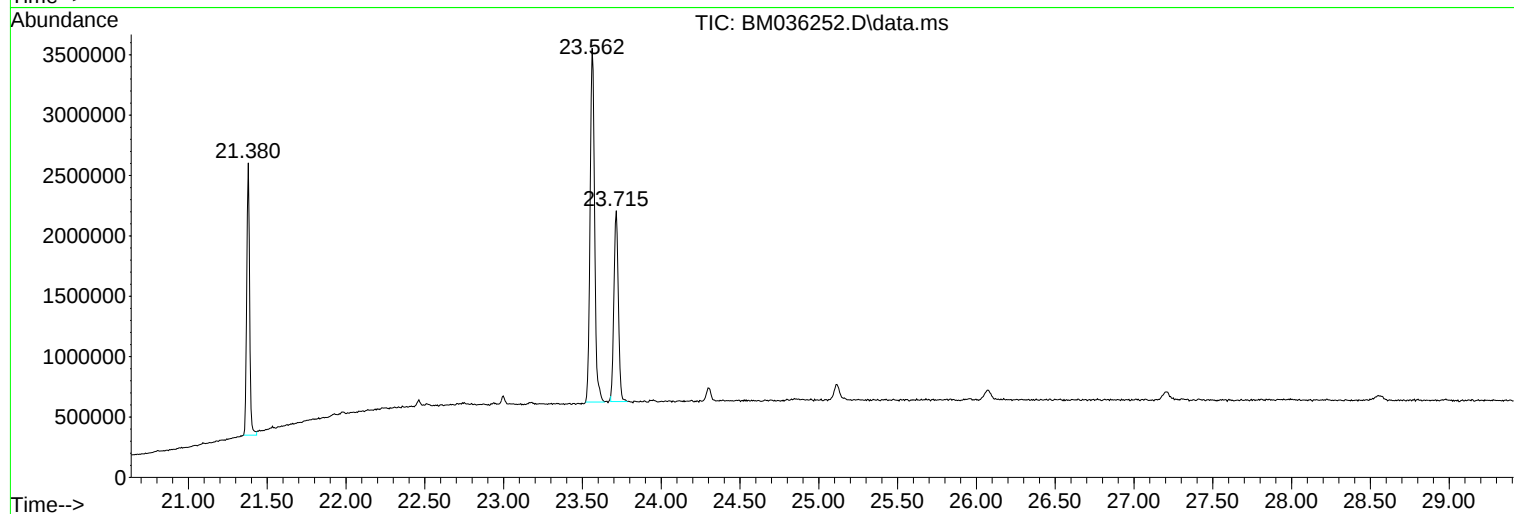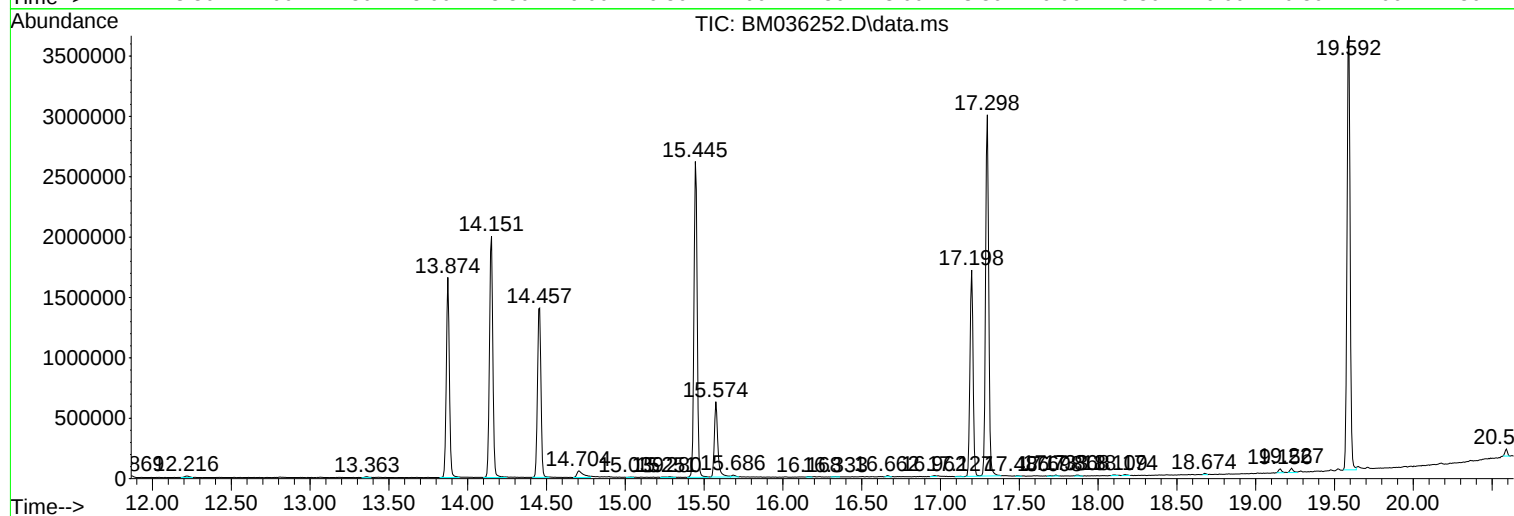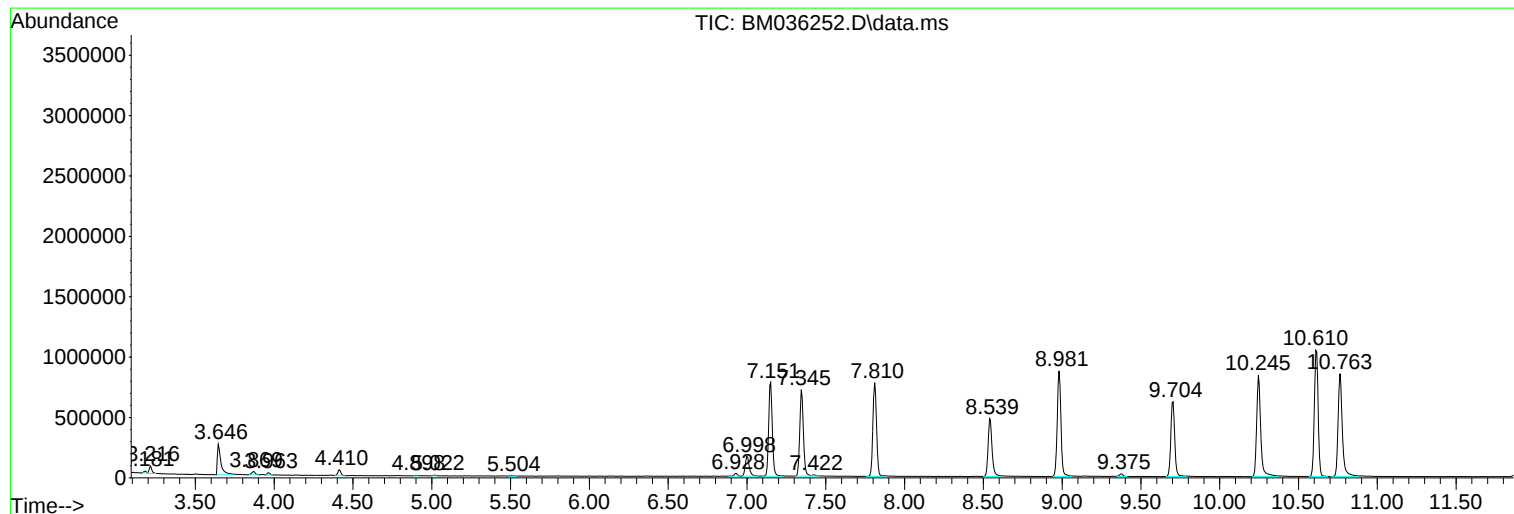

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036252.D
Acq On : 13 Aug 2022 04:58
Operator : CG/JU
Sample : N4165-05
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBY0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036252.D
Acq On : 13 Aug 2022 04:58
Operator : CG/JU
Sample : N4165-05
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBY0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc