

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036253.D
 Acq On : 13 Aug 2022 05:34
 Operator : CG/JU
 Sample : N4165-10
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGBY7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036253.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	18	22	30	rVB	44237	61218	1.16%	0.156%
2	3.646	93	95	111	rBV	168959	283495	5.38%	0.723%
3	3.869	129	133	137	rVB	20469	28734	0.55%	0.073%
4	3.963	146	149	157	rVB	16984	23146	0.44%	0.059%
5	4.410	221	225	232	rBV	38246	54084	1.03%	0.138%
6	5.016	324	328	333	rBV7	5898	11230	0.21%	0.029%
7	6.928	649	653	658	rBV	19681	27168	0.52%	0.069%
8	6.998	660	665	678	rVB	125106	227134	4.31%	0.579%
9	7.146	683	690	704	rBV	577852	939466	17.82%	2.395%
10	7.346	717	724	734	rBV	541598	872173	16.55%	2.223%
11	7.422	734	737	743	rVB6	6756	12262	0.23%	0.031%
12	7.810	795	803	811	rBV	621183	974229	18.48%	2.483%
13	7.881	812	815	820	rVB7	6911	11249	0.21%	0.029%
14	8.540	921	927	942	rBV	354362	628547	11.93%	1.602%
15	8.981	994	1002	1014	rBV	646322	1070272	20.31%	2.728%
16	9.369	1064	1068	1077	rVB2	17613	31575	0.60%	0.080%
17	9.698	1116	1124	1135	rBV	453155	783137	14.86%	1.996%
18	10.245	1210	1217	1237	rBV	605034	1121045	21.27%	2.858%
19	10.610	1271	1279	1287	rBV	811109	1344537	25.51%	3.427%
20	10.763	1298	1305	1324	rBV	547038	1068674	20.28%	2.724%
21	11.298	1390	1396	1405	rVB	2641	8012	0.15%	0.020%
22	11.869	1489	1493	1501	rBV2	10565	16642	0.32%	0.042%
23	12.216	1544	1552	1561	rVB2	10088	26418	0.50%	0.067%
24	12.822	1648	1655	1658	rBV9	4759	8784	0.17%	0.022%
25	13.075	1691	1698	1699	rBV7	4797	7310	0.14%	0.019%
26	13.875	1827	1834	1846	rBV	1200222	1716393	32.57%	4.375%
27	14.145	1873	1880	1895	rBV	1479722	2196479	41.67%	5.599%
28	14.451	1925	1932	1945	rBV	1097683	1623249	30.80%	4.138%
29	14.704	1969	1975	1986	rBV2	49674	140392	2.66%	0.358%
30	15.245	2063	2067	2070	rBV4	5743	6473	0.12%	0.017%
31	15.286	2070	2074	2082	rVB8	5815	11305	0.21%	0.029%
32	15.445	2089	2101	2117	rBV	2010769	2840414	53.89%	7.240%
33	15.574	2117	2123	2138	rVV	509807	789606	14.98%	2.013%
34	15.686	2140	2142	2149	rVB7	12247	16897	0.32%	0.043%
35	16.163	2219	2223	2225	rBV5	5637	8526	0.16%	0.022%
36	16.504	2277	2281	2287	rBV9	3595	6996	0.13%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036253.D
 Acq On : 13 Aug 2022 05:34
 Operator : CG/JU
 Sample : N4165-10
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGBY7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	16.663	2305	2308	2317	rVB7	9436	15885	0.30%	0.040%
38	16.739	2317	2321	2323	rBV5	4218	5289	0.10%	0.013%
39	16.957	2353	2358	2361	rBV5	7849	12030	0.23%	0.031%
40	17.198	2392	2399	2407	rVV	1374328	1901906	36.09%	4.848%
41	17.298	2409	2416	2432	rVB	2276261	3334810	63.27%	8.501%
42	17.533	2451	2456	2462	rBV3	10352	18020	0.34%	0.046%
43	17.733	2486	2490	2494	rVV4	7450	11057	0.21%	0.028%
44	18.098	2547	2552	2556	rBV3	22372	34642	0.66%	0.088%
45	18.168	2561	2564	2568	rVV	9130	11443	0.22%	0.029%
46	19.157	2728	2732	2736	rBV3	26854	36955	0.70%	0.094%
47	19.227	2740	2744	2751	rVB	27103	44989	0.85%	0.115%
48	19.586	2800	2805	2813	rBV	3135421	4197593	79.64%	10.700%
49	20.586	2972	2975	2981	rBV2	71248	82239	1.56%	0.210%
50	21.380	3105	3110	3119	rBV	1893316	2500586	47.44%	6.374%
51	23.562	3474	3481	3498	rVB2	2694010	5270521	100.00%	13.435%
52	23.715	3501	3507	3517	rVB2	1406950	2754969	52.27%	7.023%




Sum of corrected areas: 39230205

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036253.D
Acq On : 13 Aug 2022 05:34
Operator : CG/JU
Sample : N4165-10
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBY7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

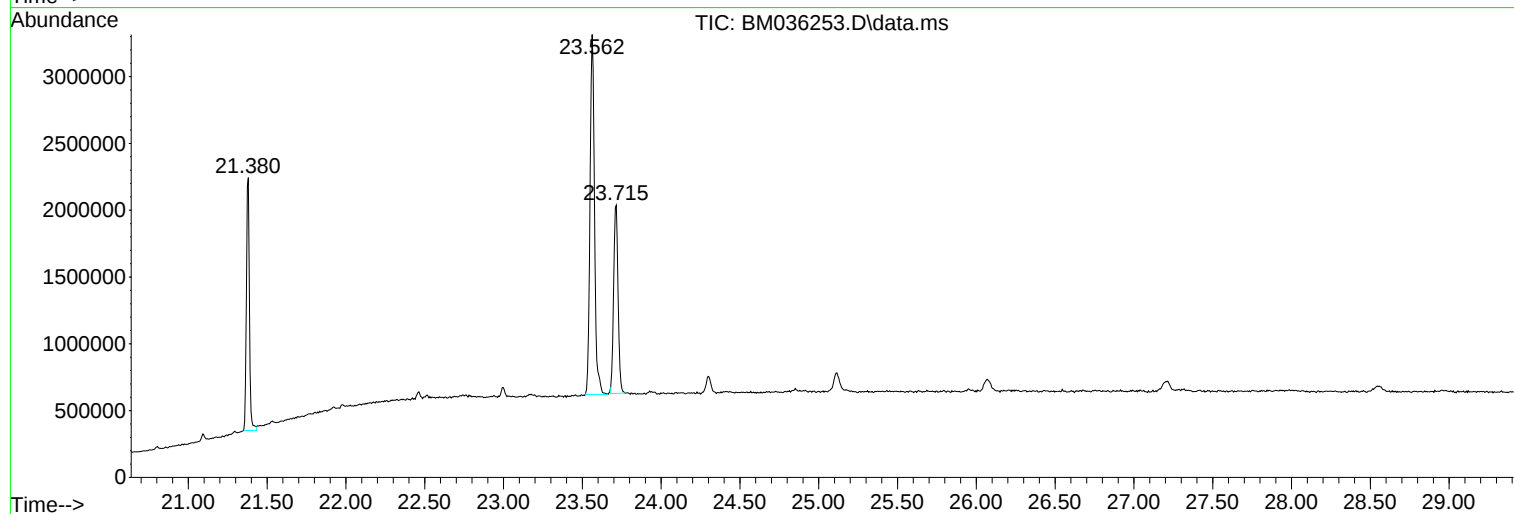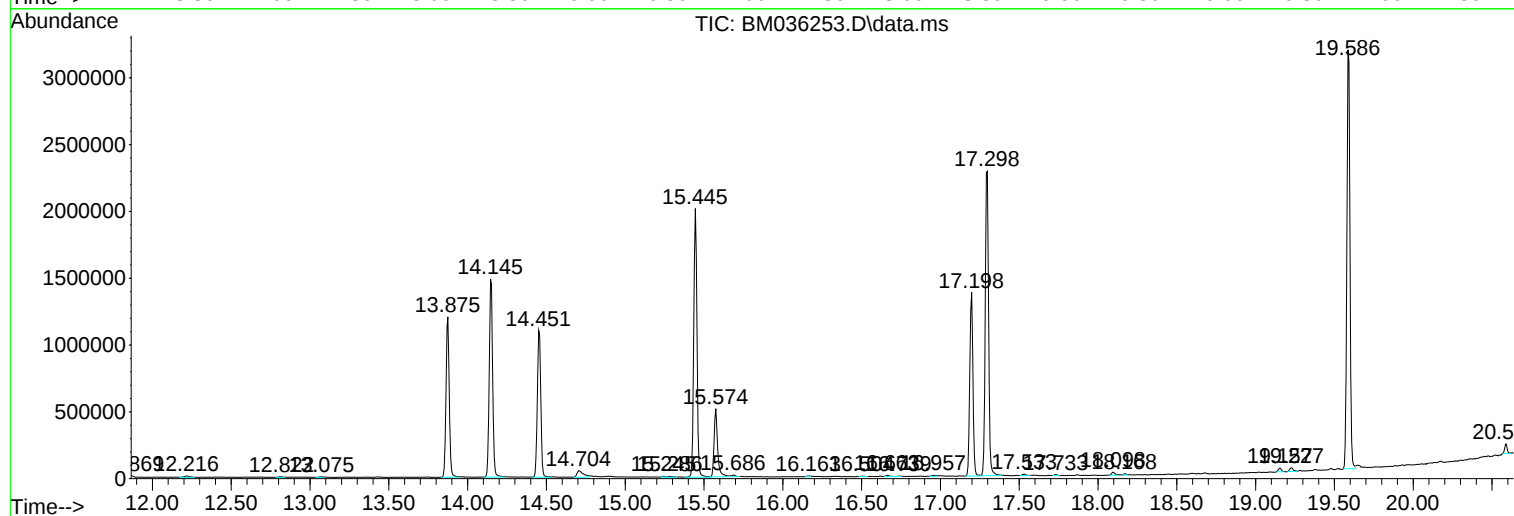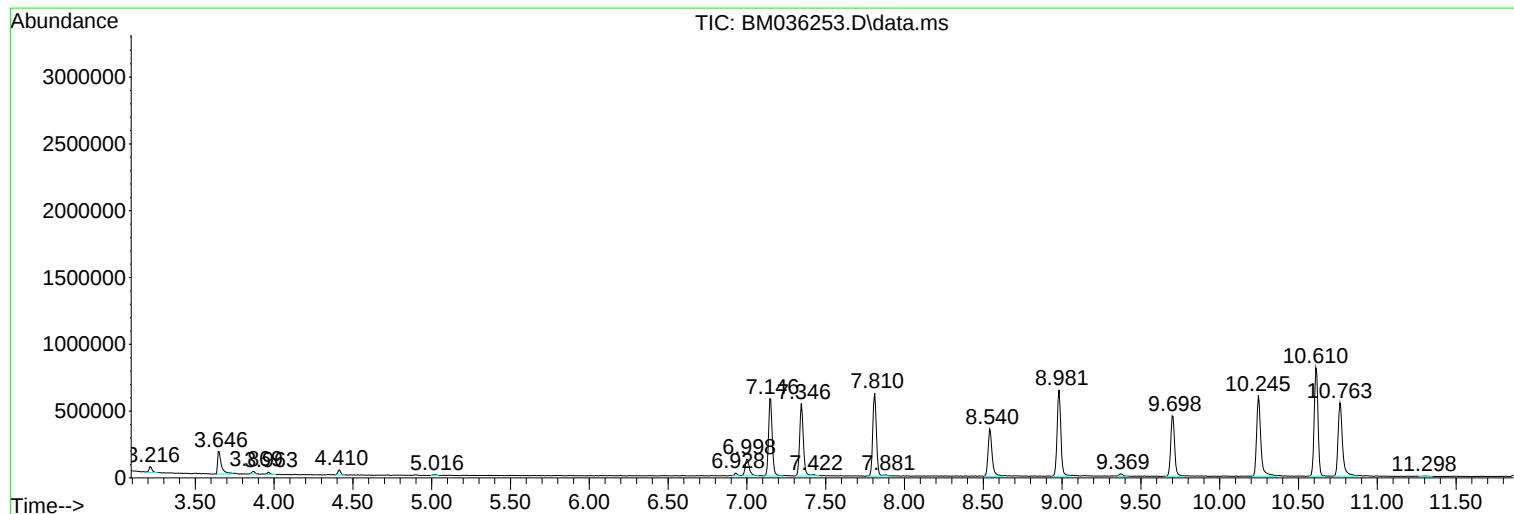

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036253.D
Acq On : 13 Aug 2022 05:34
Operator : CG/JU
Sample : N4165-10
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBY7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036253.D
Acq On : 13 Aug 2022 05:34
Operator : CG/JU
Sample : N4165-10
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBY7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------