

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036260.D
 Acq On : 13 Aug 2022 10:21
 Operator : CG/JU
 Sample : N4165-09
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGBY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036260.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	18	22	27	rVB	47588	58734	0.89%	0.111%
2	3.646	93	95	109	rBV	215049	339532	5.16%	0.643%
3	3.869	128	133	139	rBV	25987	40409	0.61%	0.077%
4	3.963	145	149	153	rVB	16536	22727	0.35%	0.043%
5	4.410	221	225	232	rVB	44222	59006	0.90%	0.112%
6	4.898	305	308	313	rVB3	5192	7339	0.11%	0.014%
7	5.016	325	328	334	rVB5	6832	11415	0.17%	0.022%
8	6.928	649	653	659	rVB	22129	32418	0.49%	0.061%
9	6.998	659	665	679	rBV	164494	287832	4.38%	0.545%
10	7.145	684	690	704	rVB	804638	1253560	19.06%	2.375%
11	7.345	716	724	734	rBV	713477	1149643	17.48%	2.178%
12	7.810	795	803	812	rBV	735370	1154057	17.55%	2.186%
13	8.539	920	927	938	rBV	496849	842521	12.81%	1.596%
14	8.981	994	1002	1015	rBV	885218	1499132	22.79%	2.840%
15	9.133	1026	1028	1033	rVB6	4281	6786	0.10%	0.013%
16	9.375	1064	1069	1077	rVB	22921	37429	0.57%	0.071%
17	9.698	1114	1124	1136	rBV	663225	1124301	17.09%	2.130%
18	10.028	1172	1180	1183	rBV8	5711	15088	0.23%	0.029%
19	10.245	1209	1217	1232	rBV	861809	1569440	23.86%	2.973%
20	10.610	1271	1279	1287	rBV	1023705	1658388	25.22%	3.142%
21	10.763	1297	1305	1322	rBV	830513	1582853	24.07%	2.999%
22	11.869	1488	1493	1497	rBV2	13258	21381	0.33%	0.041%
23	12.210	1542	1551	1561	rBV2	14039	31532	0.48%	0.060%
24	13.357	1739	1746	1752	rBV6	8256	14340	0.22%	0.027%
25	13.874	1827	1834	1846	rBV	1834228	2599960	39.53%	4.926%
26	14.145	1870	1880	1896	rBV	2289972	3291117	50.04%	6.235%
27	14.451	1923	1932	1945	rBV	1490651	2136706	32.49%	4.048%
28	14.698	1967	1974	1993	rBV2	67366	211404	3.21%	0.401%
29	14.892	2000	2007	2014	rVB8	13976	25253	0.38%	0.048%
30	15.245	2063	2067	2070	rBV5	4191	7385	0.11%	0.014%
31	15.280	2070	2073	2081	rVB5	7195	12946	0.20%	0.025%
32	15.445	2092	2101	2117	rBV	3007995	4261587	64.80%	8.074%
33	15.574	2117	2123	2138	rVV	762550	1155563	17.57%	2.189%
34	15.686	2138	2142	2148	rVB3	15675	29980	0.46%	0.057%
35	16.174	2219	2225	2228	rBV7	12139	21421	0.33%	0.041%
36	16.221	2229	2233	2238	rVB2	11632	18645	0.28%	0.035%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036260.D
 Acq On : 13 Aug 2022 10:21
 Operator : CG/JU
 Sample : N4165-09
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGBY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	16.657	2304	2307	2312	rVB3	11273	16667	0.25%	0.032%
38	17.198	2392	2399	2409	rBV	1692810	2444707	37.17%	4.632%
39	17.292	2409	2415	2430	rVV	3523322	4941405	75.13%	9.362%
40	17.404	2432	2434	2440	rVB7	9500	13492	0.21%	0.026%
41	17.733	2487	2490	2496	rVB5	9709	12351	0.19%	0.023%
42	17.868	2510	2513	2518	rBV7	5663	8943	0.14%	0.017%
43	18.098	2547	2552	2558	rBV9	17617	31757	0.48%	0.060%
44	18.168	2560	2564	2569	rVV	12668	16973	0.26%	0.032%
45	18.674	2648	2650	2655	rVB4	7941	10055	0.15%	0.019%
46	19.150	2727	2731	2736	rBV4	41734	60681	0.92%	0.115%
47	19.227	2739	2744	2748	rBV	44575	64984	0.99%	0.123%
48	19.586	2799	2805	2812	rBV	4310838	5806503	88.29%	11.000%
49	20.586	2972	2975	2980	rVB	70778	66295	1.01%	0.126%
50	21.374	3104	3109	3118	rBV	2247019	2986739	45.41%	5.658%
51	23.562	3474	3481	3495	rVB2	3386537	6576966	100.00%	12.460%
52	23.709	3500	3506	3518	rVB2	1599150	3133780	47.65%	5.937%




Sum of corrected areas: 52784128

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036260.D
Acq On : 13 Aug 2022 10:21
Operator : CG/JU
Sample : N4165-09
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBY2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

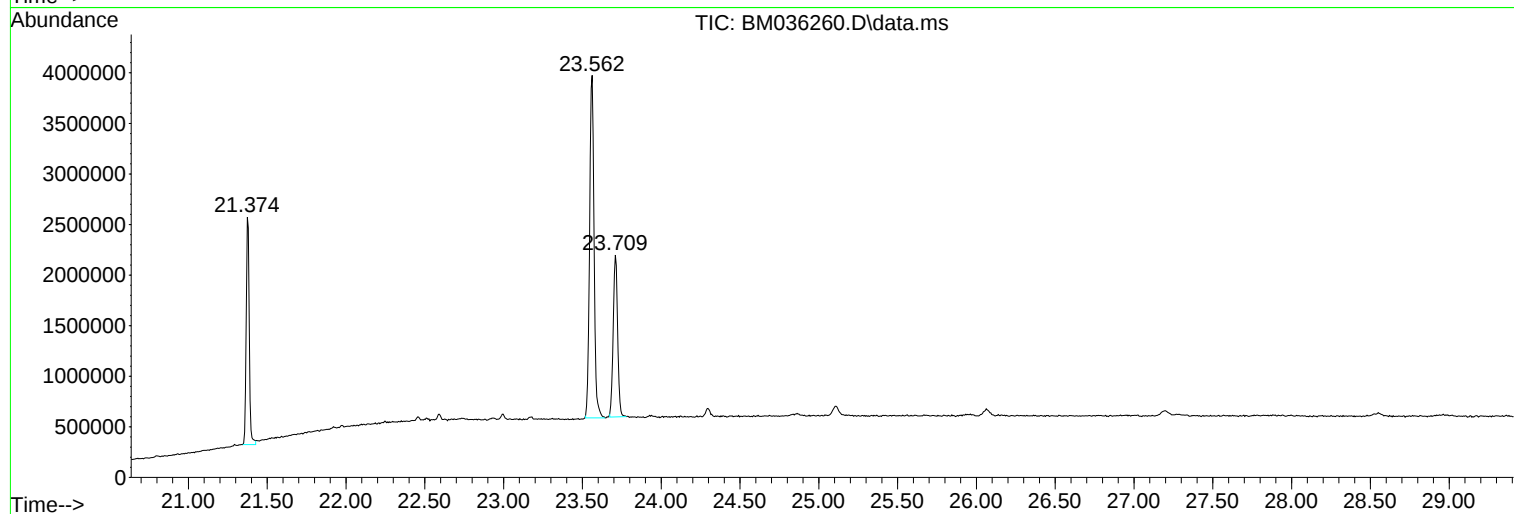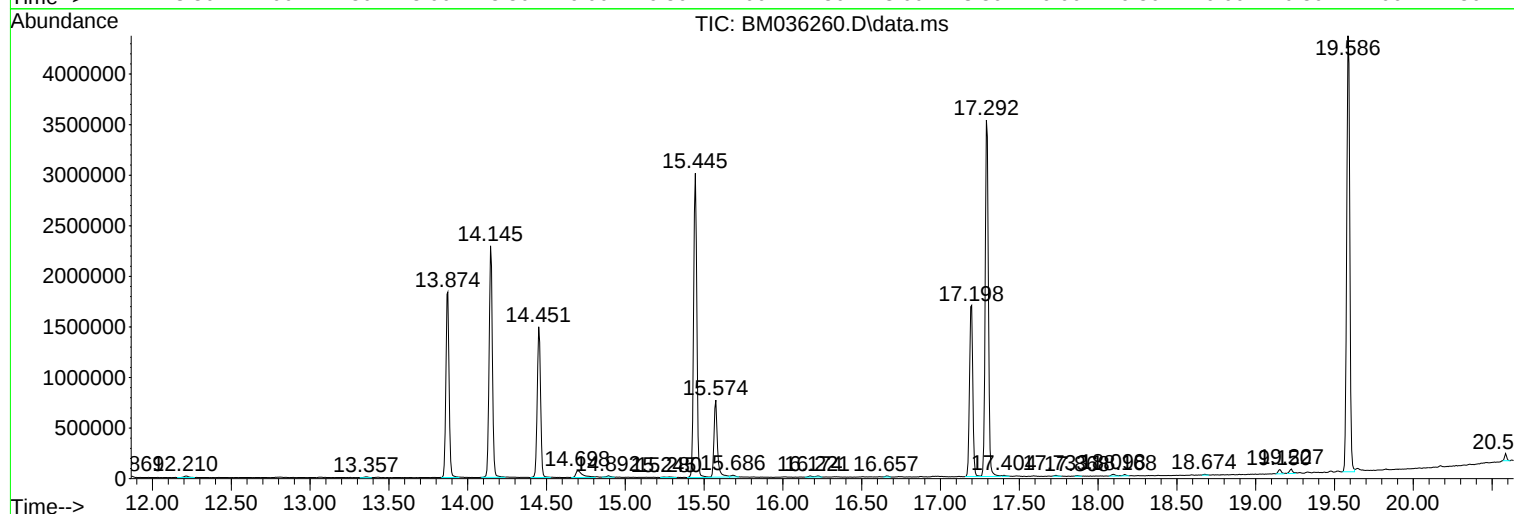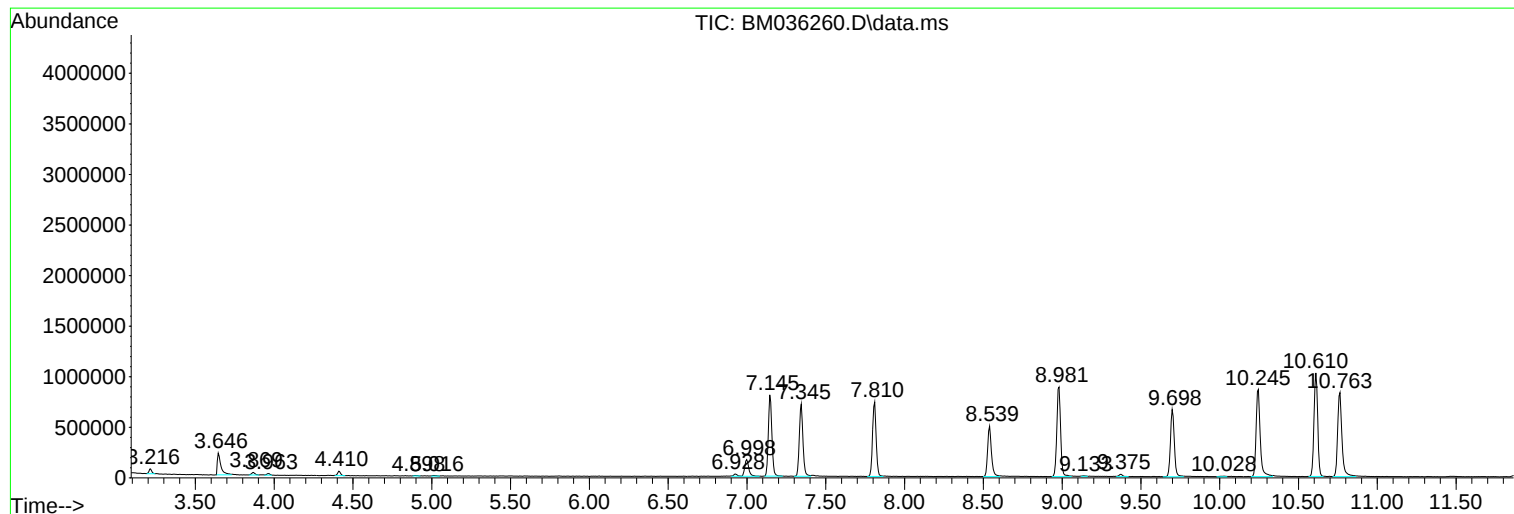

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036260.D
Acq On : 13 Aug 2022 10:21
Operator : CG/JU
Sample : N4165-09
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBY2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036260.D
Acq On : 13 Aug 2022 10:21
Operator : CG/JU
Sample : N4165-09
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBY2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc