

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036261.D
 Acq On : 13 Aug 2022 10:57
 Operator : CG/JU
 Sample : N4165-08
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGBY1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036261.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	12	16	19	rBV3	17715	22677	0.33%	0.040%
2	3.216	19	22	27	rVB	55018	63121	0.92%	0.111%
3	3.646	93	95	111	rBV	283095	426842	6.19%	0.748%
4	3.869	128	133	139	rBV	29389	44728	0.65%	0.078%
5	3.963	145	149	155	rVB	21236	27388	0.40%	0.048%
6	4.410	220	225	230	rVB	52923	69214	1.00%	0.121%
7	5.022	325	329	335	rVB6	8257	12268	0.18%	0.021%
8	6.928	648	653	658	rBV2	26913	40116	0.58%	0.070%
9	6.998	659	665	675	rVB	182399	315855	4.58%	0.553%
10	7.145	684	690	704	rVB	815458	1267268	18.38%	2.220%
11	7.345	717	724	734	rBV	732742	1187477	17.22%	2.080%
12	7.422	734	737	745	rVB3	11414	19149	0.28%	0.034%
13	7.810	796	803	812	rBV	846049	1336999	19.39%	2.342%
14	8.539	920	927	947	rBV	548016	940507	13.64%	1.647%
15	8.975	994	1001	1017	rBV	875825	1498684	21.73%	2.625%
16	9.369	1063	1068	1073	rBV2	24898	36325	0.53%	0.064%
17	9.698	1117	1124	1140	rBV	678411	1140526	16.54%	1.998%
18	10.245	1208	1217	1234	rBV	896914	1634094	23.70%	2.862%
19	10.610	1269	1279	1291	rBV	1215149	1978652	28.69%	3.466%
20	10.763	1297	1305	1323	rBV	933835	1744947	25.30%	3.056%
21	11.869	1488	1493	1500	rVB2	17095	27611	0.40%	0.048%
22	12.216	1547	1552	1558	rBV	14924	26913	0.39%	0.047%
23	13.363	1741	1747	1751	rVB9	4522	8201	0.12%	0.014%
24	13.433	1754	1759	1763	rBV4	5126	8611	0.12%	0.015%
25	13.874	1826	1834	1846	rBV	1815947	2611446	37.87%	4.574%
26	14.145	1872	1880	1893	rBV	2327807	3316051	48.09%	5.808%
27	14.451	1925	1932	1941	rBV	1838700	2522384	36.58%	4.418%
28	14.698	1968	1974	1993	rBV2	91517	273711	3.97%	0.479%
29	14.898	2005	2008	2016	rVB8	6527	12040	0.17%	0.021%
30	15.280	2069	2073	2077	rVB4	5111	7615	0.11%	0.013%
31	15.445	2091	2101	2114	rBV	3118999	4313298	62.55%	7.555%
32	15.574	2117	2123	2137	rVV	824350	1269339	18.41%	2.223%
33	15.680	2138	2141	2151	rVB4	19357	40265	0.58%	0.071%
34	16.180	2220	2226	2230	rVV9	3500	8580	0.12%	0.015%
35	16.233	2230	2235	2239	rVB6	5237	8679	0.13%	0.015%
36	16.662	2304	2308	2315	rVB2	12718	18966	0.28%	0.033%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036261.D
 Acq On : 13 Aug 2022 10:57
 Operator : CG/JU
 Sample : N4165-08
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGBY1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	16.957	2353	2358	2360	rBV6	9365	15036	0.22%	0.026%
38	17.192	2392	2398	2408	rBV	2136295	3002823	43.55%	5.260%
39	17.292	2409	2415	2426	rVV	3650555	5129675	74.39%	8.985%
40	17.727	2486	2489	2496	rVB2	9436	14186	0.21%	0.025%
41	17.868	2509	2513	2517	rBV7	5141	9065	0.13%	0.016%
42	18.098	2548	2552	2557	rBV7	11561	18733	0.27%	0.033%
43	18.168	2560	2564	2569	rVB	13390	21193	0.31%	0.037%
44	18.674	2648	2650	2656	rVB4	8761	11006	0.16%	0.019%
45	19.151	2727	2731	2739	rBV	42979	58264	0.84%	0.102%
46	19.227	2739	2744	2747	rBV	45616	64958	0.94%	0.114%
47	19.586	2799	2805	2813	rBV	4729252	6189616	89.76%	10.842%
48	20.586	2973	2975	2979	rVB2	65176	69621	1.01%	0.122%
49	21.374	3105	3109	3117	rBV	2743846	3526490	51.14%	6.177%
50	23.562	3474	3481	3498	rVB2	3644575	6895834	100.00%	12.079%
51	23.709	3500	3506	3517	rVB2	1887609	3782900	54.86%	6.626%




Sum of corrected areas: 57089947

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036261.D
Acq On : 13 Aug 2022 10:57
Operator : CG/JU
Sample : N4165-08
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBY1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

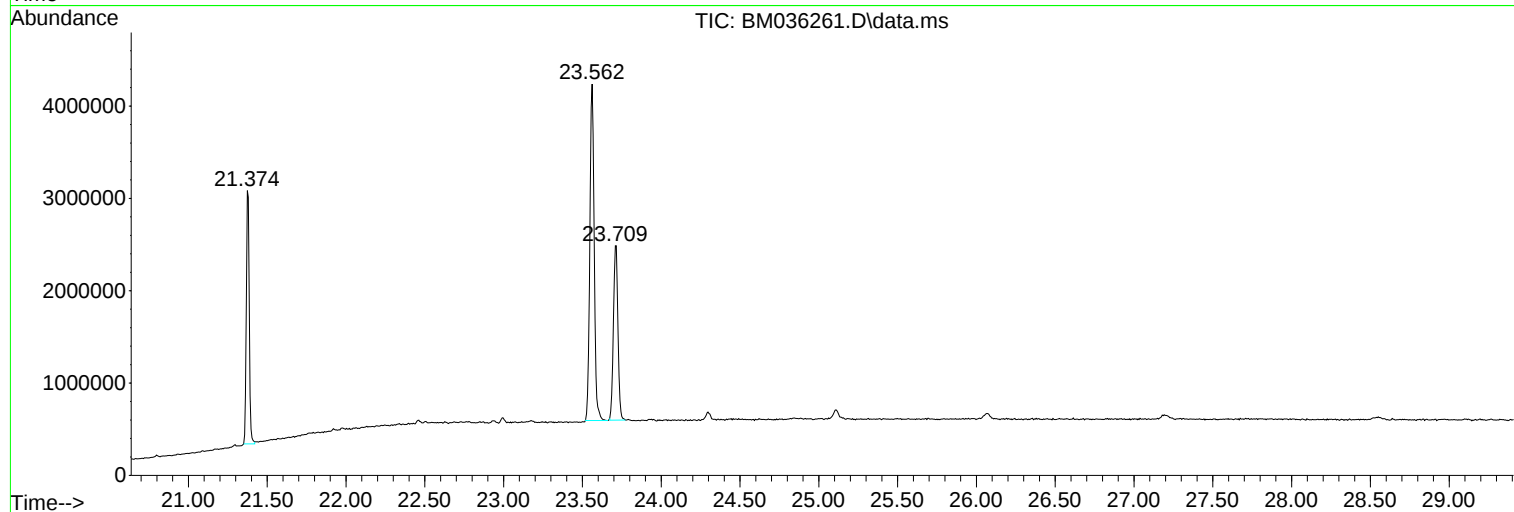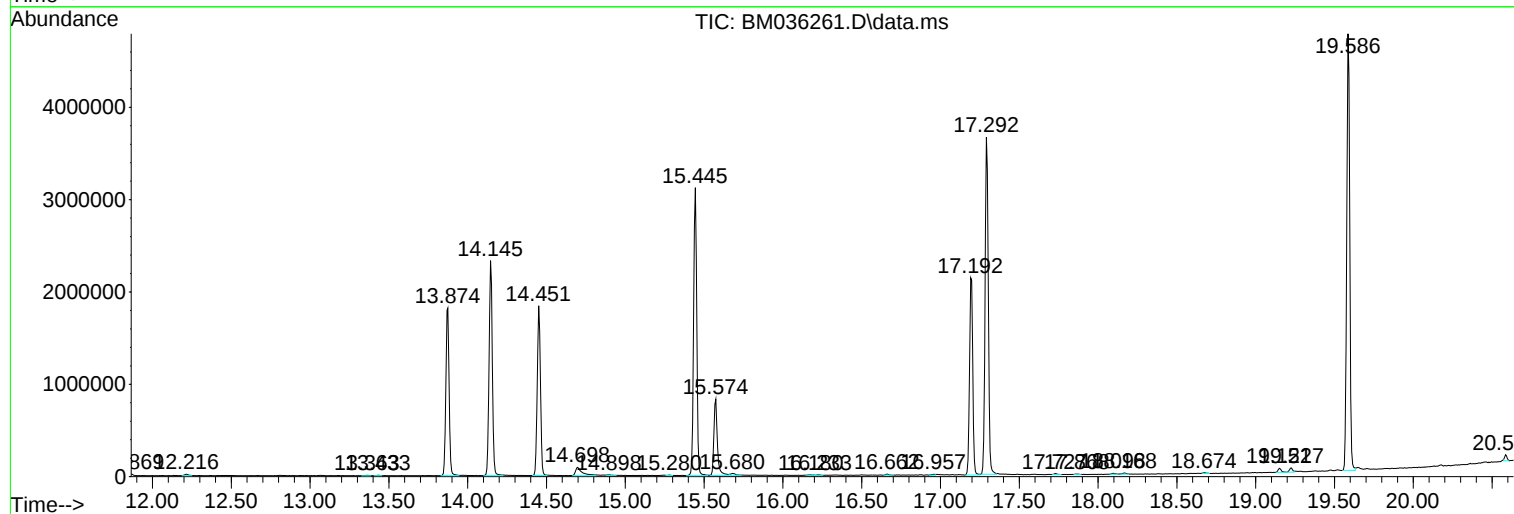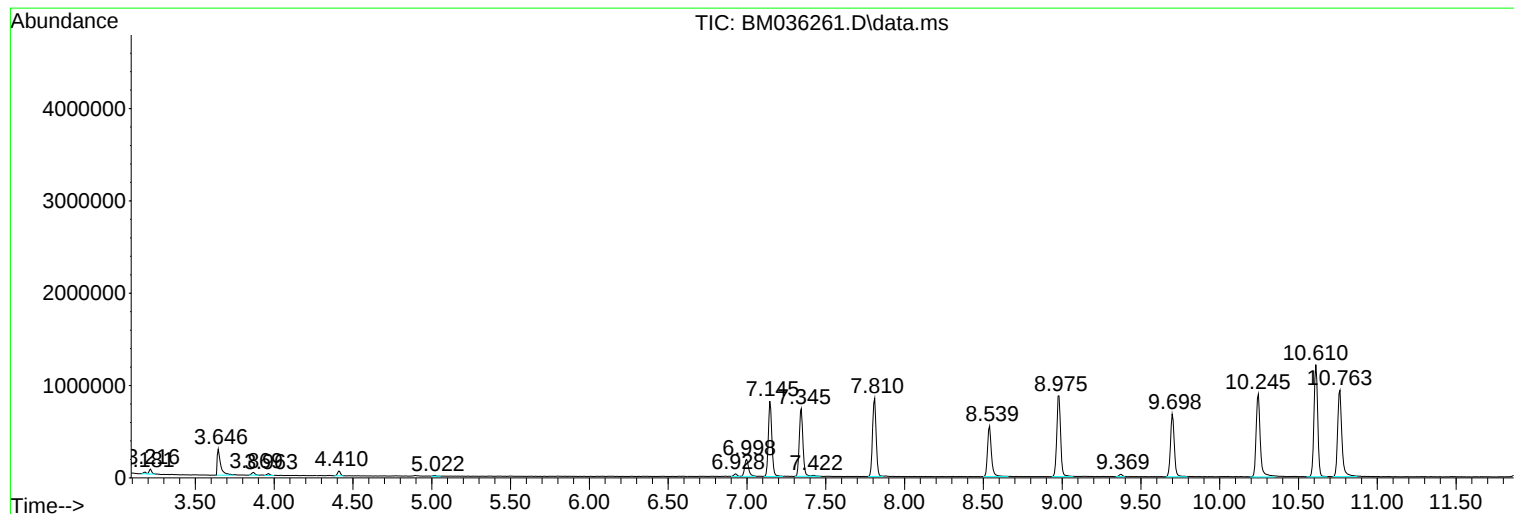

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036261.D
Acq On : 13 Aug 2022 10:57
Operator : CG/JU
Sample : N4165-08
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBY1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036261.D
Acq On : 13 Aug 2022 10:57
Operator : CG/JU
Sample : N4165-08
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBY1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------