

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036262.D
 Acq On : 13 Aug 2022 11:34
 Operator : CG/JU
 Sample : N4165-12
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGBY4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036262.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	18	22	30	rVB	56098	74852	0.99%	0.117%
2	3.646	92	95	109	rBV	291438	441723	5.83%	0.689%
3	3.869	128	133	137	rVB	30490	43784	0.58%	0.068%
4	3.963	145	149	155	rVB	21800	30422	0.40%	0.047%
5	4.410	220	225	232	rVB	59383	82055	1.08%	0.128%
6	5.016	326	328	333	rVB5	7676	10833	0.14%	0.017%
7	6.928	648	653	659	rBV	30816	38546	0.51%	0.060%
8	6.998	659	665	677	rBV	212639	363204	4.79%	0.567%
9	7.145	681	690	702	rBV	1018697	1568219	20.68%	2.446%
10	7.345	717	724	733	rBV	887284	1440557	19.00%	2.247%
11	7.422	734	737	741	rVB3	9821	13208	0.17%	0.021%
12	7.810	794	803	813	rBV	872570	1411637	18.62%	2.202%
13	8.539	920	927	944	rBV	639873	1102579	14.54%	1.720%
14	8.981	994	1002	1018	rBV	1091754	1849695	24.40%	2.885%
15	9.369	1064	1068	1073	rVB	26505	40569	0.54%	0.063%
16	9.698	1116	1124	1135	rBV	842216	1395645	18.41%	2.177%
17	10.239	1210	1216	1238	rBV	1103327	1995554	26.32%	3.113%
18	10.610	1271	1279	1288	rBV	1264079	2049175	27.03%	3.196%
19	10.757	1296	1304	1326	rBV	1144708	2161661	28.51%	3.372%
20	11.869	1487	1493	1498	rVB2	17014	27442	0.36%	0.043%
21	12.216	1545	1552	1563	rBV2	18659	41035	0.54%	0.064%
22	12.810	1648	1653	1658	rBV8	4710	9435	0.12%	0.015%
23	13.063	1692	1696	1702	rBV7	5879	12399	0.16%	0.019%
24	13.427	1753	1758	1764	rBV8	4442	8599	0.11%	0.013%
25	13.874	1825	1834	1848	rBV	2230343	3207037	42.30%	5.002%
26	14.145	1873	1880	1896	rBV	2815605	4073207	53.72%	6.353%
27	14.451	1926	1932	1941	rBV	1855748	2614298	34.48%	4.078%
28	14.698	1967	1974	1997	rBV2	87376	266814	3.52%	0.416%
29	15.251	2063	2068	2070	rBV4	5793	8663	0.11%	0.014%
30	15.280	2070	2073	2077	rVB3	6927	9780	0.13%	0.015%
31	15.445	2091	2101	2114	rBV	3678928	5171865	68.21%	8.067%
32	15.574	2117	2123	2138	rVV	887467	1377544	18.17%	2.149%
33	15.686	2138	2142	2151	rVB2	22379	42358	0.56%	0.066%
34	16.180	2220	2226	2232	rBV9	5847	14748	0.19%	0.023%
35	16.662	2303	2308	2315	rVB	15985	23534	0.31%	0.037%
36	16.951	2355	2357	2361	rBV5	6349	10439	0.14%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036262.D
 Acq On : 13 Aug 2022 11:34
 Operator : CG/JU
 Sample : N4165-12
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGBY4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	17.115	2382	2385	2392	rBV7	4717	8411	0.11%	0.013%
38	17.198	2392	2399	2406	rBV	2134284	3056394	40.31%	4.767%
39	17.292	2409	2415	2430	rVV	4234344	5841077	77.04%	9.111%
40	17.404	2430	2434	2440	rVB6	18601	31832	0.42%	0.050%
41	17.486	2445	2448	2455	rVB5	6532	11694	0.15%	0.018%
42	17.586	2463	2465	2476	rVB9	5793	13867	0.18%	0.022%
43	17.733	2485	2490	2496	rBV2	11774	18060	0.24%	0.028%
44	17.862	2509	2512	2516	rBV6	10056	13114	0.17%	0.020%
45	18.092	2547	2551	2560	rBV5	25052	48023	0.63%	0.075%
46	18.168	2560	2564	2569	rVV	15195	23586	0.31%	0.037%
47	18.674	2647	2650	2654	rVB3	10736	14390	0.19%	0.022%
48	19.151	2727	2731	2738	rBV3	50772	75705	1.00%	0.118%
49	19.227	2739	2744	2747	rBV	46896	63882	0.84%	0.100%
50	19.374	2766	2769	2773	rBV4	15373	20485	0.27%	0.032%
51	19.474	2784	2786	2791	rVB5	14310	10655	0.14%	0.017%
52	19.521	2791	2794	2799	rBV6	13001	20269	0.27%	0.032%
53	19.586	2799	2805	2813	rBV	5122600	6801919	89.71%	10.609%
54	20.586	2972	2975	2980	rVB	63271	68981	0.91%	0.108%
55	21.374	3105	3109	3118	rBV	2784236	3545017	46.76%	5.529%
56	23.562	3474	3481	3494	rVB2	4013548	7582021	100.00%	11.826%
57	23.709	3500	3506	3517	rVB2	1893654	3810547	50.26%	5.943%




Sum of corrected areas: 64113044

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036262.D
Acq On : 13 Aug 2022 11:34
Operator : CG/JU
Sample : N4165-12
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBY4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

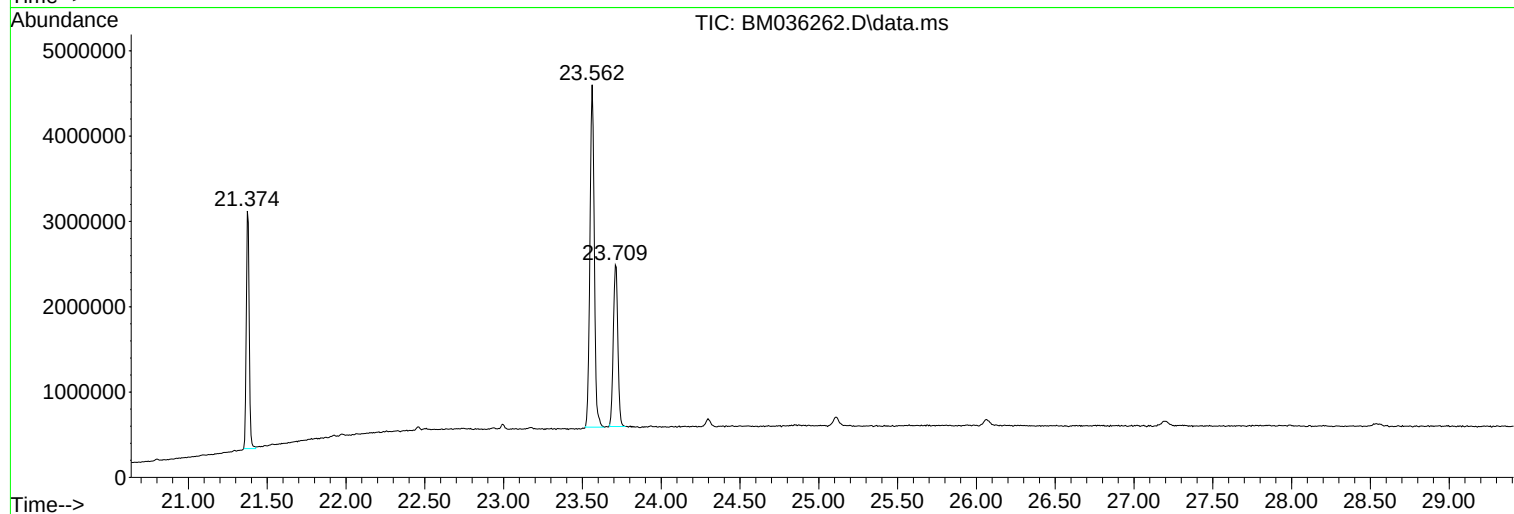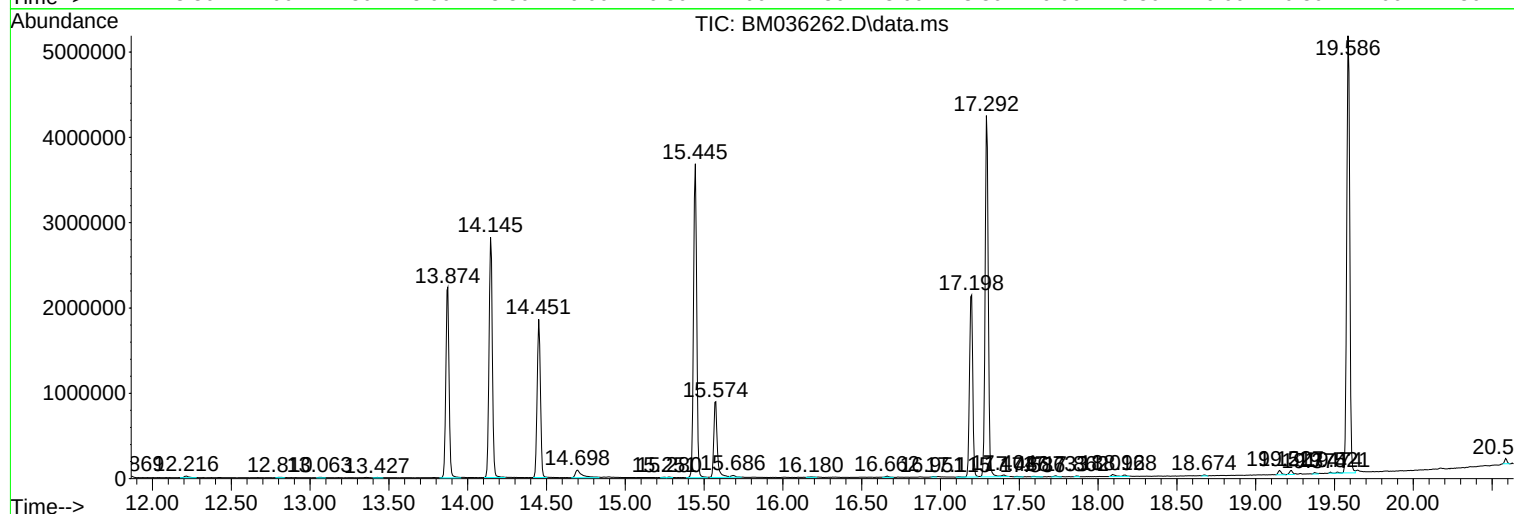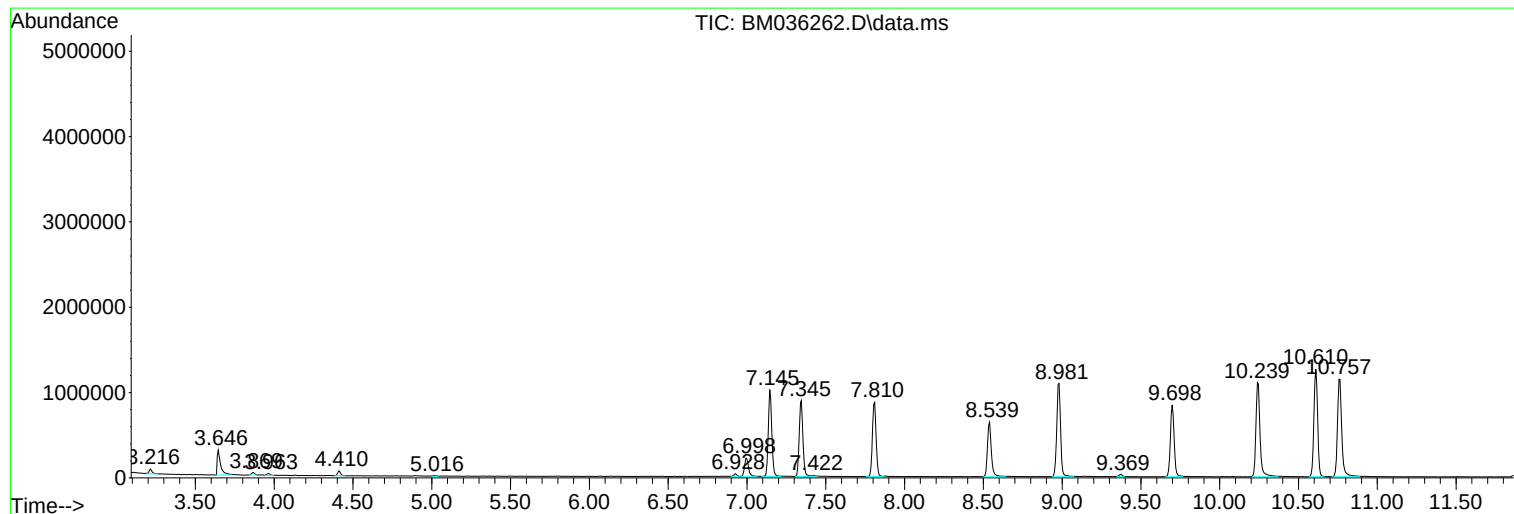

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036262.D
Acq On : 13 Aug 2022 11:34
Operator : CG/JU
Sample : N4165-12
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBY4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036262.D
Acq On : 13 Aug 2022 11:34
Operator : CG/JU
Sample : N4165-12
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBY4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc