

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036263.D
 Acq On : 13 Aug 2022 12:10
 Operator : CG/JU
 Sample : N4165-07
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGBZ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036263.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	18	22	27	rVB	46374	52657	0.81%	0.102%
2	3.646	92	95	119	rBV	262841	415901	6.40%	0.807%
3	3.869	128	133	141	rBV	27305	43796	0.67%	0.085%
4	3.963	145	149	153	rVB	20847	25983	0.40%	0.050%
5	4.410	220	225	233	rVB	50971	69713	1.07%	0.135%
6	5.016	324	328	331	rBV4	7714	10729	0.16%	0.021%
7	6.928	649	653	659	rVB	22710	33062	0.51%	0.064%
8	6.998	659	665	674	rBV	162047	285923	4.40%	0.555%
9	7.145	684	690	701	rBV	751723	1166413	17.94%	2.262%
10	7.345	717	724	734	rBV	659267	1087866	16.73%	2.110%
11	7.422	734	737	742	rVB6	7668	12869	0.20%	0.025%
12	7.810	796	803	811	rBV	772300	1235142	18.99%	2.396%
13	7.875	812	814	825	rVB10	7505	13575	0.21%	0.026%
14	8.022	833	839	846	rBV10	6886	11538	0.18%	0.022%
15	8.540	920	927	937	rBV	469018	804959	12.38%	1.561%
16	8.975	995	1001	1017	rBV	808655	1361966	20.94%	2.642%
17	9.145	1024	1030	1033	rBV7	4208	7598	0.12%	0.015%
18	9.369	1063	1068	1073	rVB	23610	38599	0.59%	0.075%
19	9.698	1117	1124	1136	rBV	600430	1002636	15.42%	1.945%
20	10.245	1210	1217	1237	rBV	773065	1449589	22.29%	2.812%
21	10.610	1270	1279	1293	rBV	1086901	1765189	27.14%	3.424%
22	10.763	1296	1305	1326	rBV	804891	1558280	23.96%	3.023%
23	11.869	1487	1493	1498	rVB	18039	26608	0.41%	0.052%
24	12.216	1547	1552	1558	rBV2	12373	24566	0.38%	0.048%
25	12.810	1644	1653	1659	rBV2	6253	15385	0.24%	0.030%
26	13.069	1693	1697	1702	rBV6	4826	7287	0.11%	0.014%
27	13.869	1825	1833	1847	rBV	1555728	2279395	35.05%	4.421%
28	14.145	1869	1880	1892	rBV	2000064	2906941	44.70%	5.638%
29	14.451	1925	1932	1944	rVV	1561715	2206931	33.94%	4.281%
30	14.698	1967	1974	1992	rBV2	73413	220794	3.40%	0.428%
31	15.286	2070	2074	2079	rVB5	5571	10826	0.17%	0.021%
32	15.445	2091	2101	2115	rBV	2613543	3741702	57.53%	7.258%
33	15.574	2117	2123	2138	rVV	674499	1043994	16.05%	2.025%
34	15.686	2138	2142	2153	rVB4	16376	34238	0.53%	0.066%
35	16.168	2219	2224	2231	rBV4	19347	45692	0.70%	0.089%
36	16.663	2304	2308	2311	rVB2	11023	12433	0.19%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
 Data File : BM036263.D
 Acq On : 13 Aug 2022 12:10
 Operator : CG/JU
 Sample : N4165-07
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGBZ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	16.957	2351	2358	2361	rBV6	10167	18525	0.28%	0.036%
38	17.115	2382	2385	2390	rBV7	4389	6991	0.11%	0.014%
39	17.192	2392	2398	2408	rBV	1816255	2623373	40.34%	5.088%
40	17.292	2409	2415	2429	rVV	3198564	4466358	68.68%	8.663%
41	17.733	2486	2490	2495	rVB4	8683	13218	0.20%	0.026%
42	17.862	2509	2512	2518	rVB7	10571	16181	0.25%	0.031%
43	18.092	2547	2551	2560	rBV5	26666	44899	0.69%	0.087%
44	18.168	2560	2564	2569	rVV	12327	17330	0.27%	0.034%
45	18.674	2647	2650	2653	rBV4	11176	12874	0.20%	0.025%
46	19.151	2727	2731	2737	rBV4	36509	58699	0.90%	0.114%
47	19.227	2739	2744	2751	rVV	35520	60465	0.93%	0.117%
48	19.586	2799	2805	2812	rBV	4121987	5461491	83.98%	10.593%
49	20.586	2972	2975	2979	rBV	68051	68301	1.05%	0.132%
50	21.092	3058	3061	3069	rBV	141940	205793	3.16%	0.399%
51	21.380	3104	3110	3119	rBV	2524325	3388723	52.11%	6.573%
52	23.562	3474	3481	3493	rVB2	3423710	6503367	100.00%	12.614%
53	23.709	3500	3506	3516	rVB2	1838496	3558547	54.72%	6.902%




Sum of corrected areas: 51555910

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036263.D
Acq On : 13 Aug 2022 12:10
Operator : CG/JU
Sample : N4165-07
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBZ5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

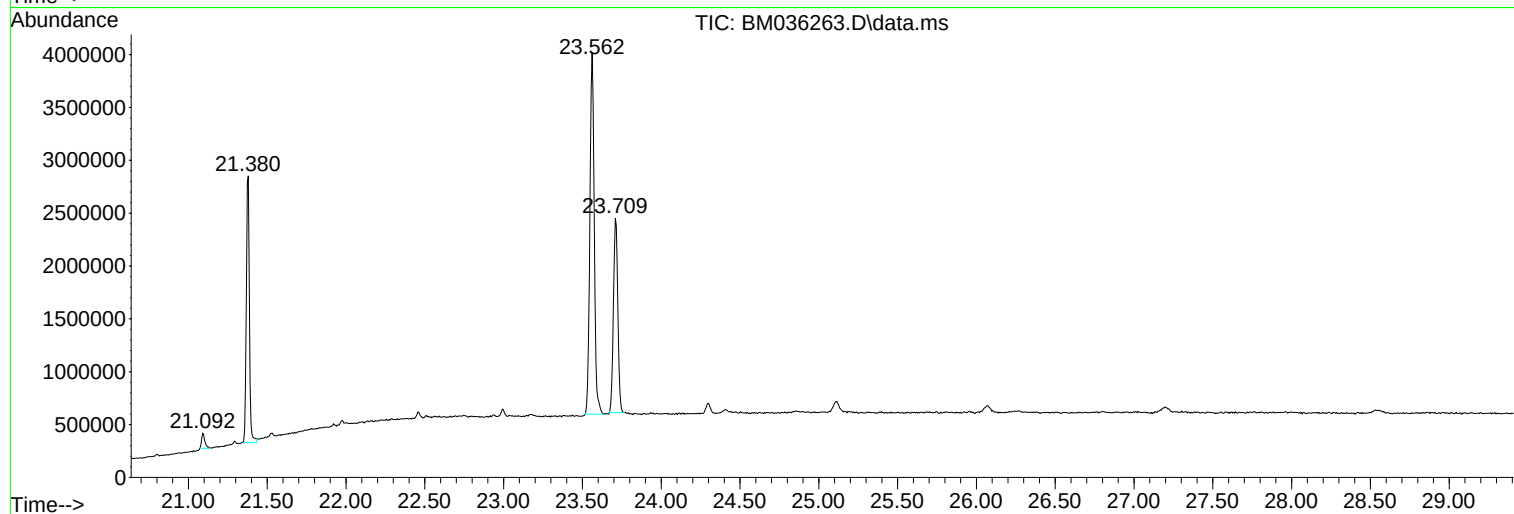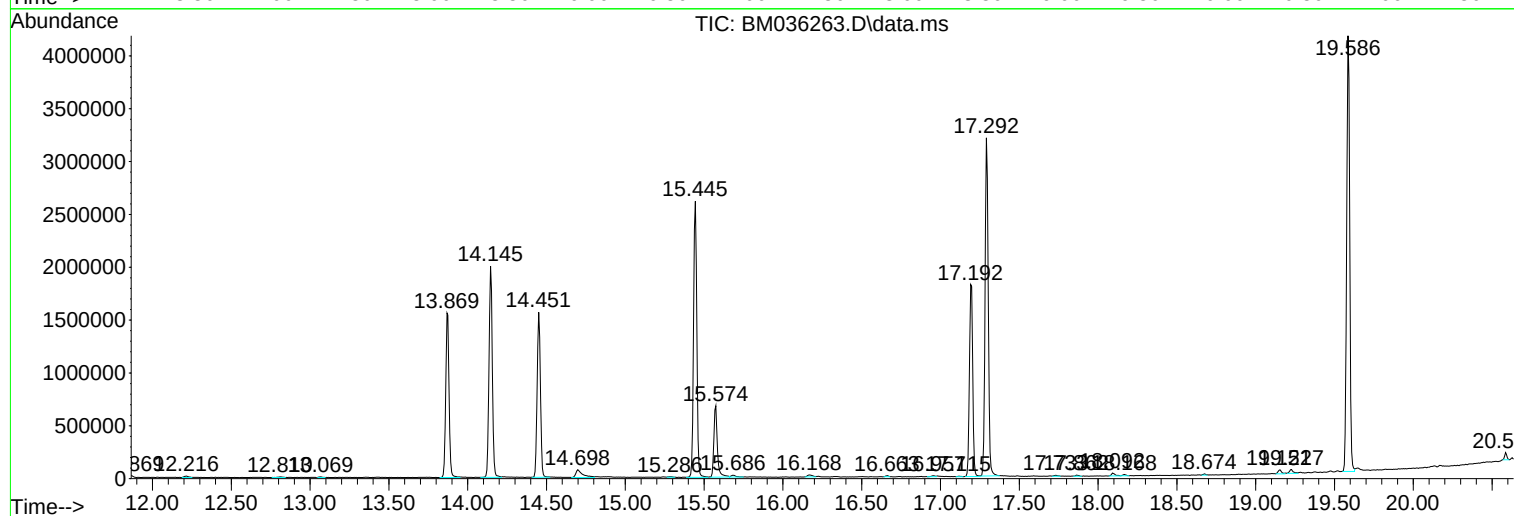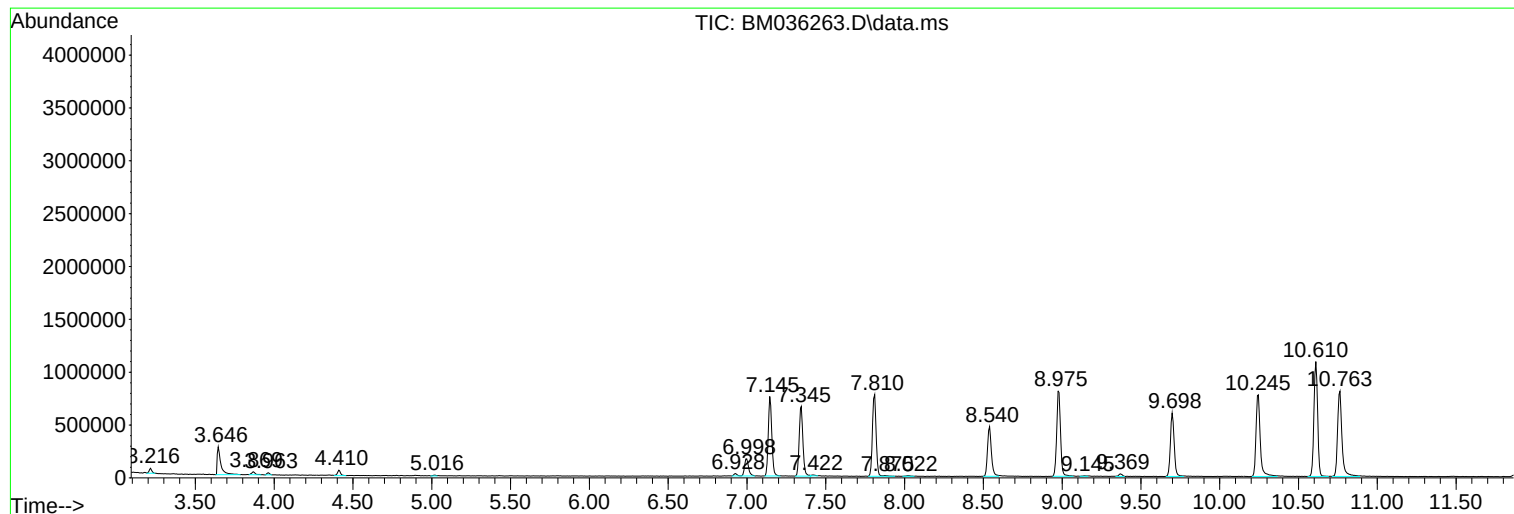

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036263.D
Acq On : 13 Aug 2022 12:10
Operator : CG/JU
Sample : N4165-07
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBZ5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081222\
Data File : BM036263.D
Acq On : 13 Aug 2022 12:10
Operator : CG/JU
Sample : N4165-07
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBZ5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc