

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081621\
 Data File : BM031770.D
 Acq On : 17 Aug 2021 03:03
 Operator : CG/JU
 Sample : M3408-15
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 34N

Quant Time: Aug 17 03:35:00 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 16 16:42:38 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.551	152	32444	20.000	ng	# 0.00
21) Naphthalene-d8	10.310	136	129630	20.000	ng	# 0.00
39) Acenaphthene-d10	14.186	164	84298	20.000	ng	0.00
64) Phenanthrene-d10	16.939	188	185279	20.000	ng	0.00
76) Chrysene-d12	21.139	240	190117	20.000	ng	0.00
86) Perylene-d12	23.286	264	178046	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.187	112	311915	154.304	ng	0.00
7) Phenol-d6	6.746	99	363224	124.005	ng	0.00
23) Nitrobenzene-d5	8.704	82	298413	96.389	ng	0.00
42) 2,4,6-Tribromophenol	15.686	330	156396	150.635	ng	0.00
45) 2-Fluorobiphenyl	12.798	172	555766	87.752	ng	0.00
79) Terphenyl-d14	19.586	244	1193987	105.814	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081621\
Data File : BM031770.D
Acq On : 17 Aug 2021 03:03
Operator : CG/JU
Sample : M3408-15
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
34N

Quant Time: Aug 17 03:35:00 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 16 16:42:38 2021
Response via : Initial Calibration




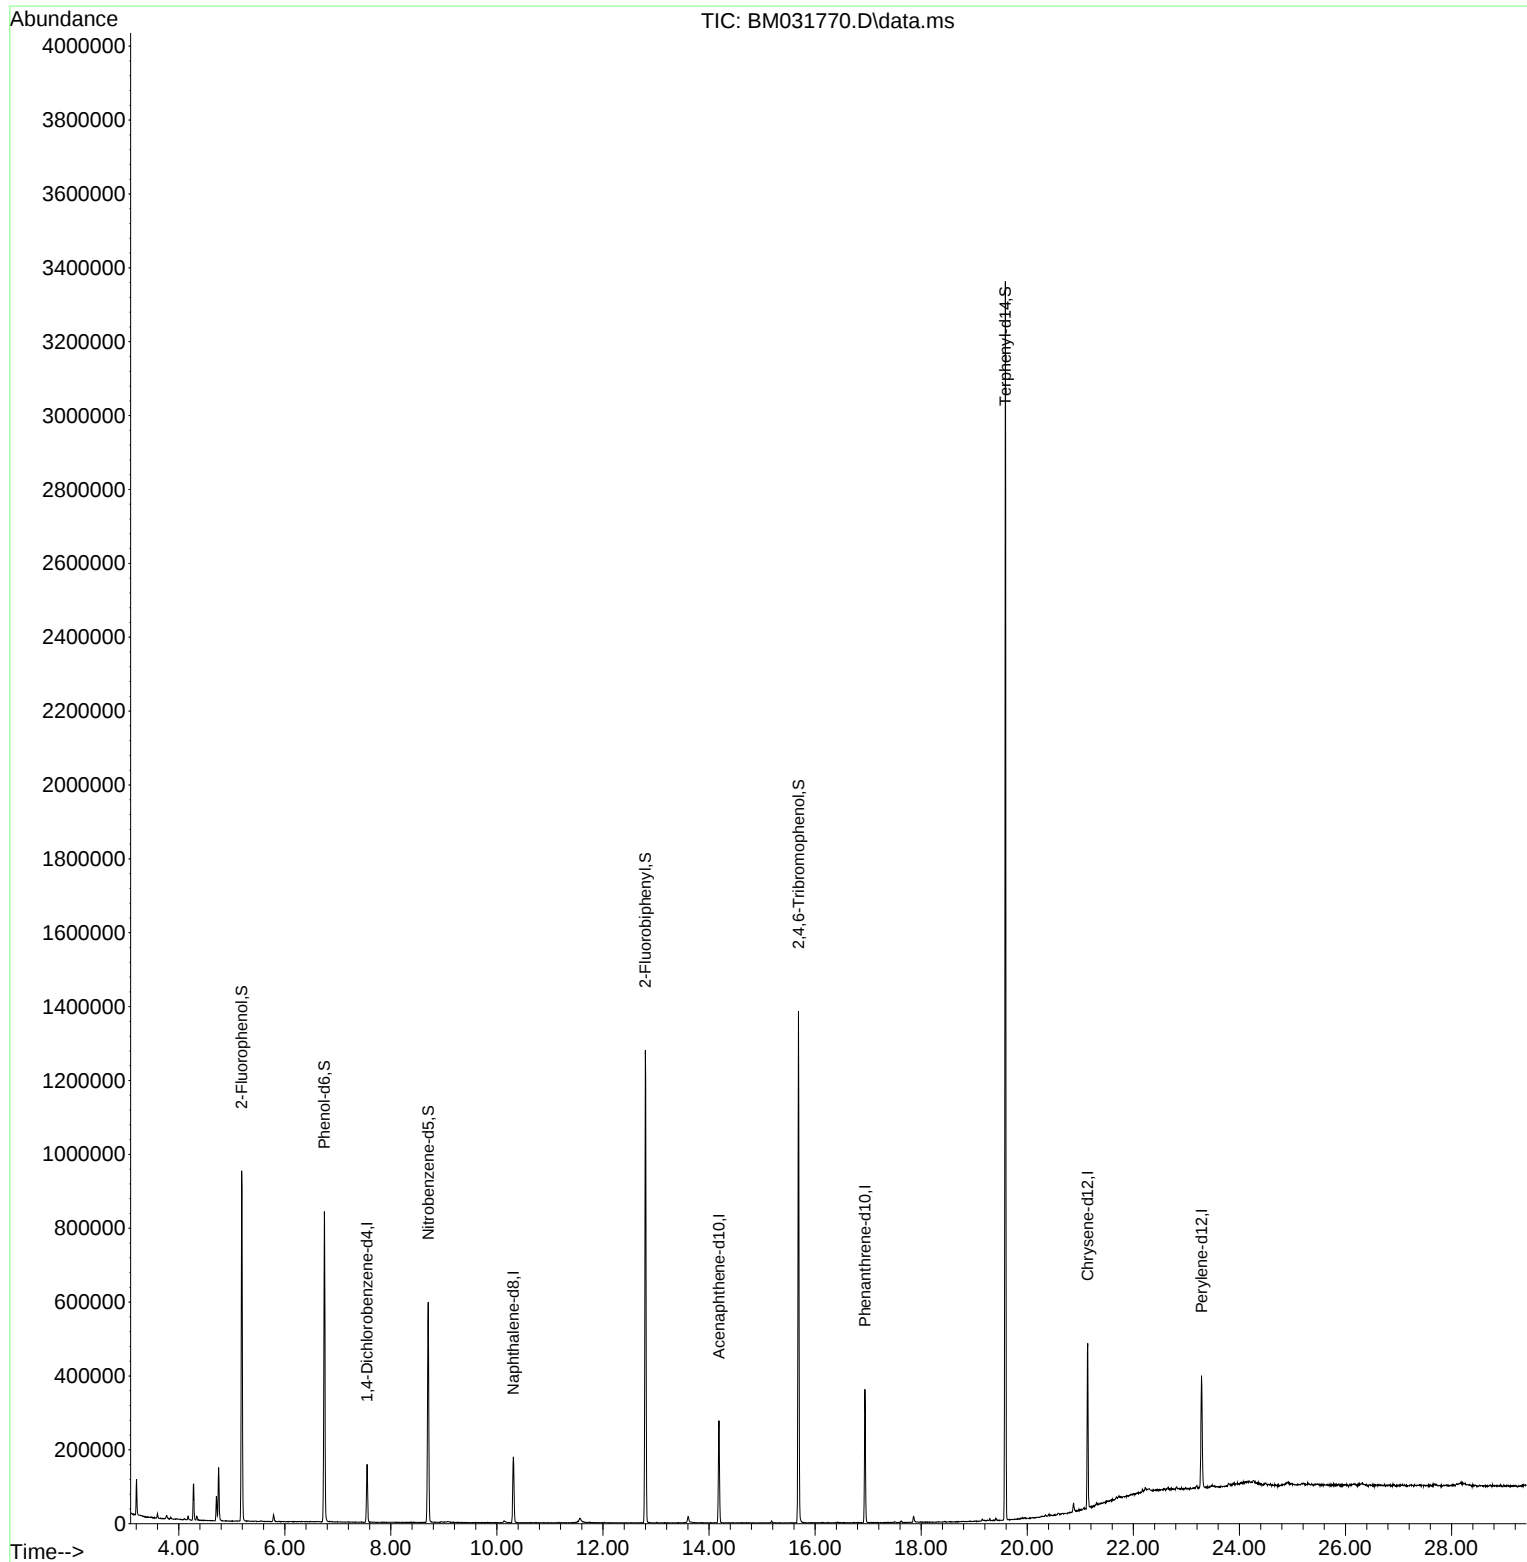


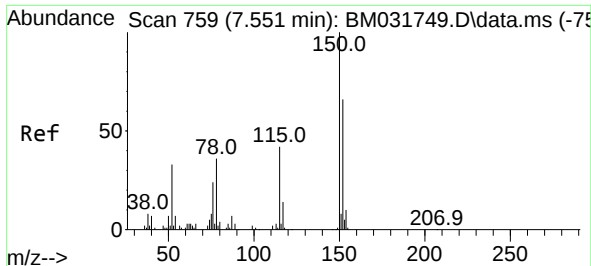

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.551 min Scan# 759
Delta R.T. 0.000 min
Lab File: BM031770.D
Acq: 17 Aug 2021 03:03




Instrument :
BNA_M
ClientSampleId :
34N


Tgt Ion:152 Resp: 32444
Ion Ratio Lower Upper
152 100
150 154.4 125.9 188.9
115 68.5 44.6 67.0#

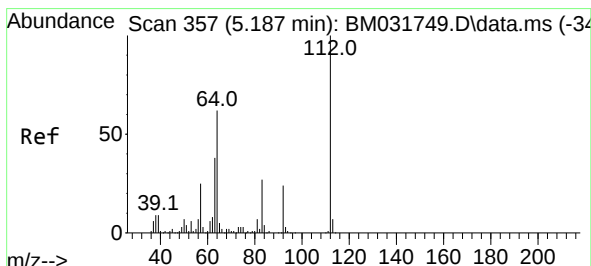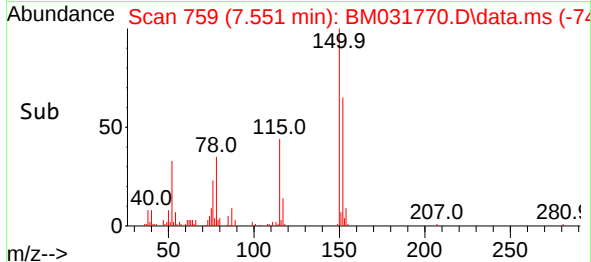

#5
2-Fluorophenol
Concen: 154.304 ng
RT: 5.187 min Scan# 357
Delta R.T. 0.000 min
Lab File: BM031770.D
Acq: 17 Aug 2021 03:03

Tgt Ion:112 Resp: 311915
Ion Ratio Lower Upper
112 100
64 63.4 47.1 70.7
63 41.0 27.3 40.9#


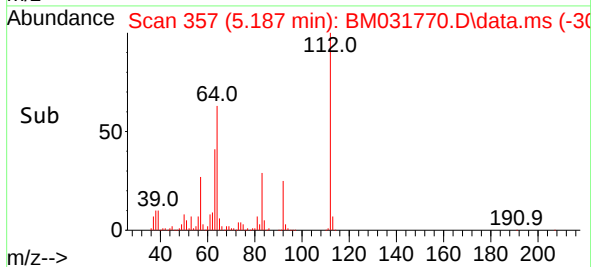

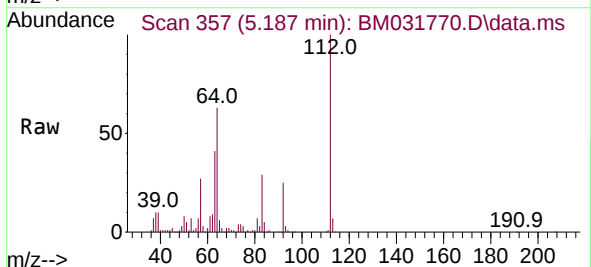


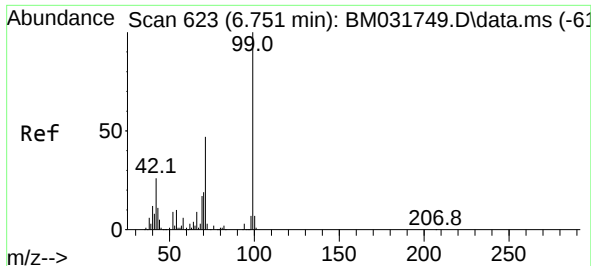

#7
Phenol-d6
Concen: 124.005 ng
RT: 6.746 min Scan# 622
Delta R.T. -0.006 min
Lab File: BM031770.D
Acq: 17 Aug 2021 03:03




Instrument :
BNA_M
ClientSampleId :
34N

Tgt Ion: 99 Resp: 363224
Ion Ratio Lower Upper
99 100
42 29.4 18.0 27.0#
71 50.7 30.9 46.3#

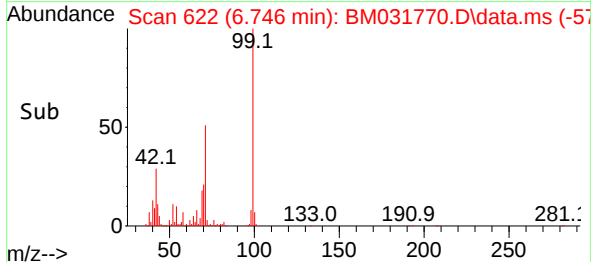

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.310 min Scan# 1228
Delta R.T. -0.006 min
Lab File: BM031770.D
Acq: 17 Aug 2021 03:03

Tgt Ion:136 Resp: 129630
Ion Ratio Lower Upper
136 100
137 10.7 8.4 12.6
54 8.8 5.5 8.3#
68 4.6 4.2 6.2


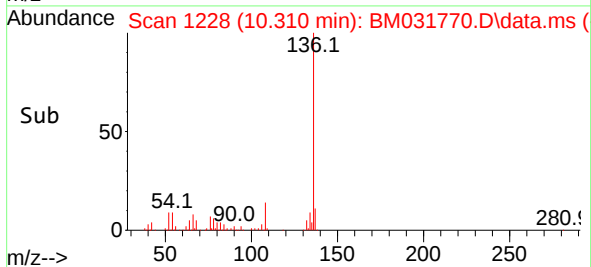

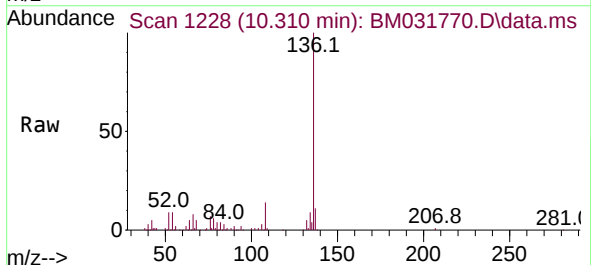




#23
Nitrobenzene-d5
Concen: 96.389 ng
RT: 8.704 min Scan# 955
Delta R.T. 0.000 min
Lab File: BM031770.D
Acq: 17 Aug 2021 03:03




Instrument :
BNA_M
ClientSampled :
34N


Tgt Ion: 82 Resp: 298413
Ion Ratio Lower Upper
82 100
128 37.0 31.1 46.7
54 57.9 37.3 55.9#

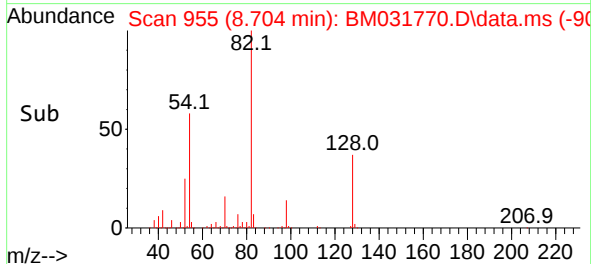

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.186 min Scan# 1887
Delta R.T. -0.006 min
Lab File: BM031770.D
Acq: 17 Aug 2021 03:03

Tgt Ion: 164 Resp: 84298
Ion Ratio Lower Upper
164 100
162 103.5 83.4 125.0
160 43.7 37.2 55.8


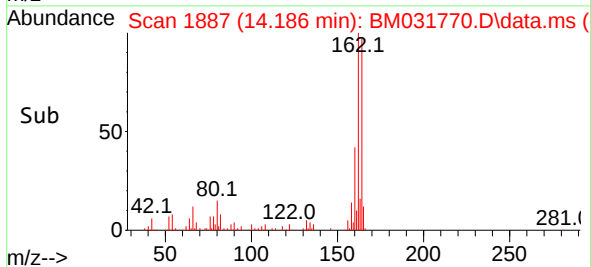

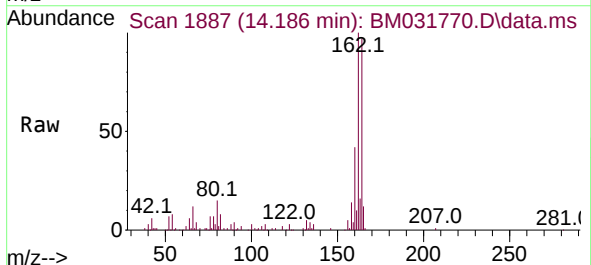


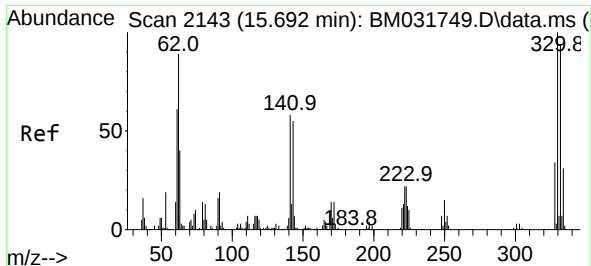

#42
2,4,6-Tribromophenol
Concen: 150.635 ng
RT: 15.686 min Scan# 2142
Delta R.T. -0.006 min
Lab File: BM031770.D
Acq: 17 Aug 2021 03:03




Instrument :
BNA_M
ClientSampled :
34N


Tgt Ion:330 Resp: 156396
Ion Ratio Lower Upper
330 100
332 94.0 77.0 115.4
141 61.6 30.2 45.2#

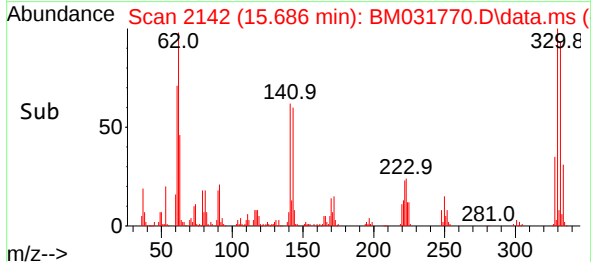

#45
2-Fluorobiphenyl
Concen: 87.752 ng
RT: 12.798 min Scan# 1651
Delta R.T. -0.006 min
Lab File: BM031770.D
Acq: 17 Aug 2021 03:03

Tgt Ion:172 Resp: 555766
Ion Ratio Lower Upper
172 100
171 35.0 28.6 43.0
170 23.0 18.4 27.6


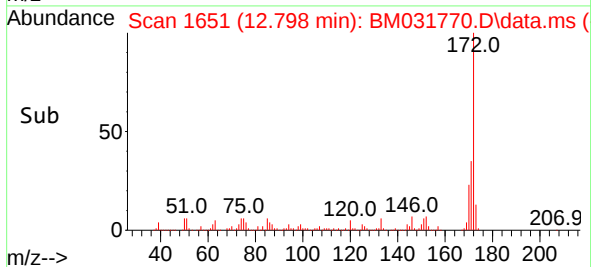

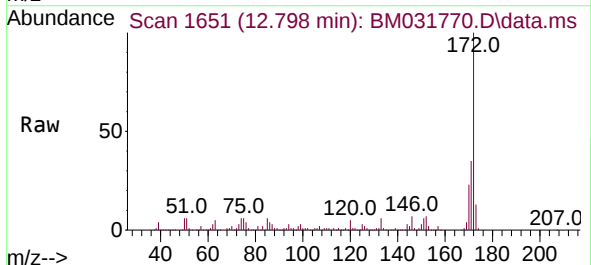




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 16.939 min Scan# 2355
Delta R.T. -0.006 min
Lab File: BM031770.D
Acq: 17 Aug 2021 03:03




Instrument :
BNA_M
ClientSampleId :
34N


Tgt Ion:188	Resp: 185279
Ion Ratio	Lower Upper
188 100	
94 7.3	6.0 9.0
80 8.4	6.6 9.8

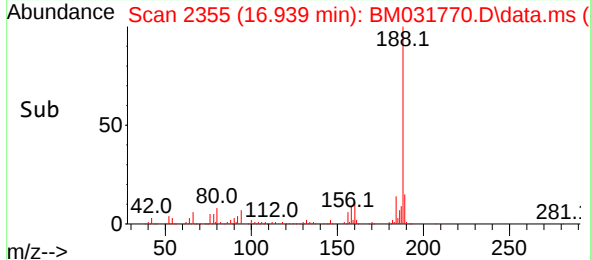

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.139 min Scan# 3069
Delta R.T. -0.006 min
Lab File: BM031770.D
Acq: 17 Aug 2021 03:03

Tgt Ion:240	Resp: 190117
Ion Ratio	Lower Upper
240 100	
120 7.7	7.0 10.6
236 24.9	21.0 31.4


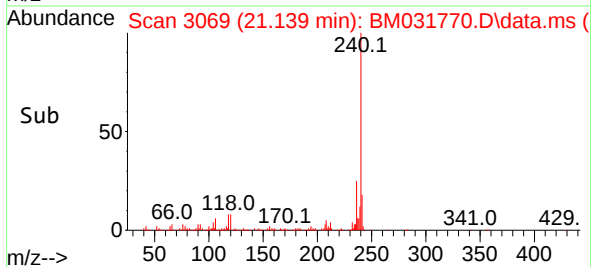

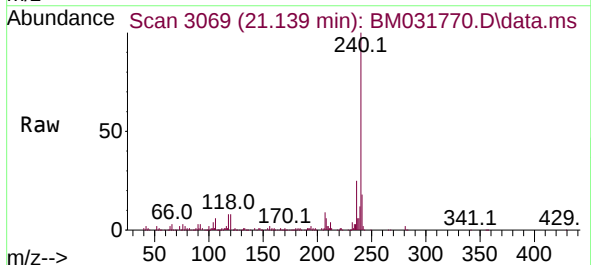


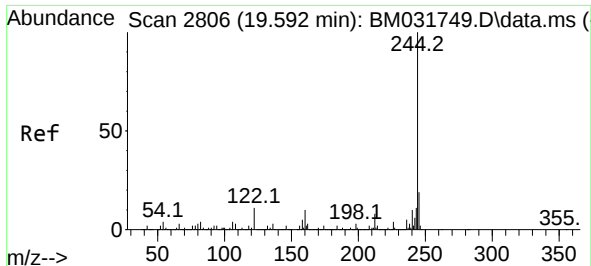

#79
 Terphenyl-d14
 Concen: 105.814 ng
 RT: 19.586 min Scan# 2805
 Delta R.T. -0.006 min
 Lab File: BM031770.D
 Acq: 17 Aug 2021 03:03

Instrument :
 BNA_M
 ClientSampleId :
 34N

Tgt Ion:244 Resp: 1193987
 Ion Ratio Lower Upper
 244 100
 212 8.4 6.3 9.5
 122 10.6 6.9 10.3#

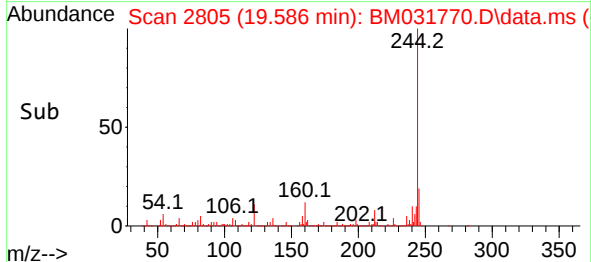

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.286 min Scan# 3434
 Delta R.T. -0.012 min
 Lab File: BM031770.D
 Acq: 17 Aug 2021 03:03

Tgt Ion:264 Resp: 178046
 Ion Ratio Lower Upper
 264 100
 260 23.1 19.8 29.8
 265 21.7 17.7 26.5

