
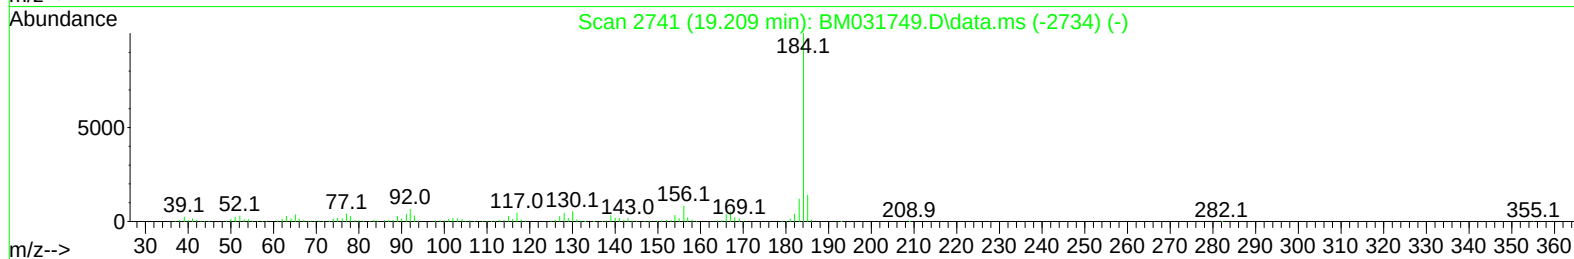
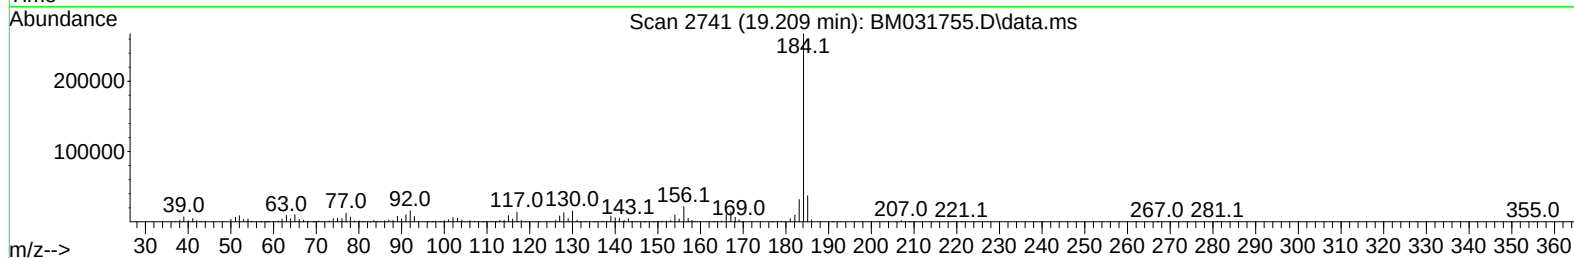


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081621\
Data File : BM031755.D
Acq On : 16 Aug 2021 17:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 16 18:35:45 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 16 16:42:38 2021
Response via : Initial Calibration

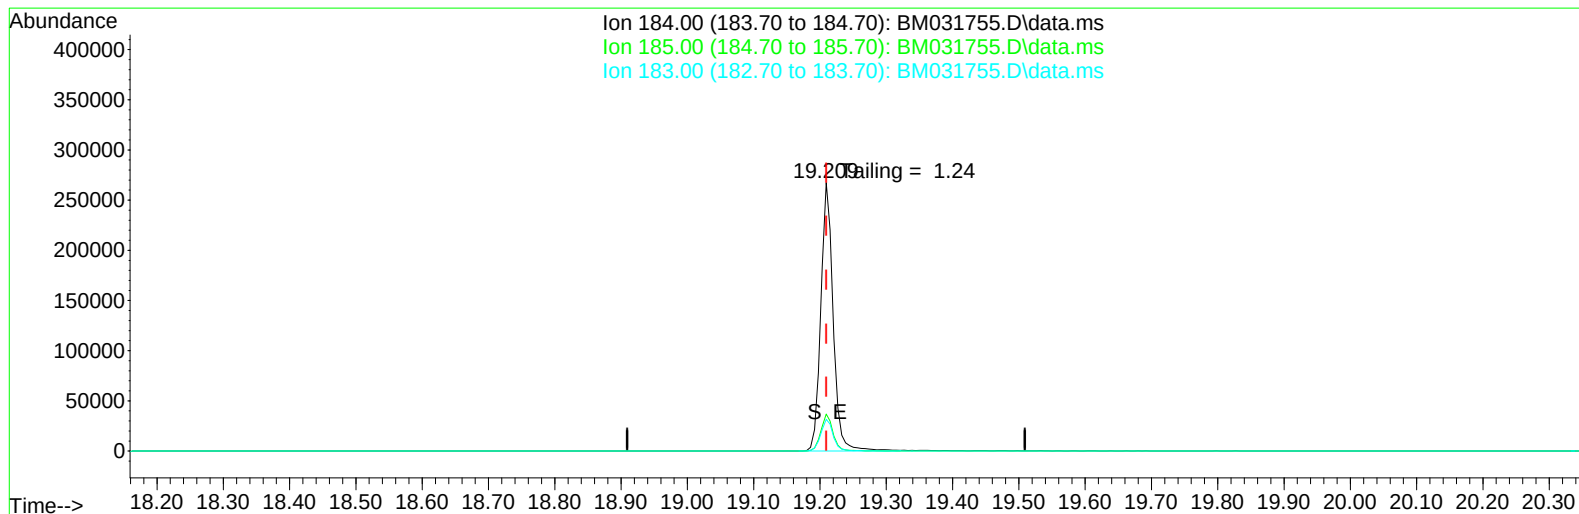

TIC: BM031755.D\data.ms

(77) Benzidine




19.209min (+ 0.000) 0.00 ng

response 347646

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.80
183.00	12.30	11.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081621\
Data File : BM031755.D
Acq On : 16 Aug 2021 17:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 16 18:35:45 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 16 16:42:38 2021
Response via : Initial Calibration

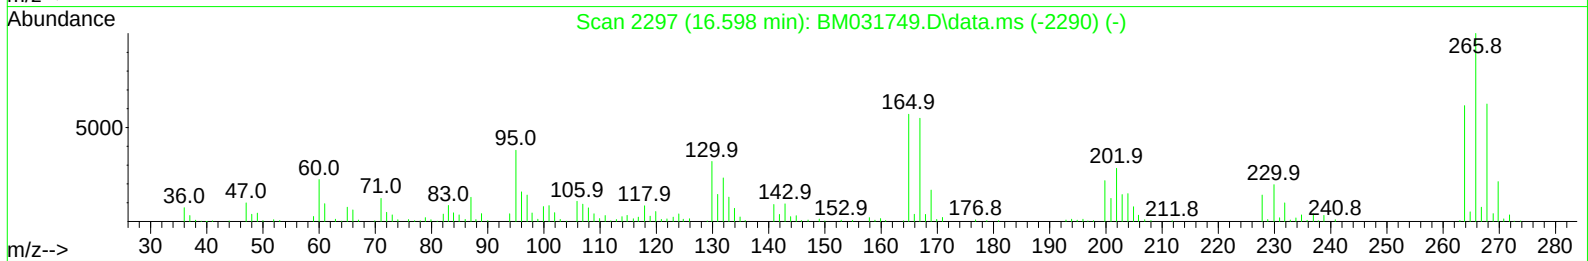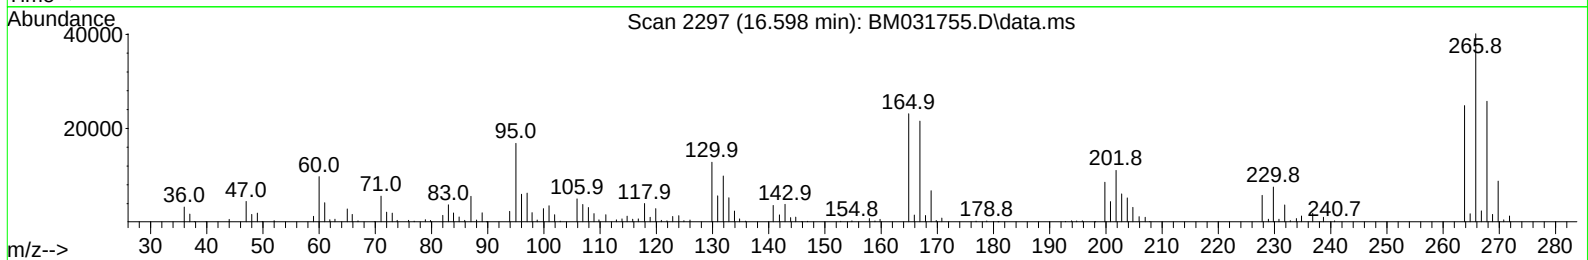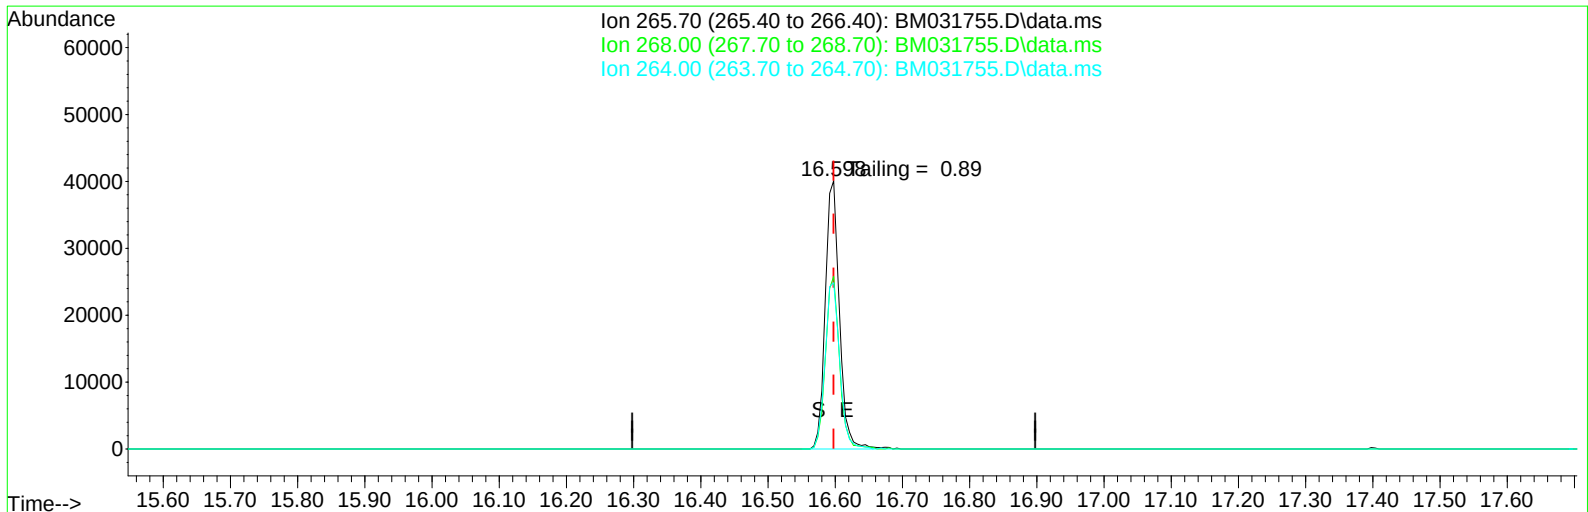

TIC: BM031755.D\data.ms

(70) Pentachlorophenol (C)

16.598min (+ 0.000) 0.00 ng

response 58735

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	64.25
264.00	64.90	61.93
0.00	0.00	0.00