

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081621\
 Data File : BM031759.D
 Acq On : 16 Aug 2021 20:15
 Operator : CG/JU
 Sample : M3407-12
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 26S

Quant Time: Aug 17 08:09:03 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 16 16:42:38 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.551	152	34210	20.000	ng	# 0.00
21) Naphthalene-d8	10.310	136	138158	20.000	ng	# 0.00
39) Acenaphthene-d10	14.186	164	90184	20.000	ng	0.00
64) Phenanthrene-d10	16.939	188	197593	20.000	ng	0.00
76) Chrysene-d12	21.139	240	217144	20.000	ng	0.00
86) Perylene-d12	23.291	264	215173	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.193	112	293331	137.619	ng	0.00
7) Phenol-d6	6.745	99	317269	102.724	ng	0.00
23) Nitrobenzene-d5	8.704	82	316400	95.891	ng	0.00
42) 2,4,6-Tribromophenol	15.692	330	163130	146.867	ng	0.00
45) 2-Fluorobiphenyl	12.804	172	633072	93.434	ng	0.00
79) Terphenyl-d14	19.592	244	1318776	102.327	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081621\
Data File : BM031759.D
Acq On : 16 Aug 2021 20:15
Operator : CG/JU
Sample : M3407-12
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
26S

Quant Time: Aug 17 08:09:03 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 16 16:42:38 2021
Response via : Initial Calibration




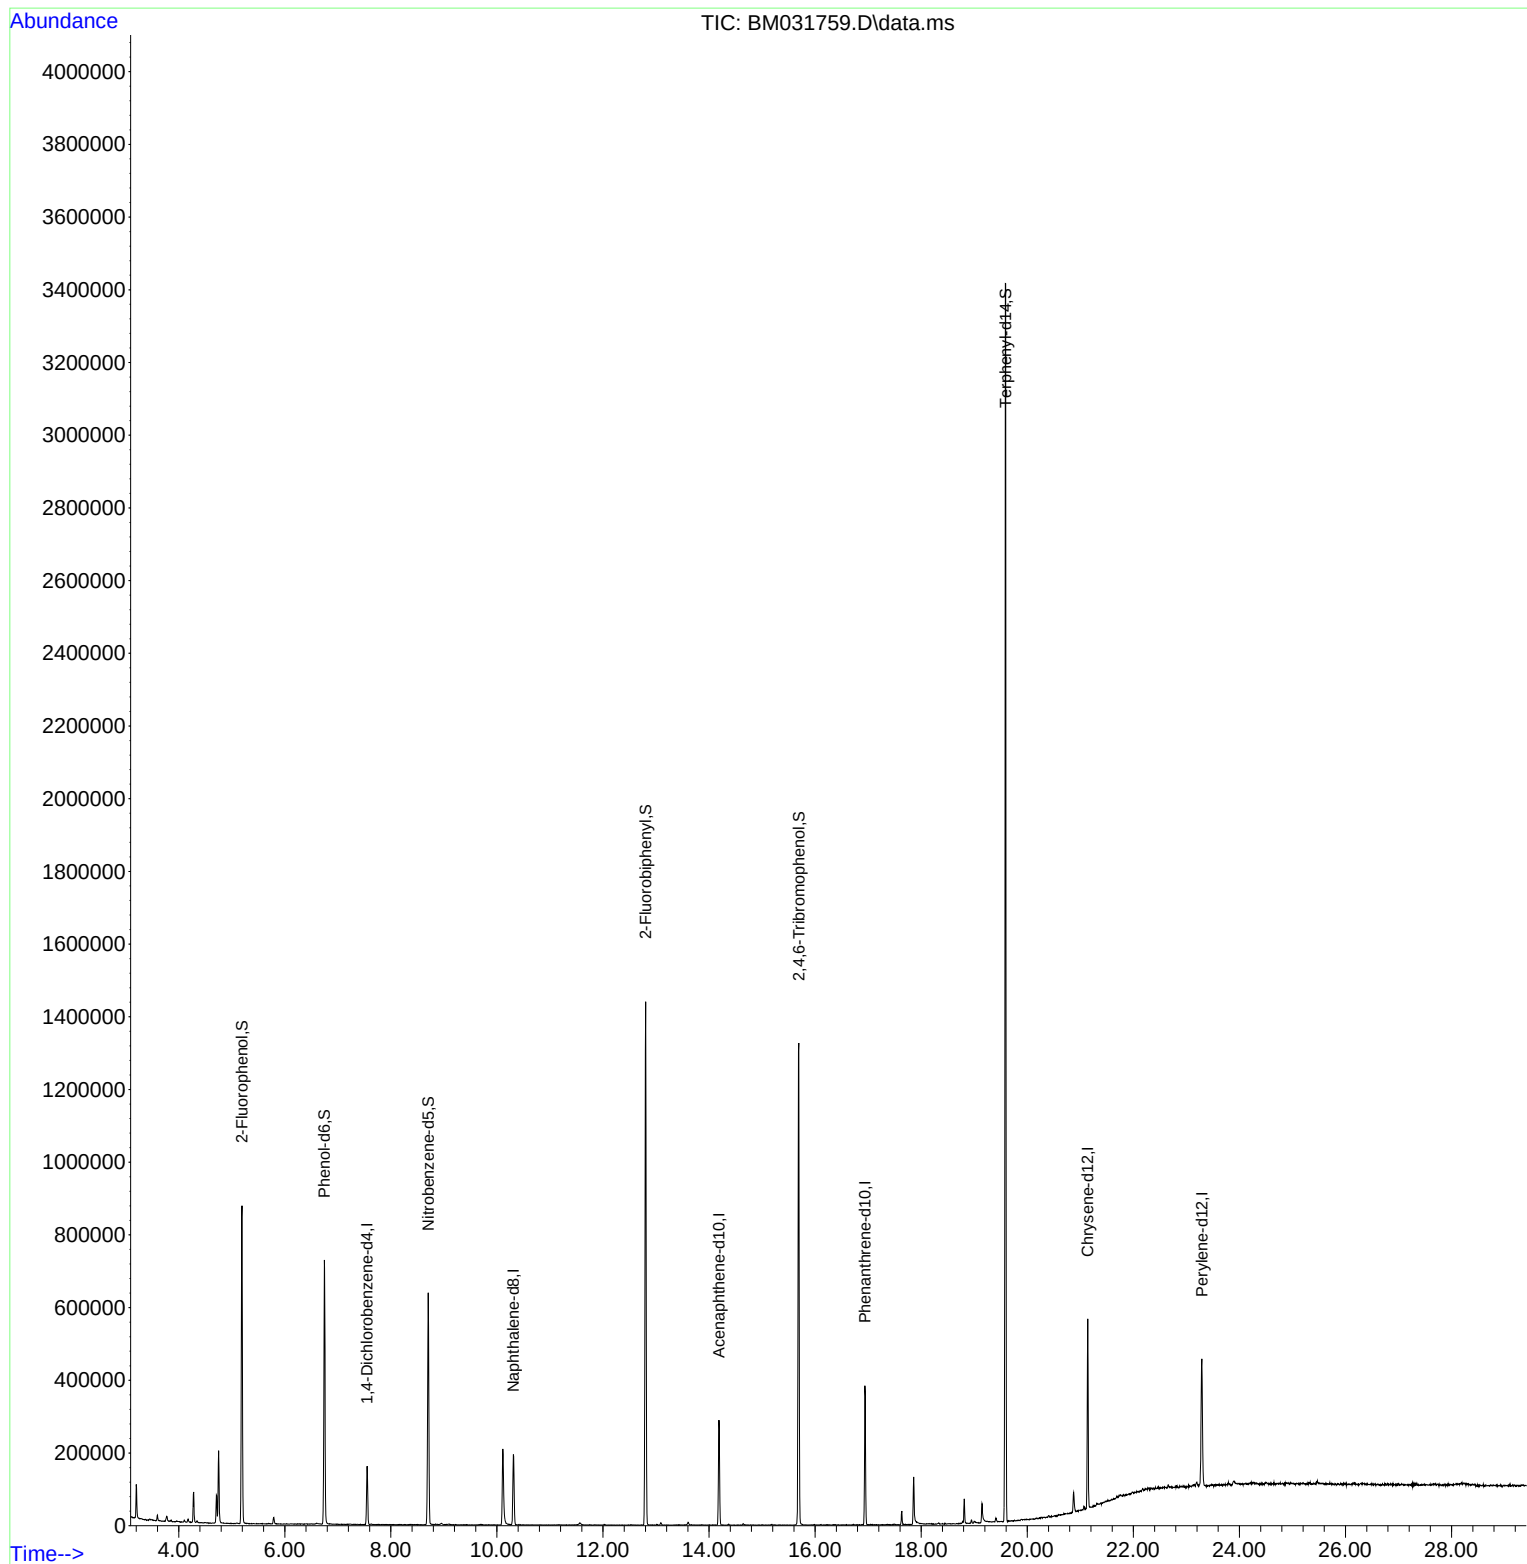




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.551 min Scan# 759
Delta R.T. 0.000 min
Lab File: BM031759.D
Acq: 16 Aug 2021 20:15




Instrument :
BNA_M
ClientSampleId :
26S


Tgt Ion:152 Resp: 34210
Ion Ratio Lower Upper
152 100
150 164.4 125.9 188.9
115 67.9 44.6 67.0#

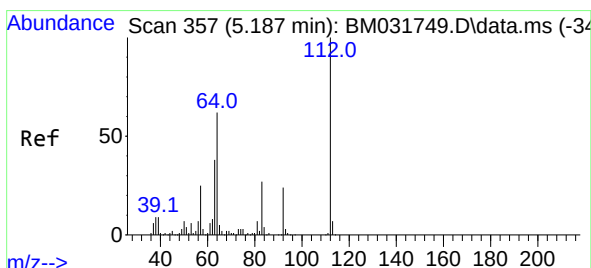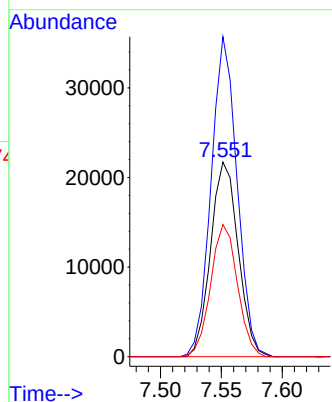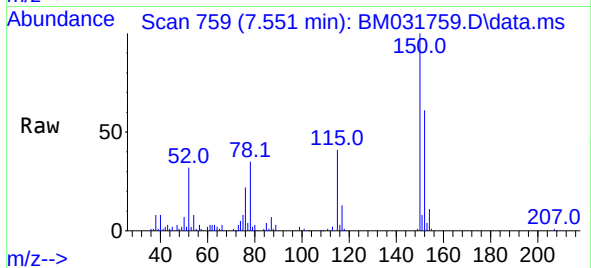

#5
2-Fluorophenol
Concen: 137.619 ng
RT: 5.193 min Scan# 358
Delta R.T. 0.006 min
Lab File: BM031759.D
Acq: 16 Aug 2021 20:15

Tgt Ion:112 Resp: 293331
Ion Ratio Lower Upper
112 100
64 60.8 47.1 70.7
63 39.6 27.3 40.9


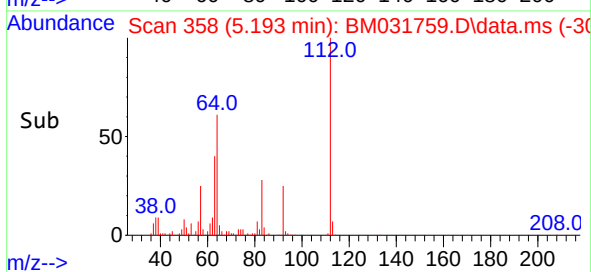
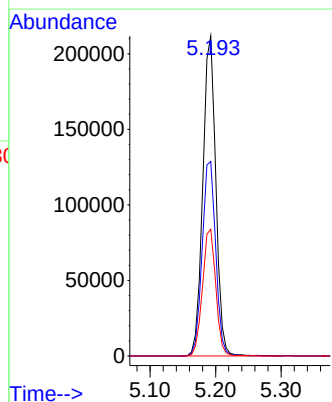





#7
Phenol-d6
Concen: 102.724 ng
RT: 6.745 min Scan# 622
Delta R.T. -0.006 min
Lab File: BM031759.D
Acq: 16 Aug 2021 20:15




Instrument :
BNA_M
ClientSampleId :
26S


Tgt Ion: 99 Resp: 317269
Ion Ratio Lower Upper
99 100
42 29.2 18.0 27.0#
71 50.2 30.9 46.3#

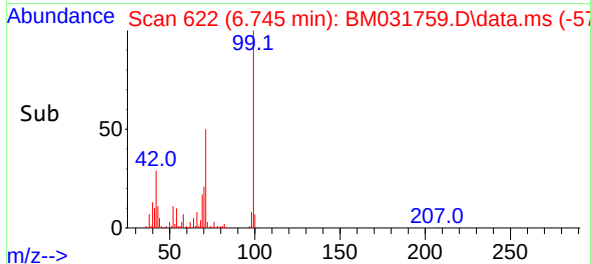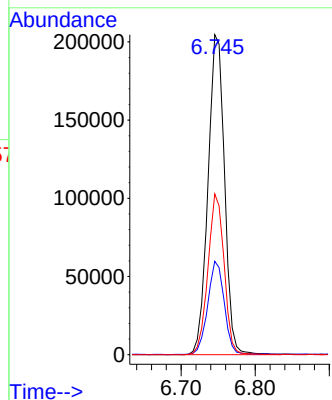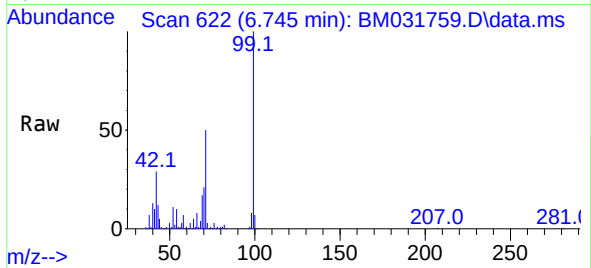

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.310 min Scan# 1228
Delta R.T. -0.006 min
Lab File: BM031759.D
Acq: 16 Aug 2021 20:15

Tgt Ion: 136 Resp: 138158
Ion Ratio Lower Upper
136 100
137 10.9 8.4 12.6
54 9.6 5.5 8.3#
68 4.9 4.2 6.2


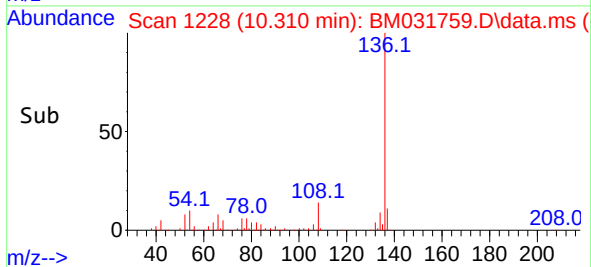
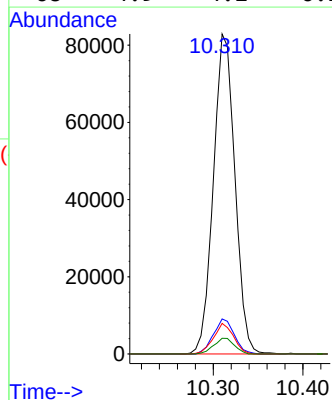
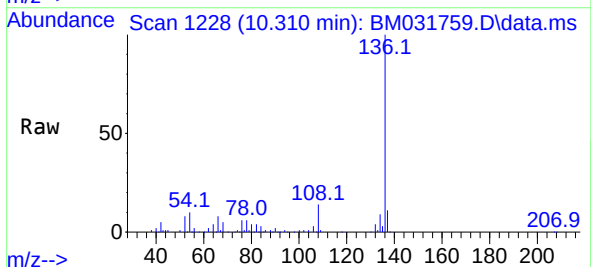




#23
Nitrobenzene-d5
Concen: 95.891 ng
RT: 8.704 min Scan# 955
Delta R.T. 0.000 min
Lab File: BM031759.D
Acq: 16 Aug 2021 20:15




Instrument :
BNA_M
ClientSampleId :
26S


Tgt Ion: 82 Resp: 316400
Ion Ratio Lower Upper
82 100
128 36.7 31.1 46.7
54 57.8 37.3 55.9#

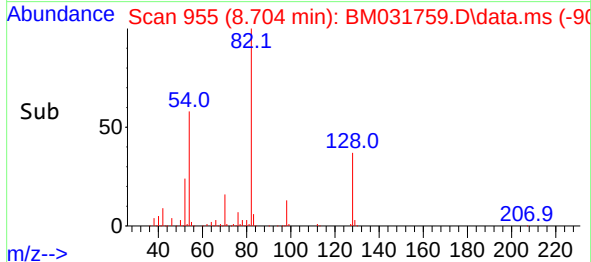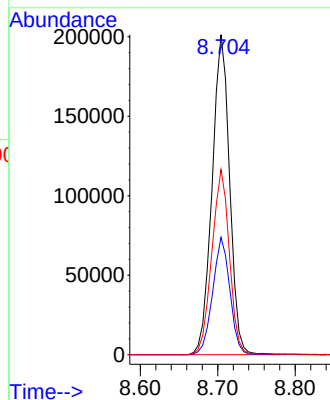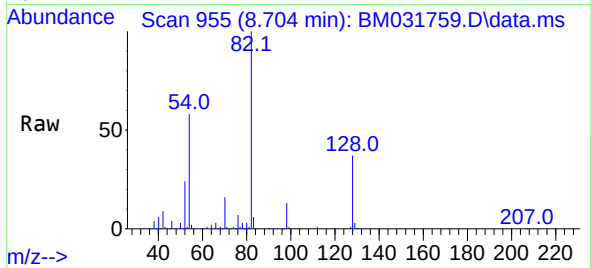

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.186 min Scan# 1887
Delta R.T. -0.006 min
Lab File: BM031759.D
Acq: 16 Aug 2021 20:15

Tgt Ion:164 Resp: 90184
Ion Ratio Lower Upper
164 100
162 103.4 83.4 125.0
160 45.3 37.2 55.8


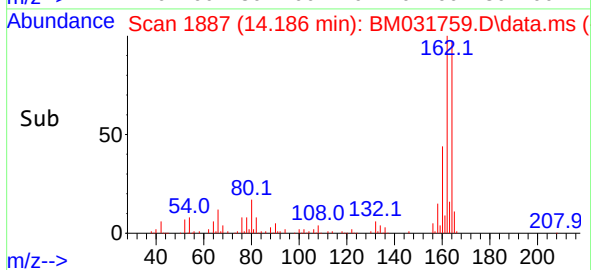
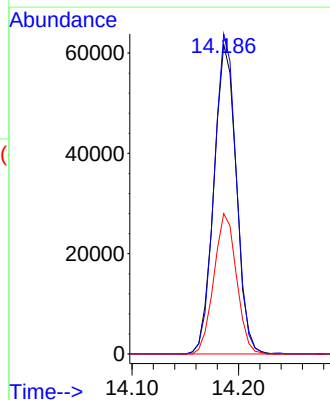
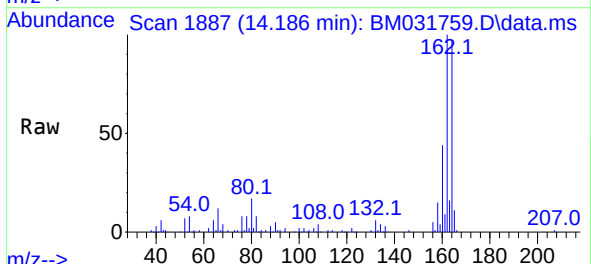




#42
2,4,6-Tribromophenol
Concen: 146.867 ng
RT: 15.692 min Scan# 2143
Delta R.T. 0.000 min
Lab File: BM031759.D
Acq: 16 Aug 2021 20:15




Instrument :
BNA_M
ClientSampleId :
26S


Tgt Ion:330 Resp: 163130
Ion Ratio Lower Upper
330 100
332 95.6 77.0 115.4
141 60.9 30.2 45.2#

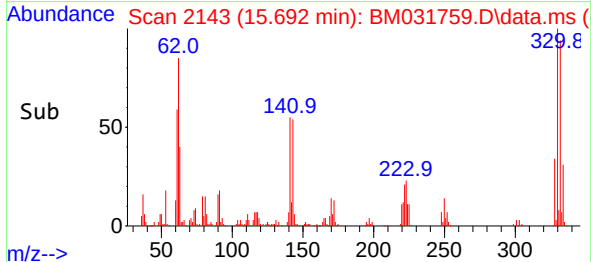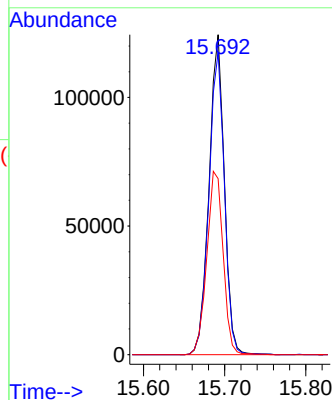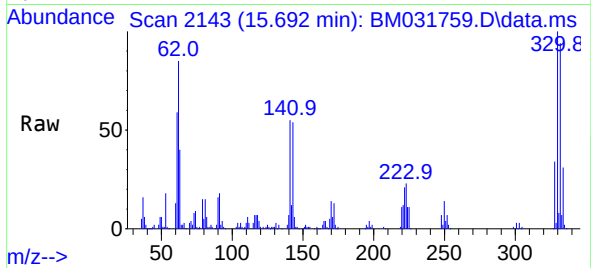

#45
2-Fluorobiphenyl
Concen: 93.434 ng
RT: 12.804 min Scan# 1652
Delta R.T. 0.000 min
Lab File: BM031759.D
Acq: 16 Aug 2021 20:15

Tgt Ion:172 Resp: 633072
Ion Ratio Lower Upper
172 100
171 35.0 28.6 43.0
170 22.8 18.4 27.6


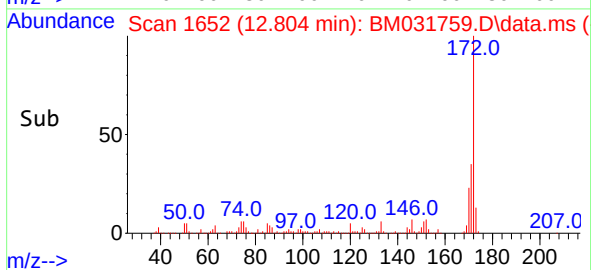
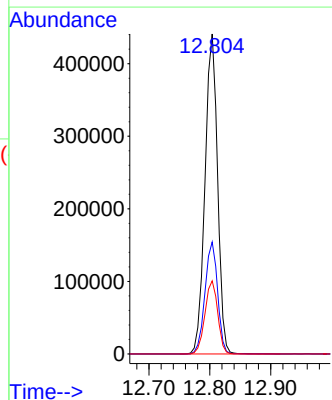
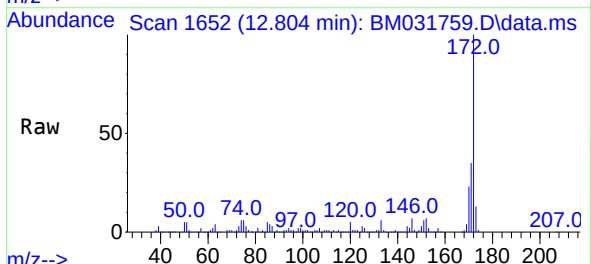




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 16.939 min Scan# 2355
Delta R.T. -0.006 min
Lab File: BM031759.D
Acq: 16 Aug 2021 20:15




Instrument :
BNA_M
ClientSampleId :
26S


Tgt Ion:188 Resp: 197593
Ion Ratio Lower Upper
188 100
94 7.6 6.0 9.0
80 8.8 6.6 9.8

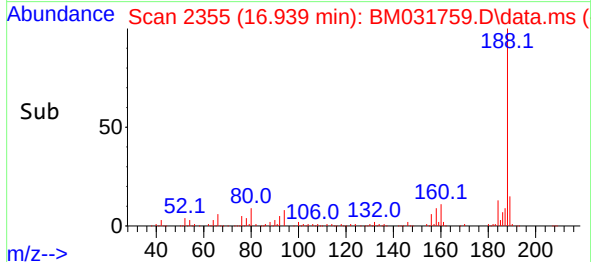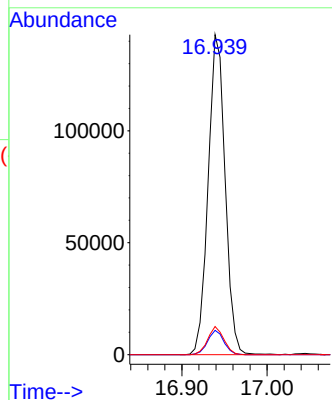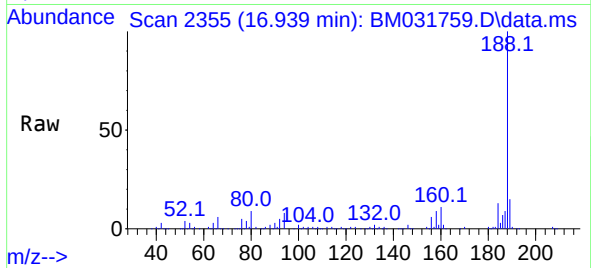

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.139 min Scan# 3069
Delta R.T. -0.006 min
Lab File: BM031759.D
Acq: 16 Aug 2021 20:15

Tgt Ion:240 Resp: 217144
Ion Ratio Lower Upper
240 100
120 9.0 7.0 10.6
236 26.5 21.0 31.4


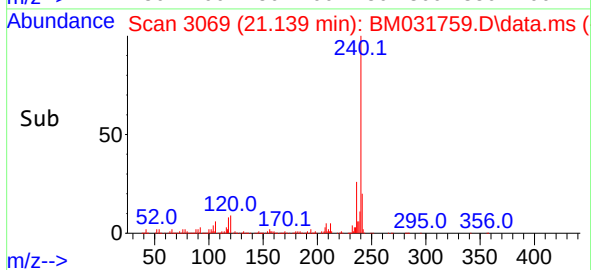
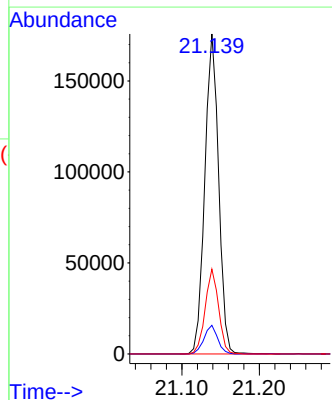
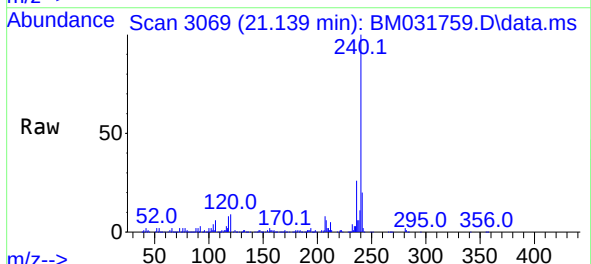




#79
 Terphenyl-d14
 Concen: 102.327 ng
 RT: 19.592 min Scan# 2806
 Delta R.T. 0.000 min
 Lab File: BM031759.D
 Acq: 16 Aug 2021 20:15

Instrument :
 BNA_M
 ClientSampleId :
 26S

Tgt Ion:244 Resp: 1318776
 Ion Ratio Lower Upper
 244 100
 212 8.1 6.3 9.5
 122 9.1 6.9 10.3

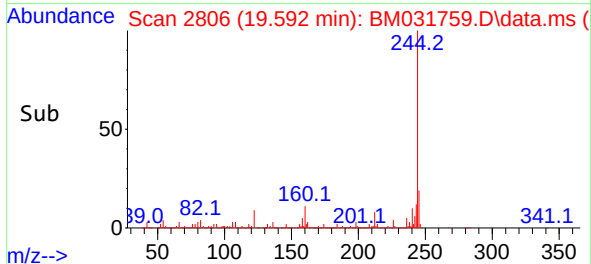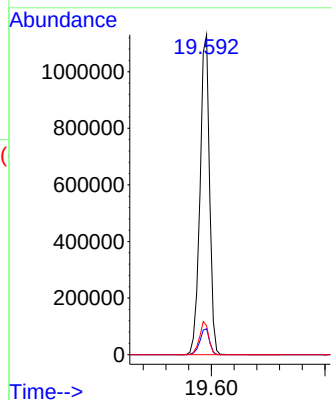

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.291 min Scan# 3435
 Delta R.T. -0.006 min
 Lab File: BM031759.D
 Acq: 16 Aug 2021 20:15

Tgt Ion:264 Resp: 215173
 Ion Ratio Lower Upper
 264 100
 260 22.7 19.8 29.8
 265 21.9 17.7 26.5

