
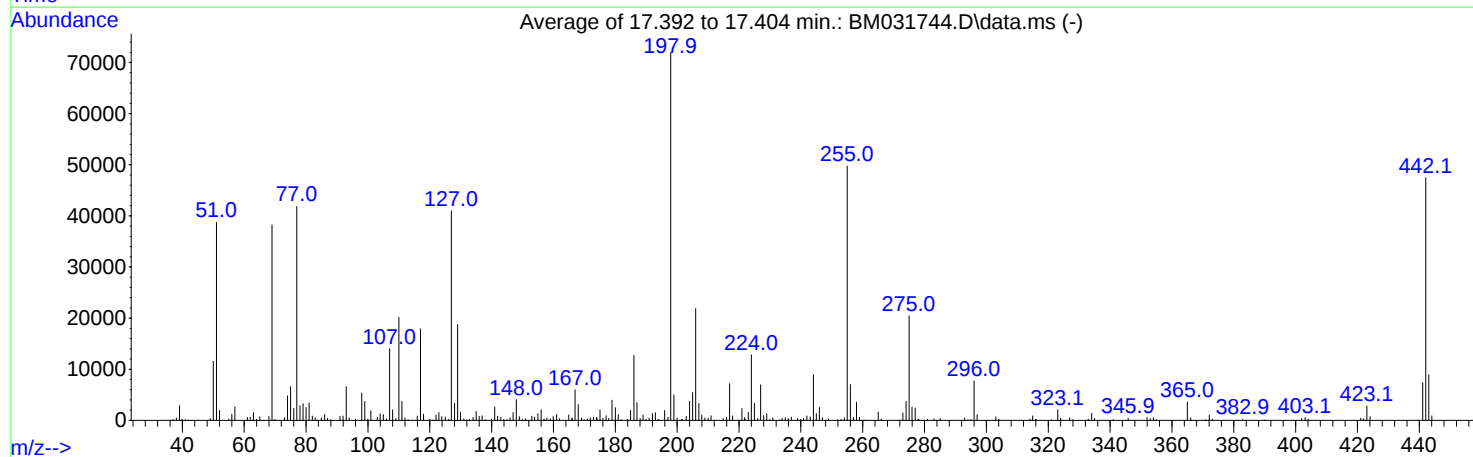


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081621\
 Data File : BM031744.D
 Acq On : 16 Aug 2021 10:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 16 16:42:38 2021

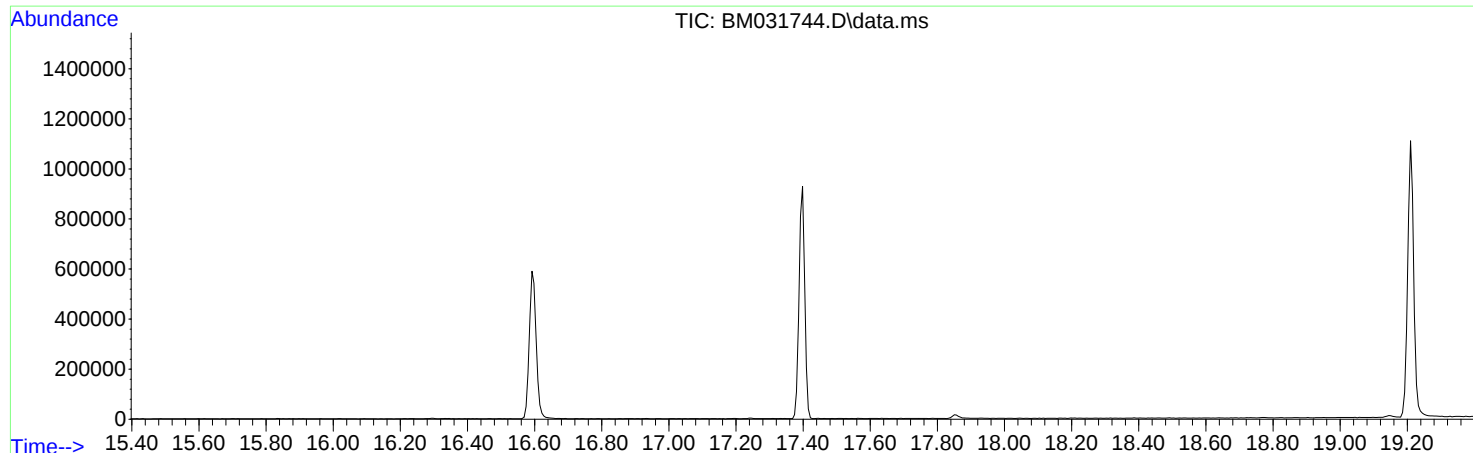




AutoFind: Scans 2432, 2433, 2434; Background Corrected with Scan 2426

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.8	38723	PASS
68	69	0.00	2	2.0	758	PASS
69	198	0.00	100	53.1	38205	PASS
70	69	0.00	2	0.3	131	PASS
127	198	10	80	56.9	40965	PASS
197	198	0.00	2	0.9	618	PASS
198	198	100	100	100.0	71955	PASS
199	198	5	9	6.9	4989	PASS
275	198	10	60	28.4	20437	PASS
365	198	1	100	5.0	3610	PASS
441	198	0.01	100	10.2	7375	PASS
442	442	50	100	100.0	47493	PASS
443	442	15	24	18.8	8935	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081621\
Data File : BM031744.D
Acq On : 16 Aug 2021 10:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 16 18:28:20 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 16 16:42:38 2021
Response via : Initial Calibration

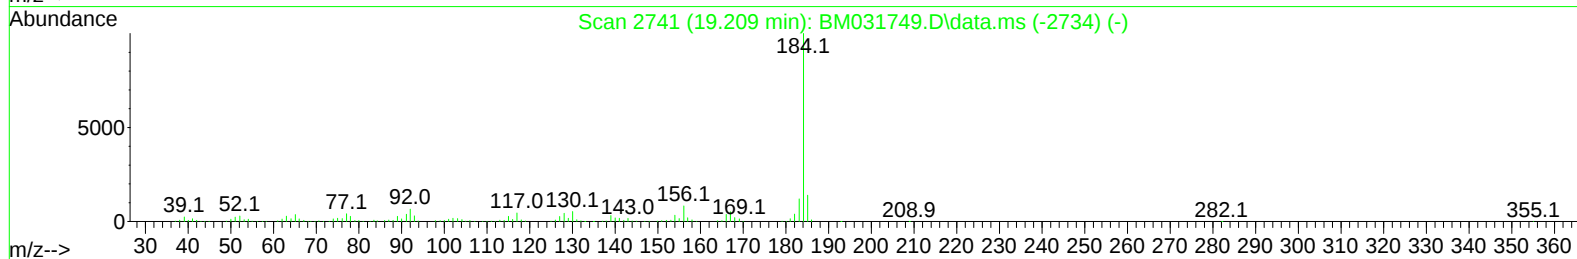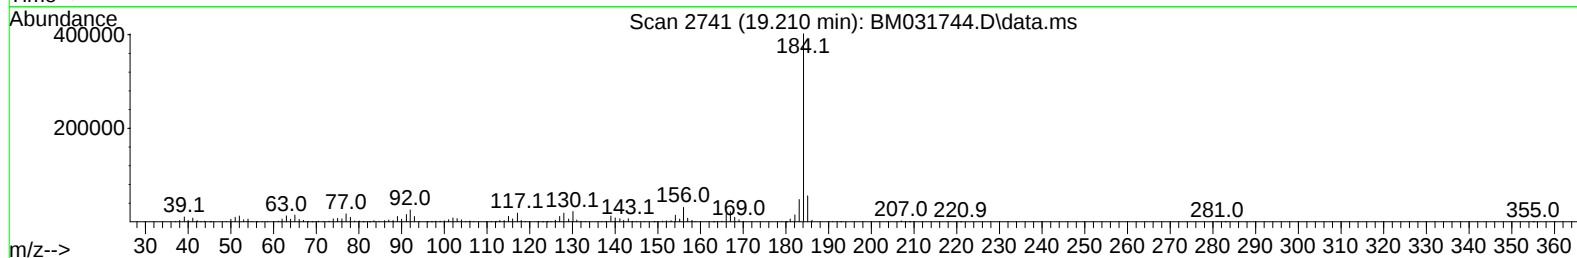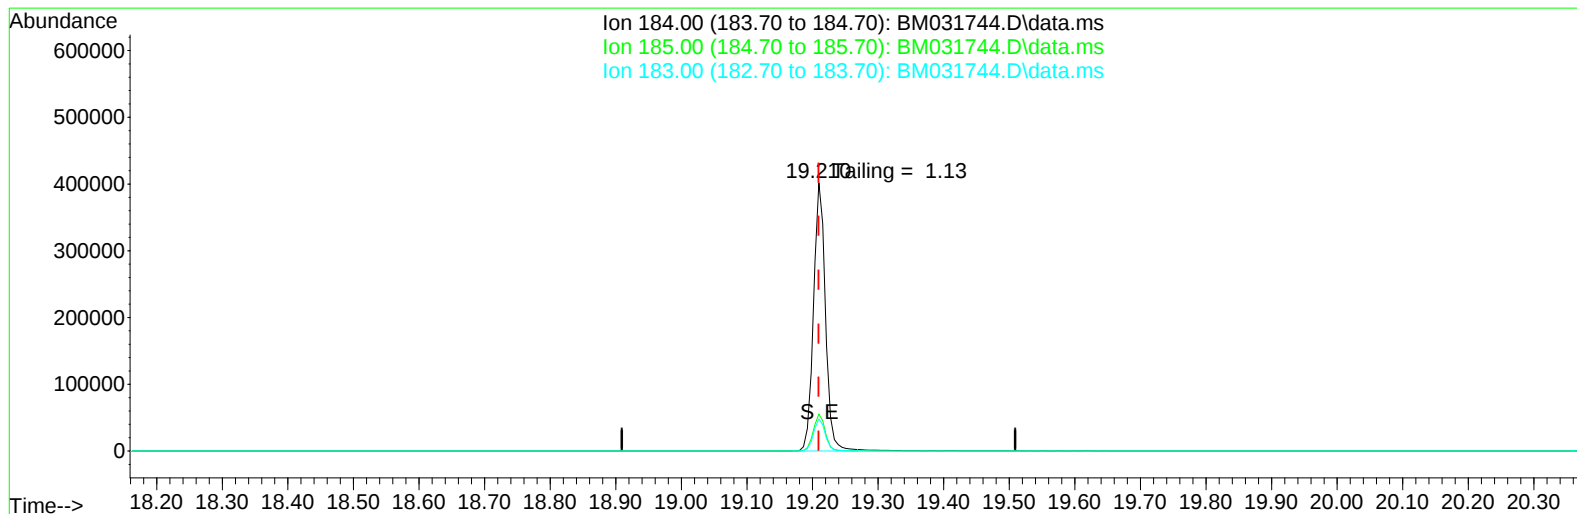

TIC: BM031744.D\data.ms

(77) Benzidine

19.210min (+ 0.000) 0.00 ng




response 513271

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.79
183.00	12.30	11.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081621\
Data File : BM031744.D
Acq On : 16 Aug 2021 10:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 16 18:28:20 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 16 16:42:38 2021
Response via : Initial Calibration

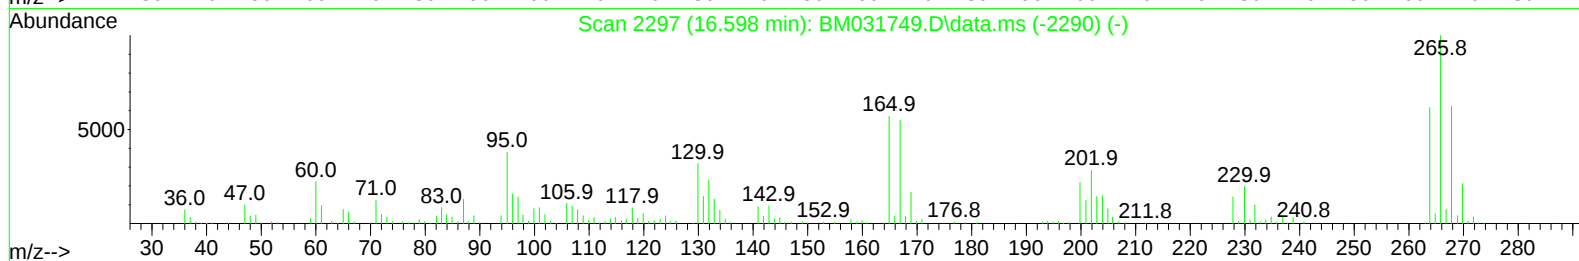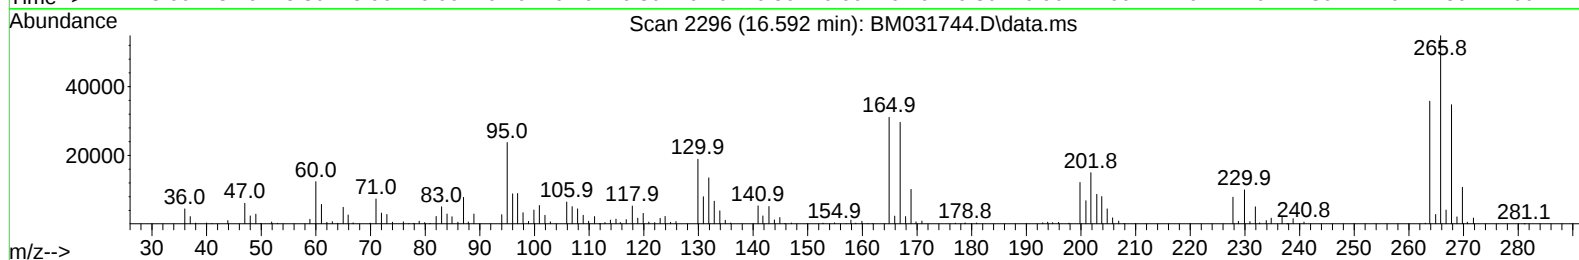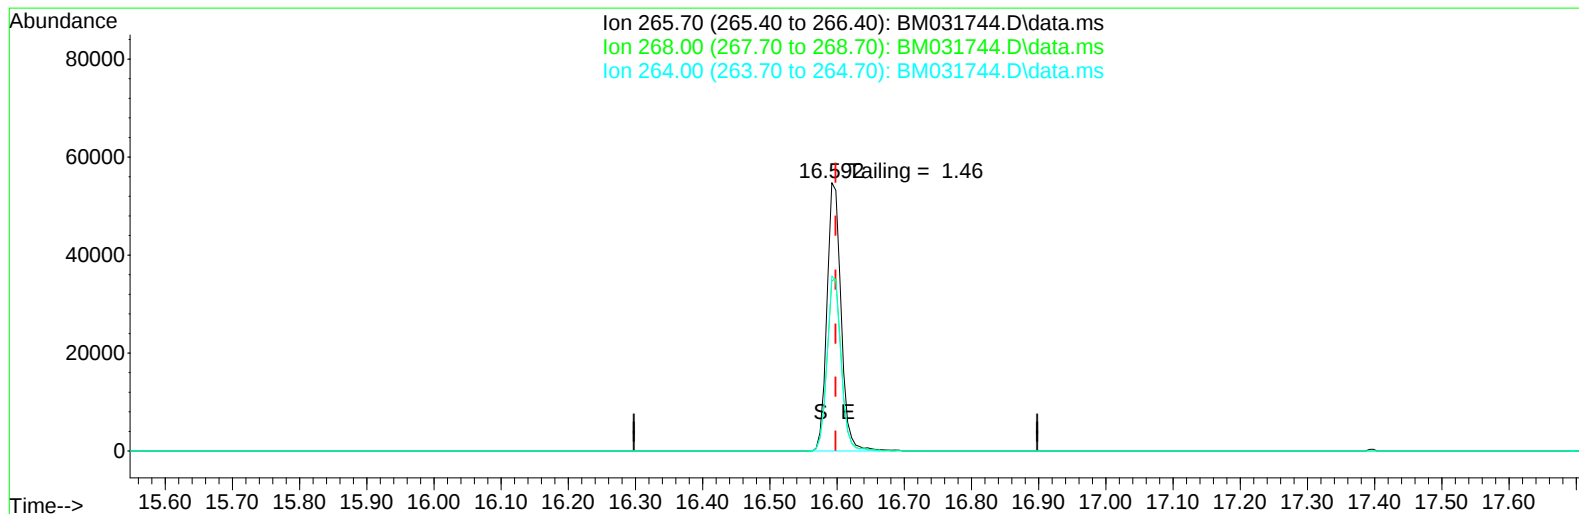

TIC: BM031744.D\data.ms

(70) Pentachlorophenol (C)

16.592min (-0.005) 0.00 ng

response 80302

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	63.45
264.00	64.90	65.25
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/16/2021	BNA_M	<u>BM031744.D</u>
Compound Name	Response	Retention Time
DDT	275381	20.45
DDD	6919	20.04
DDE	191	19.49
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7110	282491	2.52