
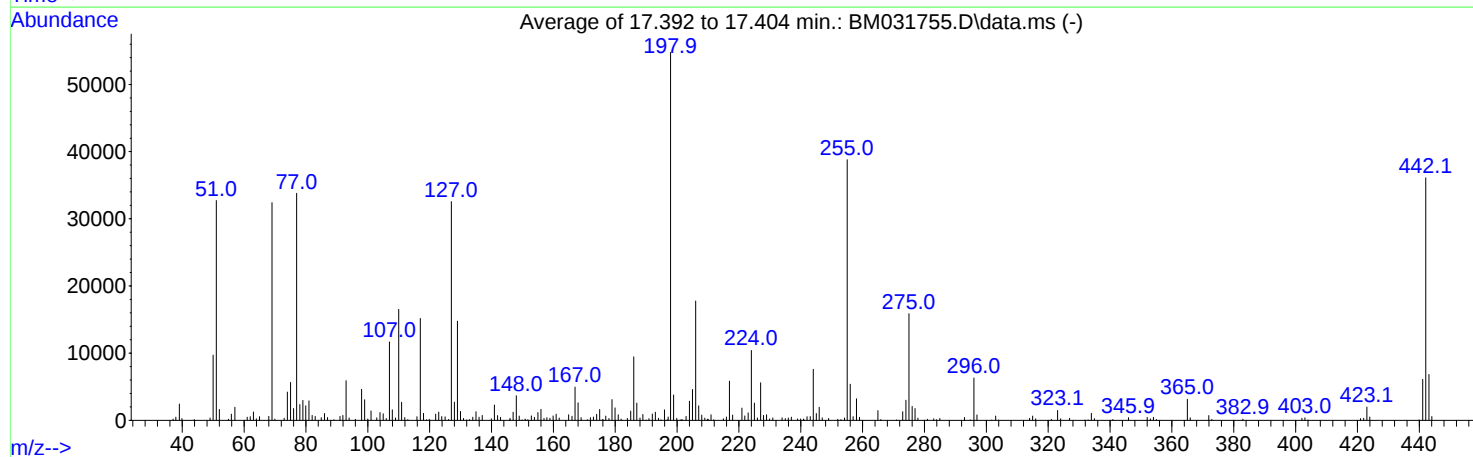


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081621\
 Data File : BM031755.D
 Acq On : 16 Aug 2021 17:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 16 16:42:38 2021

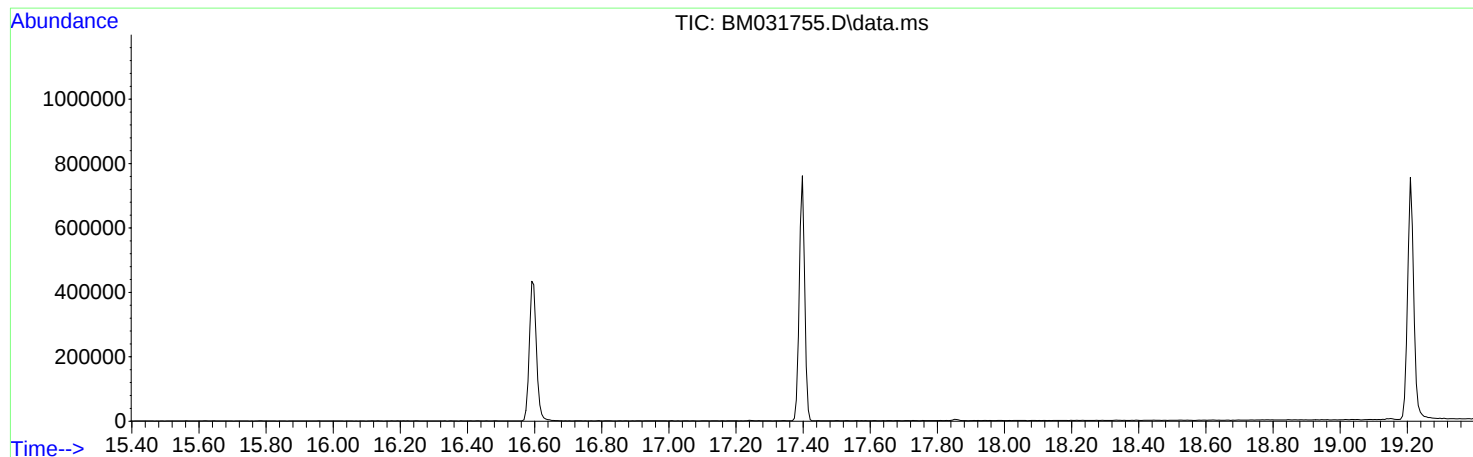




AutoFind: Scans 2432, 2433, 2434; Background Corrected with Scan 2426

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.8	32733	PASS
68	69	0.00	2	1.8	588	PASS
69	198	0.00	100	59.2	32419	PASS
70	69	0.00	2	0.6	199	PASS
127	198	10	80	59.5	32552	PASS
197	198	0.00	2	0.9	511	PASS
198	198	100	100	100.0	54755	PASS
199	198	5	9	6.9	3783	PASS
275	198	10	60	29.0	15892	PASS
365	198	1	100	5.7	3142	PASS
441	198	0.01	100	11.1	6098	PASS
442	442	50	100	100.0	36099	PASS
443	442	15	24	18.9	6834	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081621\
Data File : BM031755.D
Acq On : 16 Aug 2021 17:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 16 18:35:45 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 16 16:42:38 2021
Response via : Initial Calibration

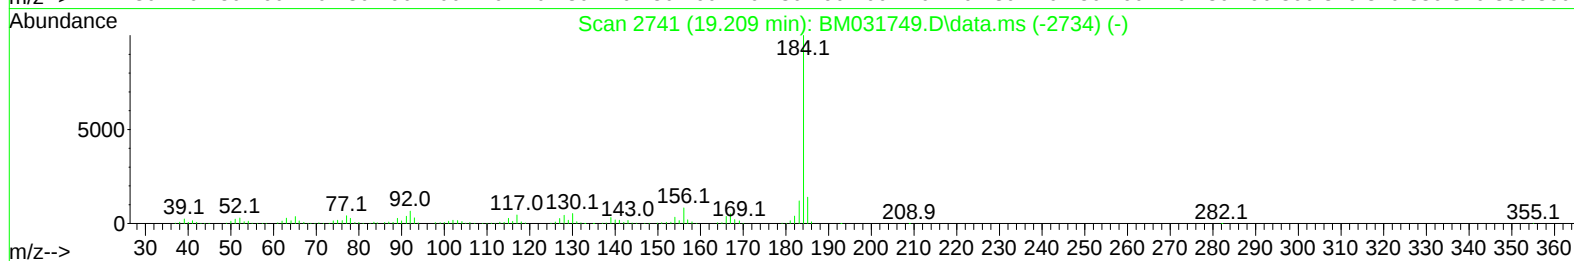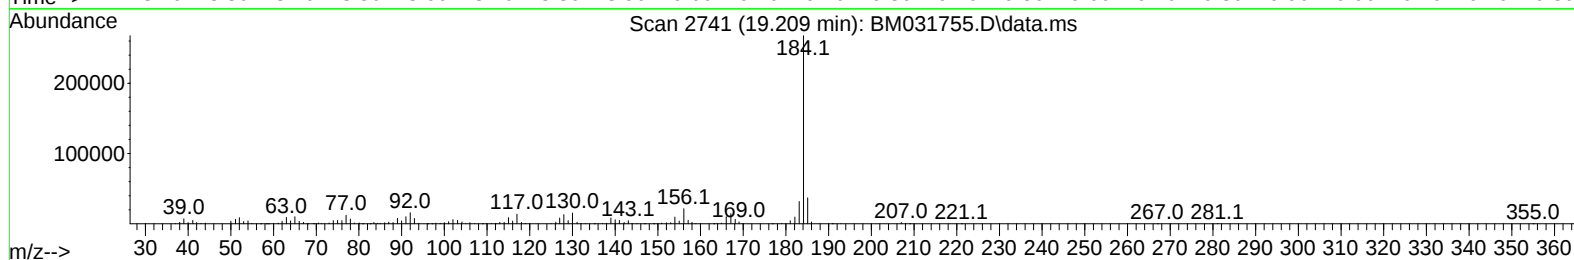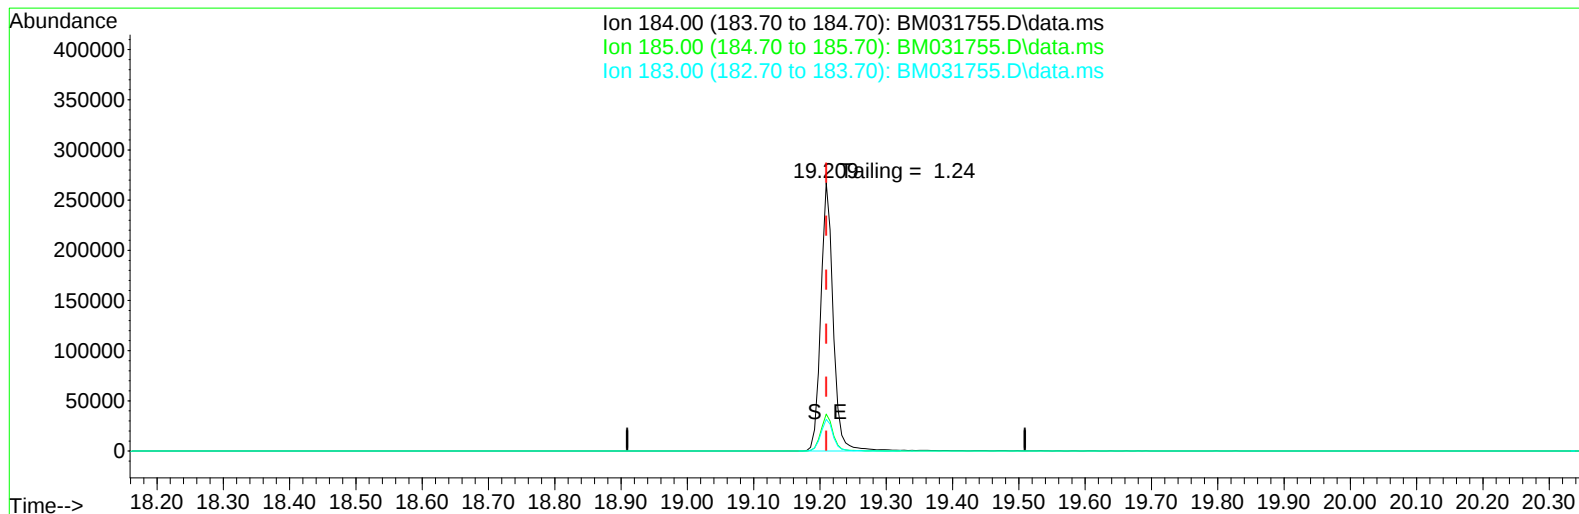

TIC: BM031755.D\data.ms

(77) Benzidine

19.209min (+ 0.000) 0.00 ng




response 347646

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.80
183.00	12.30	11.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081621\
Data File : BM031755.D
Acq On : 16 Aug 2021 17:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 16 18:35:45 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 16 16:42:38 2021
Response via : Initial Calibration

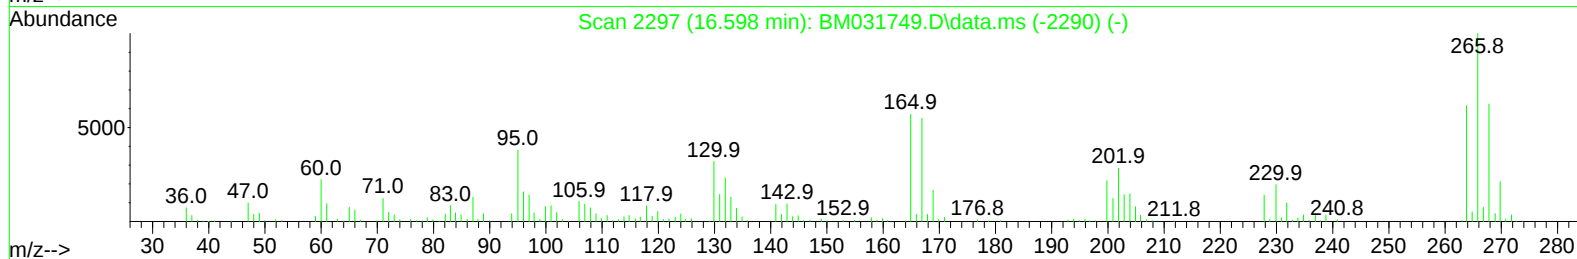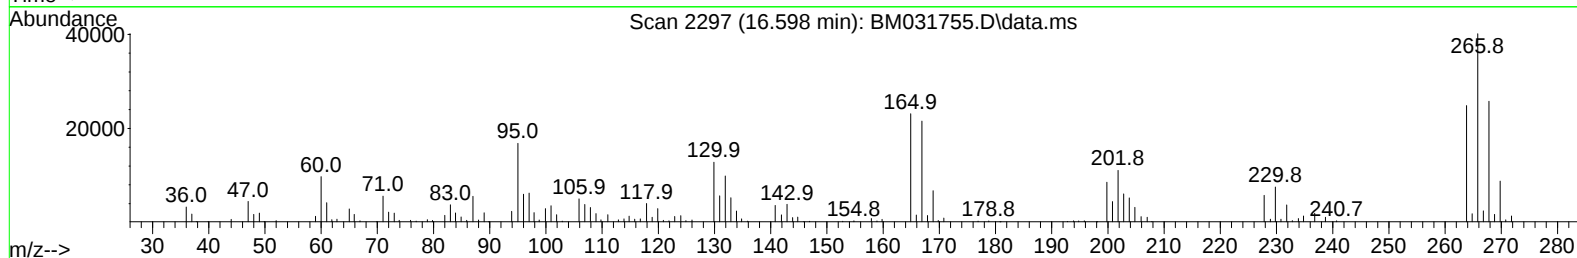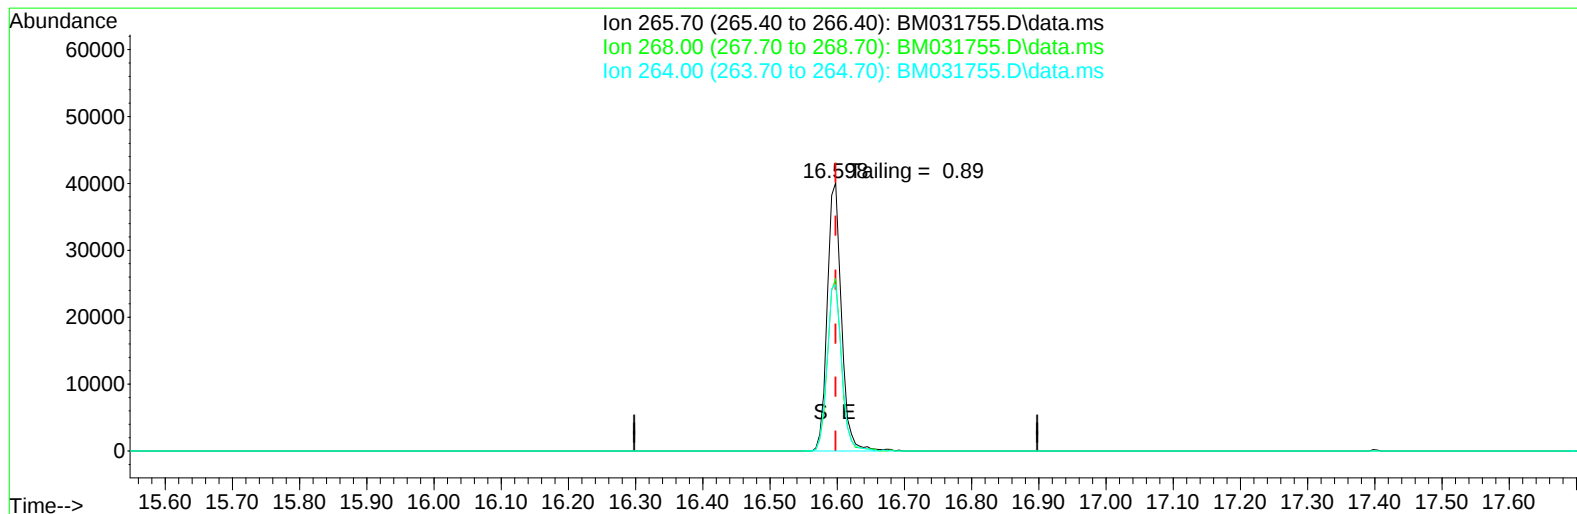

TIC: BM031755.D\data.ms

(70) Pentachlorophenol (C)

16.598min (+ 0.000) 0.00 ng

response 58735

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	64.25
264.00	64.90	61.93
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/16/2021	BNA_M	<u>BM031755.D</u>
Compound Name	Response	Retention Time
DDT	203197	20.44
DDD	9123	20.04
DDE	152	19.49
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9275	212472	4.37

Instrument :
BNA_M
ClientSampleId :
DFTPP