

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081721\
 Data File : BM031777.D
 Acq On : 17 Aug 2021 11:45
 Operator : CG/JU
 Sample : PB138394BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB138394BL

Quant Time: Aug 17 12:18:21 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 16 16:42:38 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.551	152	37933	20.000	ng	0.00
21) Naphthalene-d8	10.310	136	149107	20.000	ng	# 0.00
39) Acenaphthene-d10	14.186	164	97752	20.000	ng	0.00
64) Phenanthrene-d10	16.939	188	215234	20.000	ng	0.00
76) Chrysene-d12	21.139	240	202986	20.000	ng	0.00
86) Perylene-d12	23.285	264	179418	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.187	112	236110	99.901	ng	0.00
7) Phenol-d6	6.745	99	288475	84.234	ng	0.00
23) Nitrobenzene-d5	8.698	82	316059	88.753	ng	0.00
42) 2,4,6-Tribromophenol	15.686	330	92497	76.828	ng	0.00
45) 2-Fluorobiphenyl	12.798	172	665847	90.663	ng	0.00
79) Terphenyl-d14	19.586	244	1307875	108.559	ng	0.00
Target Compounds						
15) Benzyl Alcohol	7.863	79	5936	2.013	ng	# 47


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081721\
Data File : BM031777.D
Acq On : 17 Aug 2021 11:45
Operator : CG/JU
Sample : PB138394BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB138394BL

Quant Time: Aug 17 12:18:21 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 16 16:42:38 2021
Response via : Initial Calibration




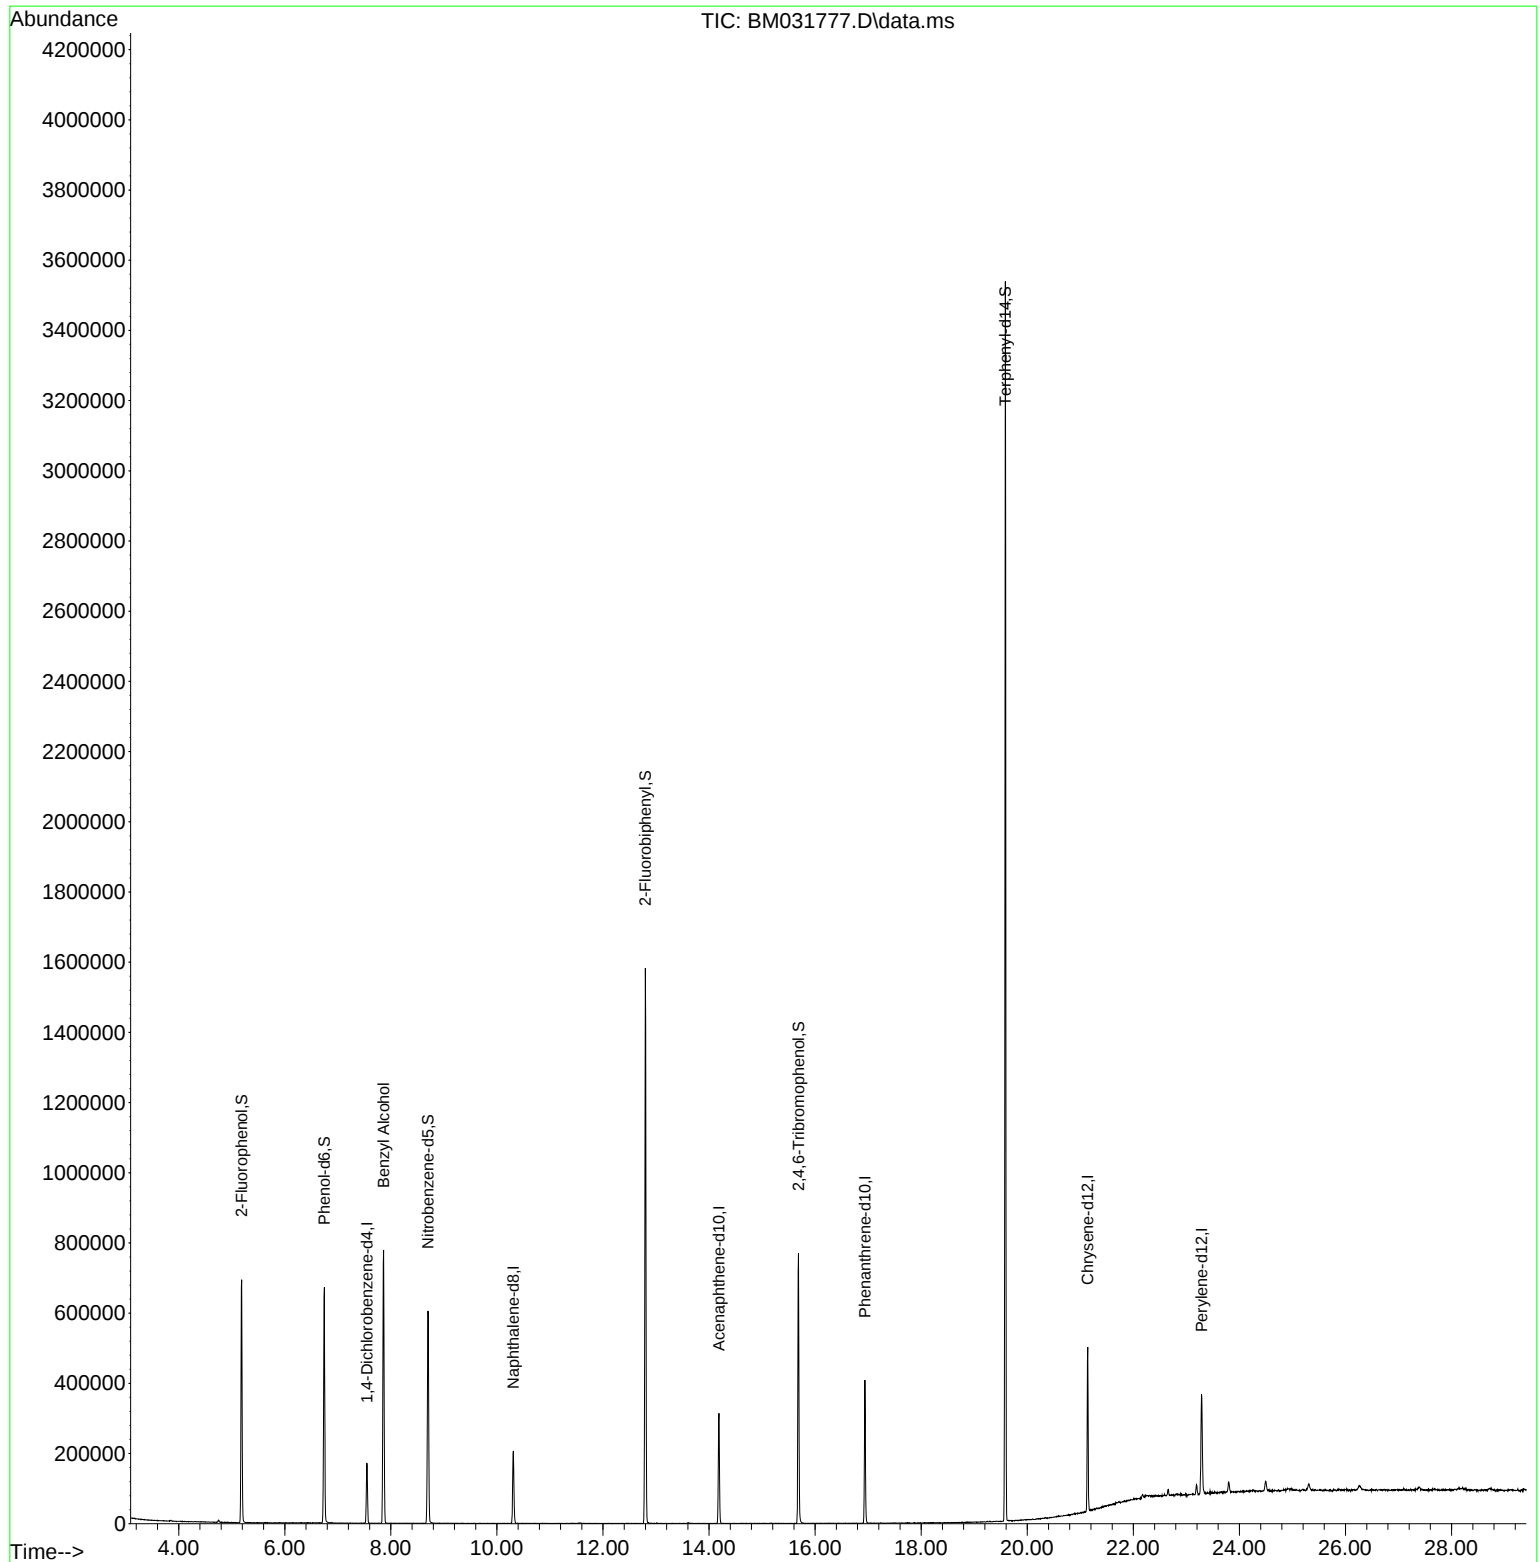


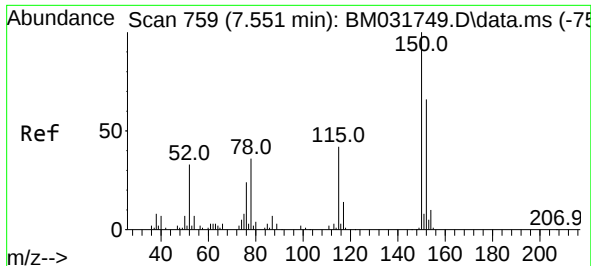

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.551 min Scan# 759
Delta R.T. 0.000 min
Lab File: BM031777.D
Acq: 17 Aug 2021 11:45




Instrument :
BNA_M
ClientSampleId :
PB138394BL


Tgt Ion:152 Resp: 37933
Ion Ratio Lower Upper
152 100
150 144.4 125.9 188.9
115 59.1 44.6 67.0

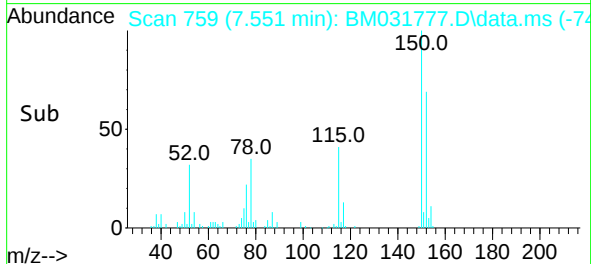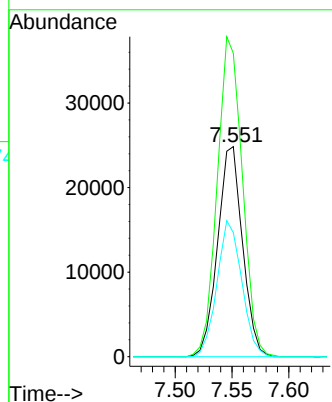

#5
2-Fluorophenol
Concen: 99.901 ng
RT: 5.187 min Scan# 357
Delta R.T. 0.000 min
Lab File: BM031777.D
Acq: 17 Aug 2021 11:45

Tgt Ion:112 Resp: 236110
Ion Ratio Lower Upper
112 100
64 62.2 47.1 70.7
63 39.7 27.3 40.9


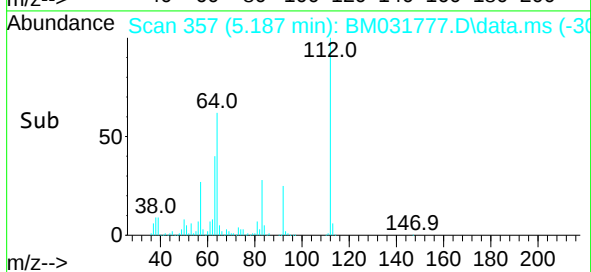
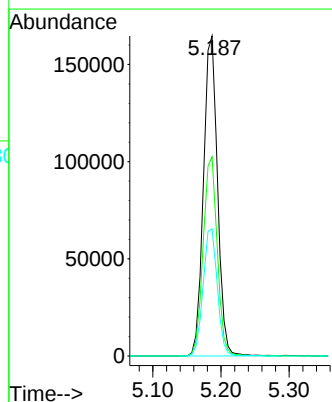
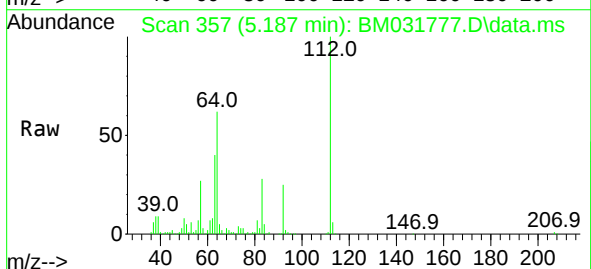


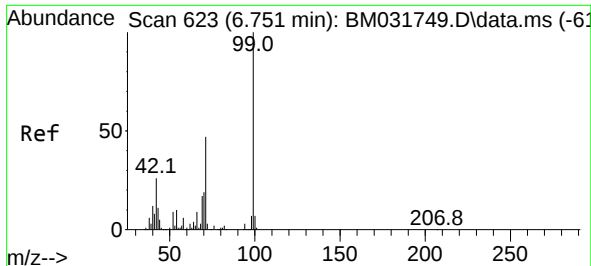

#7
Phenol-d6
Concen: 84.234 ng
RT: 6.745 min Scan# 622
Delta R.T. -0.006 min
Lab File: BM031777.D
Acq: 17 Aug 2021 11:45




Instrument :
BNA_M
ClientSampleId :
PB138394BL


Tgt Ion: 99 Resp: 288475
Ion Ratio Lower Upper
99 100
42 28.1 18.0 27.0#
71 49.3 30.9 46.3#

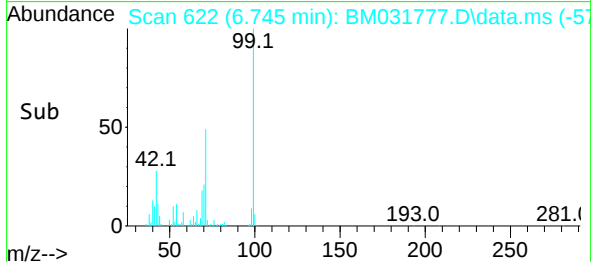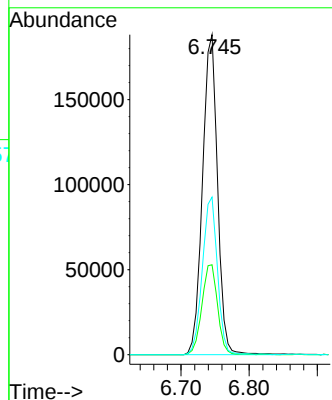

#15
Benzyl Alcohol
Concen: 2.013 ng
RT: 7.863 min Scan# 812
Delta R.T. 0.059 min
Lab File: BM031777.D
Acq: 17 Aug 2021 11:45

Tgt Ion: 79 Resp: 5936
Ion Ratio Lower Upper
79 100
108 49.9 57.0 85.4#
77 134.5 54.6 81.8#


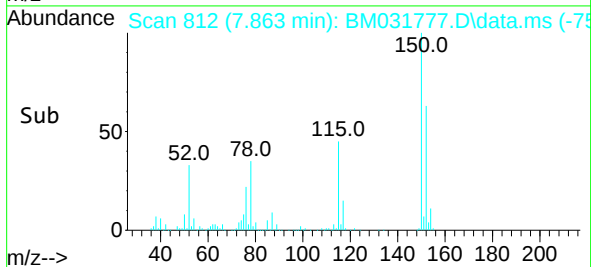
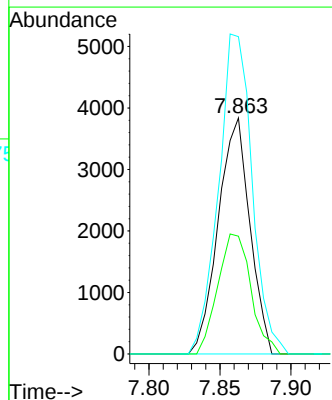
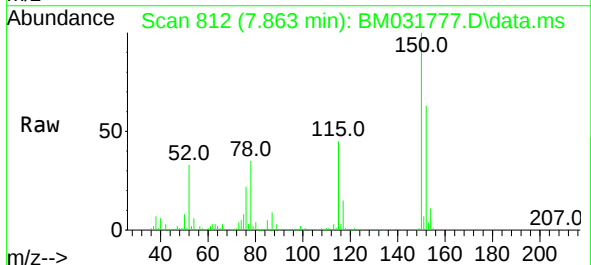


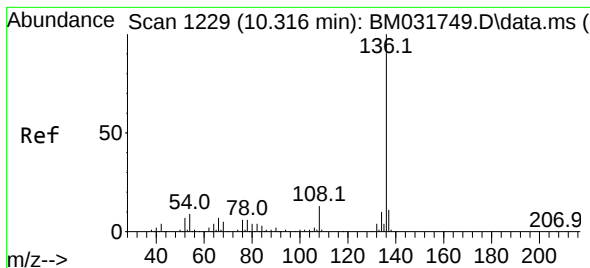

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.310 min Scan# 1228
Delta R.T. -0.006 min
Lab File: BM031777.D
Acq: 17 Aug 2021 11:45




Instrument :
BNA_M
ClientSampleId :
PB138394BL


Tgt Ion:	136	Resp:	149107
Ion Ratio	Lower	Upper	
136	100		
137	10.5	8.4	12.6
54	9.0	5.5	8.3#
68	4.2	4.2	6.2

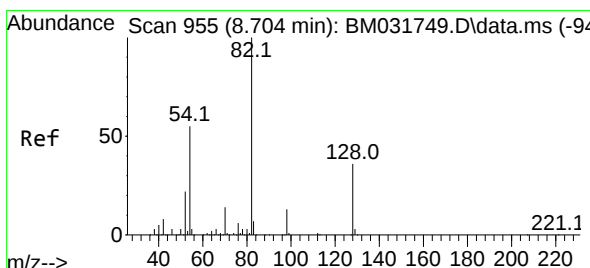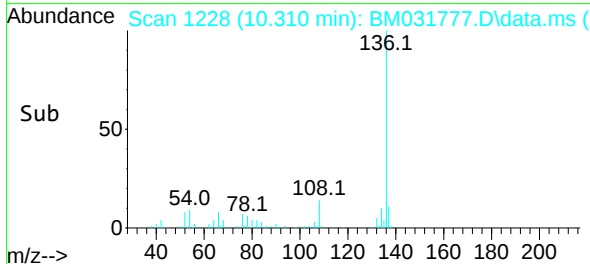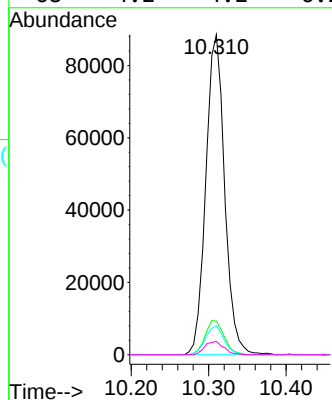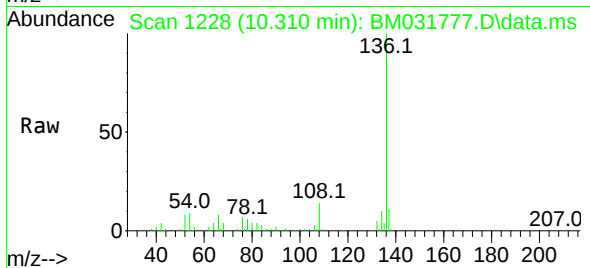

#23
Nitrobenzene-d5
Concen: 88.753 ng
RT: 8.698 min Scan# 954
Delta R.T. -0.006 min
Lab File: BM031777.D
Acq: 17 Aug 2021 11:45

Tgt Ion:	82	Resp:	316059
Ion Ratio	Lower	Upper	
82	100		
128	36.8	31.1	46.7
54	59.7	37.3	55.9#


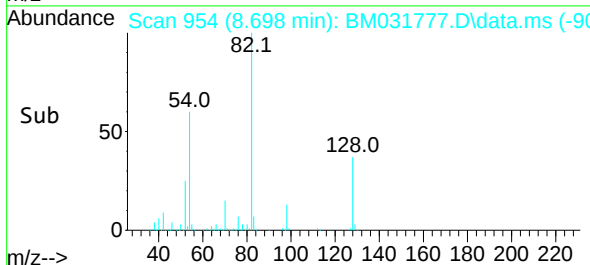
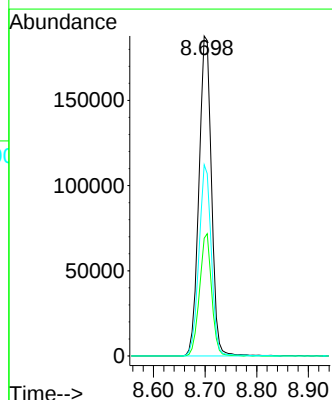
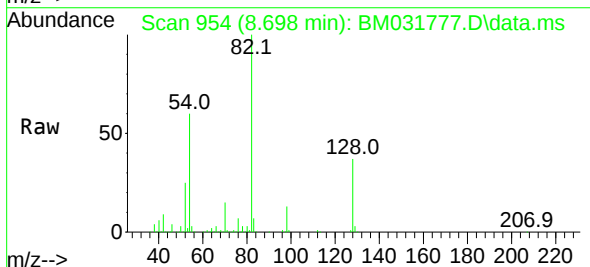


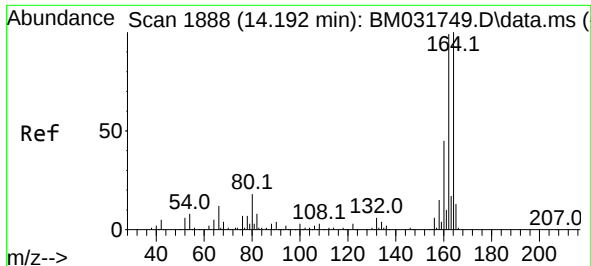

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.186 min Scan# 1887
Delta R.T. -0.006 min
Lab File: BM031777.D
Acq: 17 Aug 2021 11:45




Instrument :
BNA_M
ClientSampleId :
PB138394BL


Tgt Ion:164 Resp: 97752
Ion Ratio Lower Upper
164 100
162 101.3 83.4 125.0
160 45.9 37.2 55.8

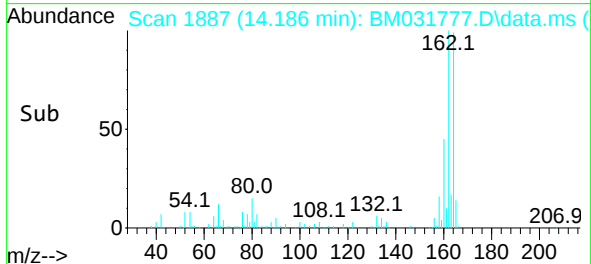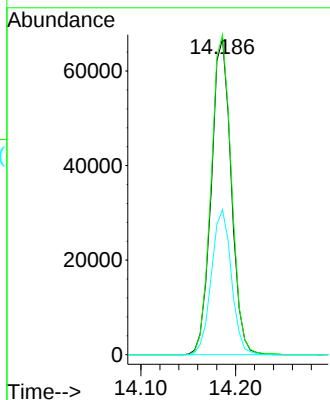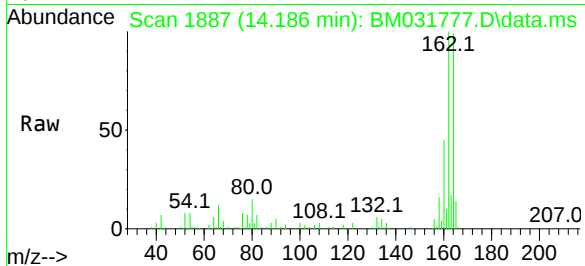

#42
2,4,6-Tribromophenol
Concen: 76.828 ng
RT: 15.686 min Scan# 2142
Delta R.T. -0.006 min
Lab File: BM031777.D
Acq: 17 Aug 2021 11:45

Tgt Ion:330 Resp: 92497
Ion Ratio Lower Upper
330 100
332 96.6 77.0 115.4
141 61.4 30.2 45.2#


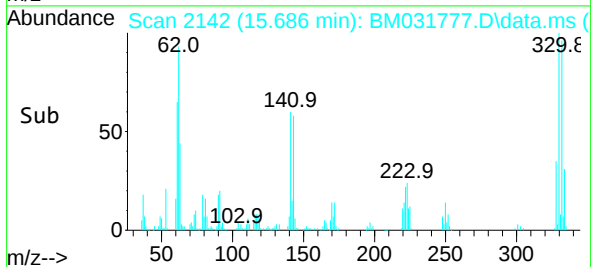
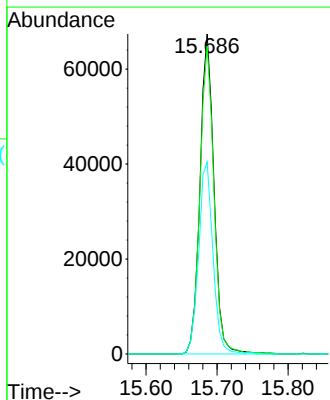
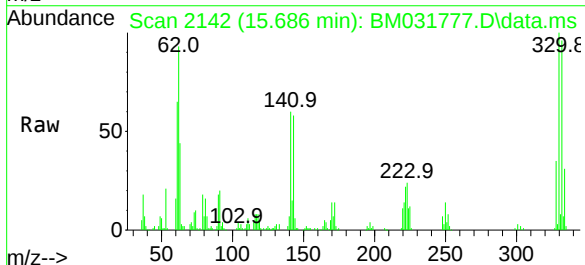




#45
2-Fluorobiphenyl
Concen: 90.663 ng
RT: 12.798 min Scan# 1651
Delta R.T. -0.006 min
Lab File: BM031777.D
Acq: 17 Aug 2021 11:45




Instrument :
BNA_M
ClientSampleId :
PB138394BL


Tgt Ion:172	Resp:	665847
Ion Ratio	Lower	Upper
172	100	
171	35.5	28.6 43.0
170	23.4	18.4 27.6

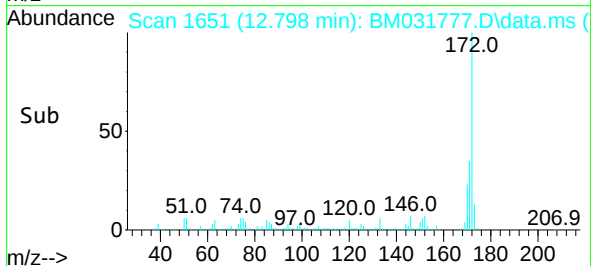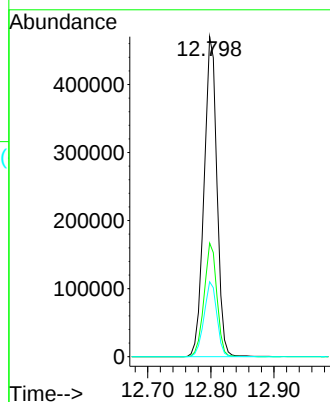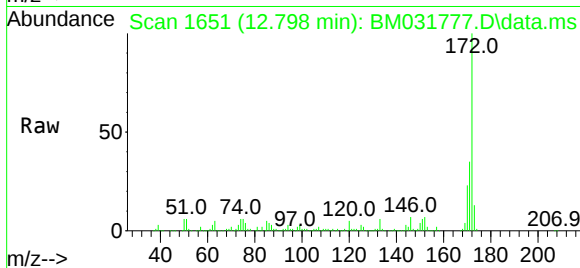

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 16.939 min Scan# 2355
Delta R.T. -0.006 min
Lab File: BM031777.D
Acq: 17 Aug 2021 11:45

Tgt Ion:188	Resp:	215234
Ion Ratio	Lower	Upper
188	100	
94	6.8	6.0 9.0
80	7.7	6.6 9.8

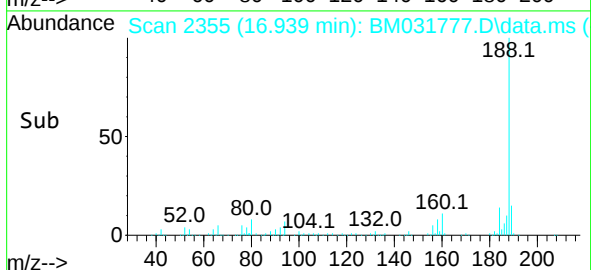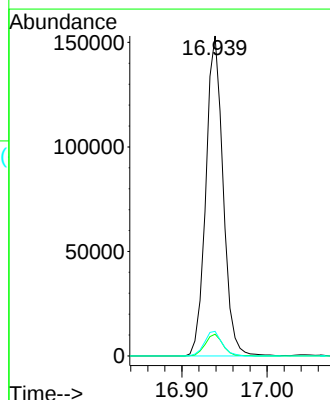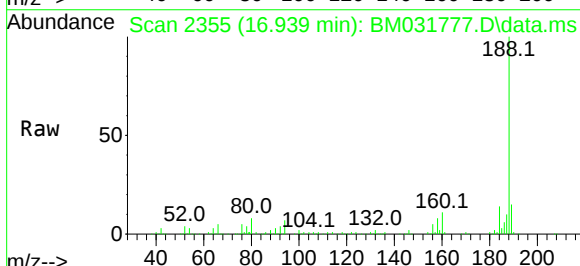



#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.139 min Scan# 3069

Delta R.T. -0.006 min

Lab File: BM031777.D

Acq: 17 Aug 2021 11:45





Tgt Ion:240 Resp: 202986

Ion Ratio Lower Upper

240 100

120 8.3 7.0 10.6

236 26.4 21.0 31.4

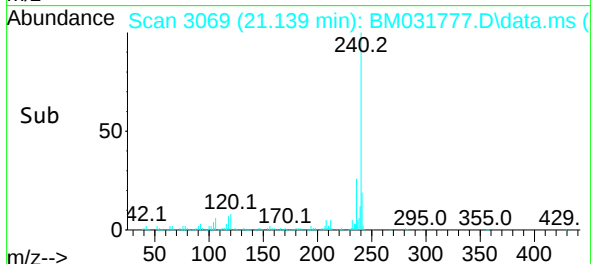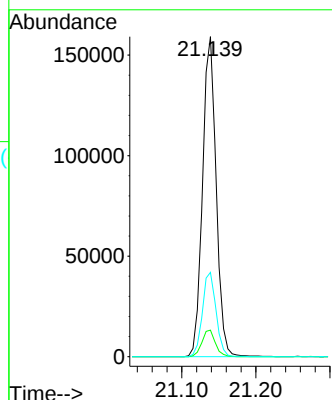

#79

Terphenyl-d14

Concen: 108.559 ng

RT: 19.586 min Scan# 2805

Delta R.T. -0.006 min

Lab File: BM031777.D

Acq: 17 Aug 2021 11:45




Tgt Ion:244 Resp: 1307875


Ion Ratio Lower Upper

244 100

212 8.3 6.3 9.5

122 10.6 6.9 10.3#

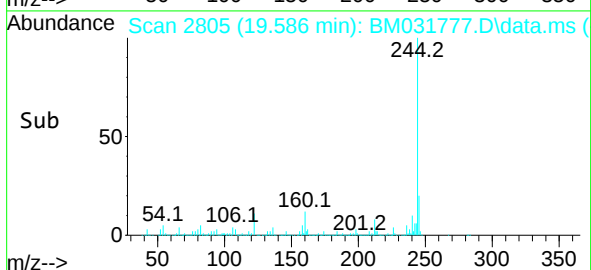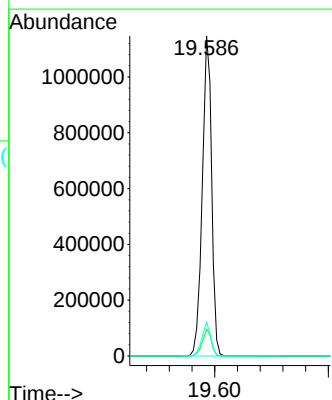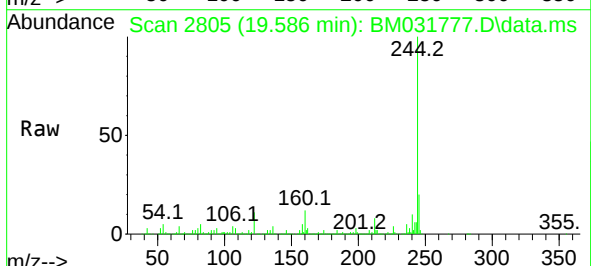

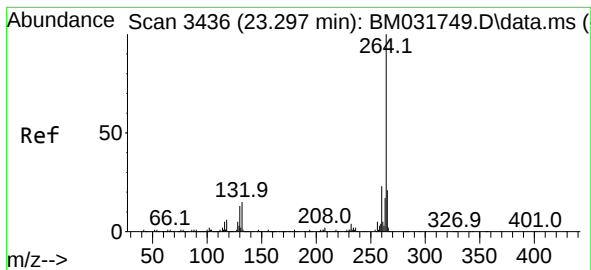

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.285 min Scan# 3434
 Delta R.T. -0.012 min
 Lab File: BM031777.D
 Acq: 17 Aug 2021 11:45

Instrument :
 BNA_M
 ClientSampleId :
 PB138394BL

Tgt Ion:264 Resp: 179418
 Ion Ratio Lower Upper
 264 100
 260 23.3 19.8 29.8
 265 20.6 17.7 26.5

