


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081721\
 Data File : BM031775.D
 Acq On : 17 Aug 2021 09:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 16 16:42:38 2021

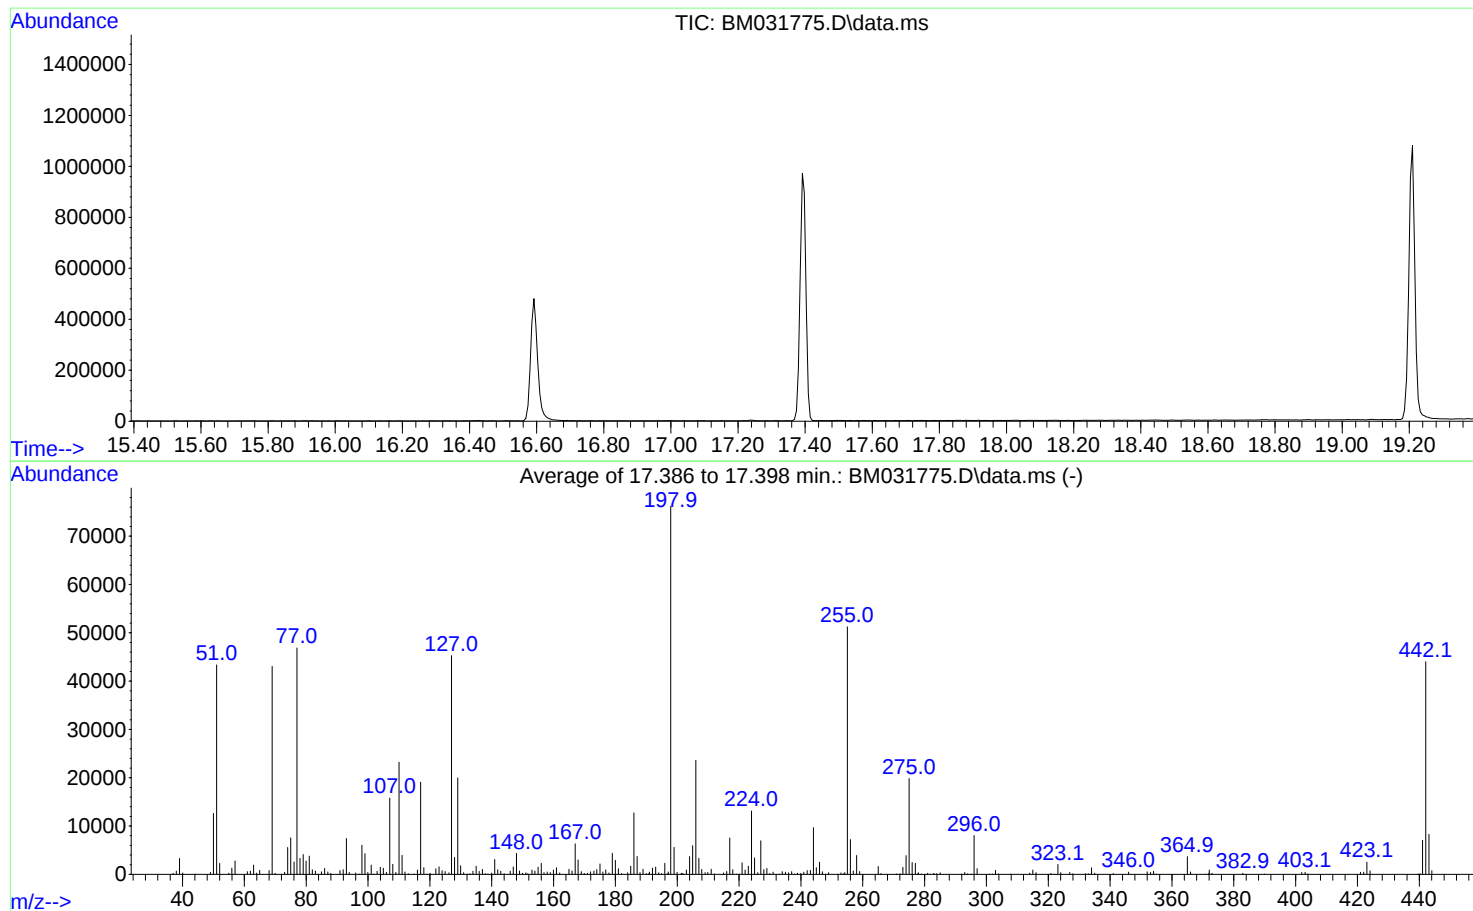




AutoFind: Scans 2431, 2432, 2433; Background Corrected with Scan 2425

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.9	43344	PASS
68	69	0.00	2	1.8	789	PASS
69	198	0.00	100	56.6	43061	PASS
70	69	0.00	2	0.6	240	PASS
127	198	10	80	59.5	45280	PASS
197	198	0.00	2	0.7	495	PASS
198	198	100	100	100.0	76141	PASS
199	198	5	9	7.4	5605	PASS
275	198	10	60	26.0	19824	PASS
365	198	1	100	4.8	3672	PASS
441	198	0.01	100	9.3	7059	PASS
442	442	50	100	100.0	44021	PASS
443	442	15	24	18.8	8292	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081721\
 Data File : BM031775.D
 Acq On : 17 Aug 2021 09:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Aug 17 12:14:54 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 16 16:42:38 2021
 Response via : Initial Calibration

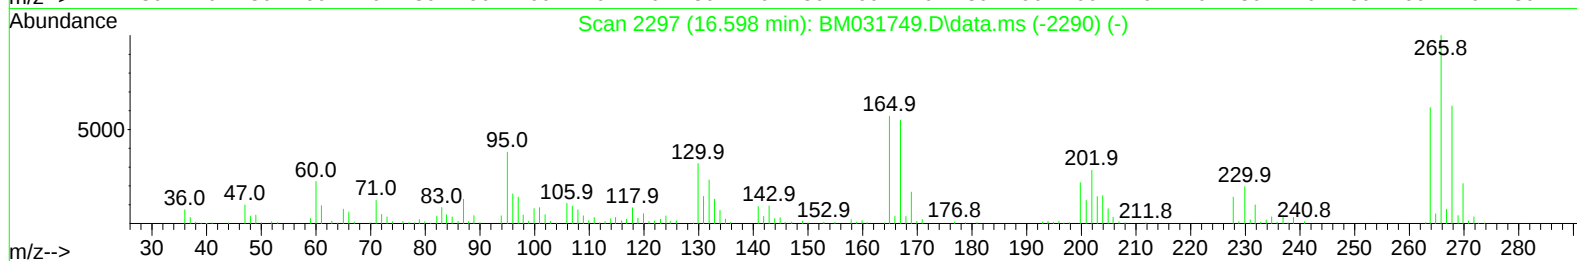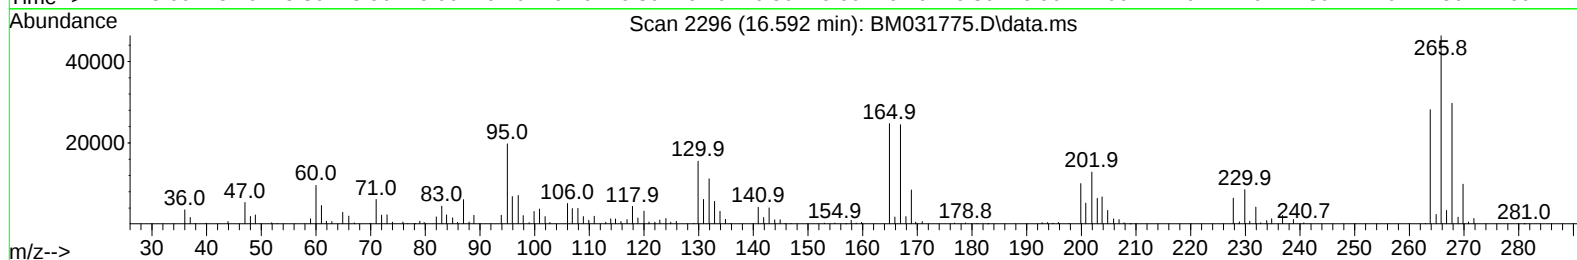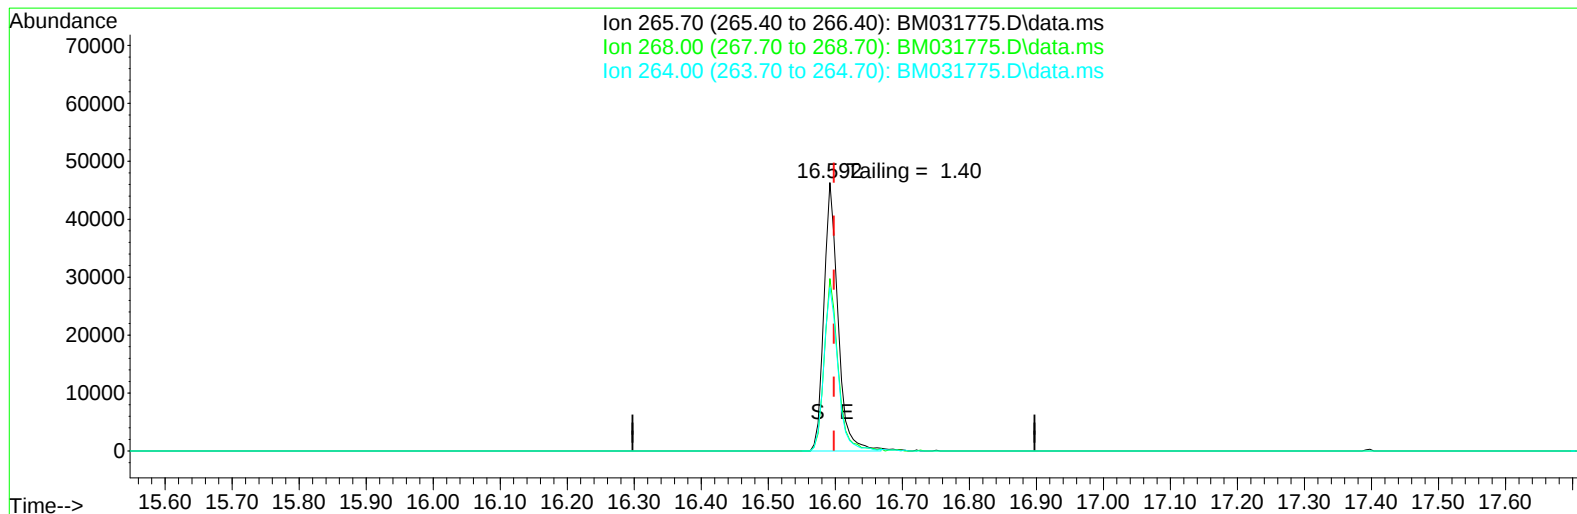

TIC: BM031775.D\data.ms

(70) Pentachlorophenol (C)

16.592min (-0.006) 0.00 ng




response 68482

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	64.21
264.00	64.90	60.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081721\
Data File : BM031775.D
Acq On : 17 Aug 2021 09:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 17 12:14:54 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 16 16:42:38 2021
Response via : Initial Calibration

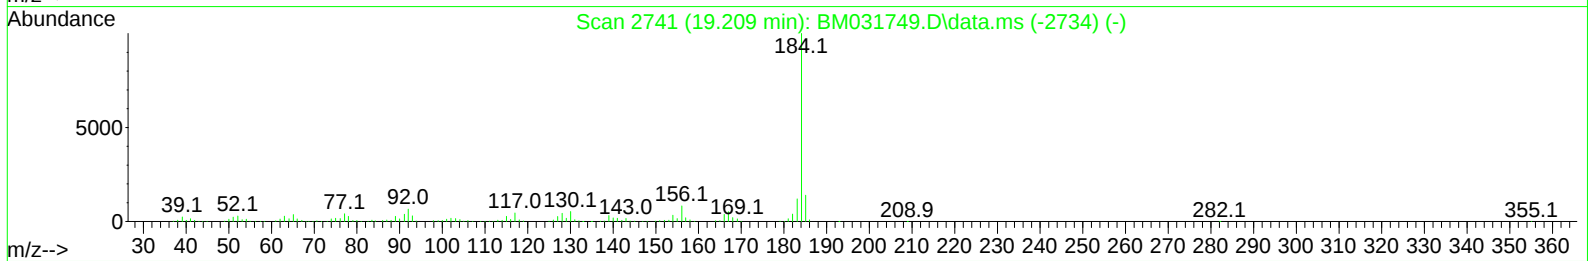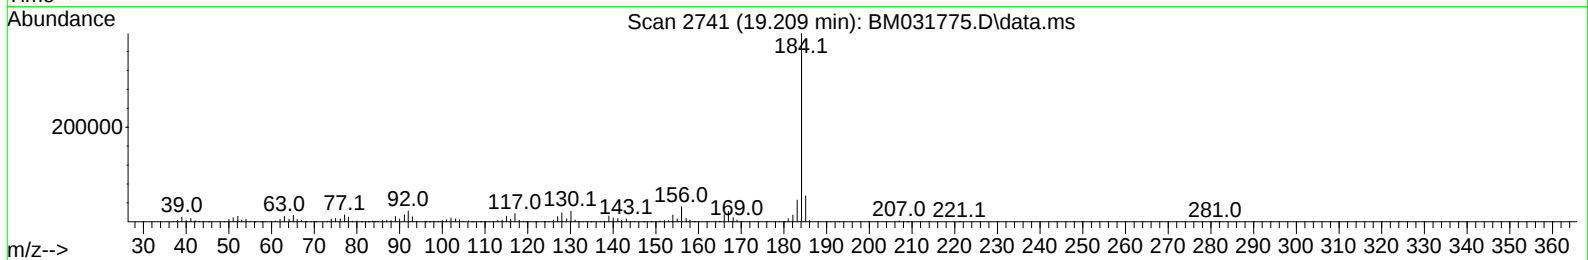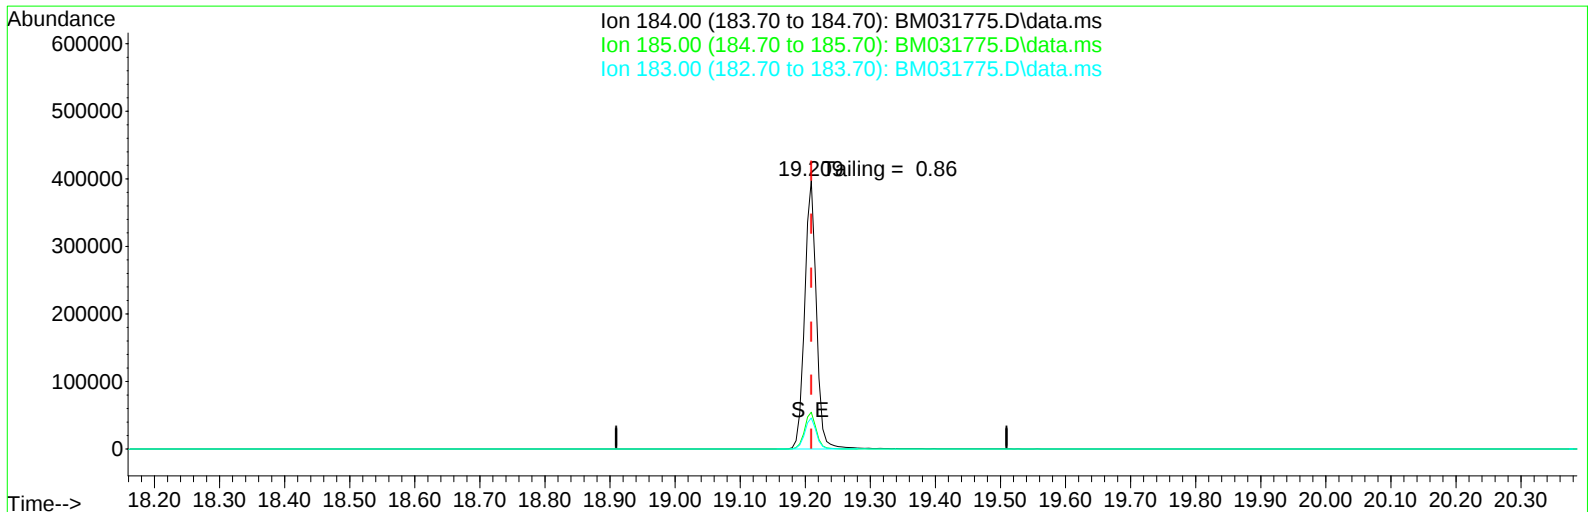

TIC: BM031775.D\data.ms

(77) Benzidine

19.209min (+ 0.000) 0.00 ng

response 501271

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.74
183.00	12.30	11.57
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/17/2021	BNA_M	<u>BM031775.D</u>
Compound Name	Response	Retention Time
DDT	258383	20.43
DDD	13222	20
DDE	1014	19.49
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14236	272619	5.22

Instrument :
BNA_M
ClientSampleId :
DFTPP