


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081721\
 Data File : BM031783.D
 Acq On : 17 Aug 2021 16:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 16 16:42:38 2021

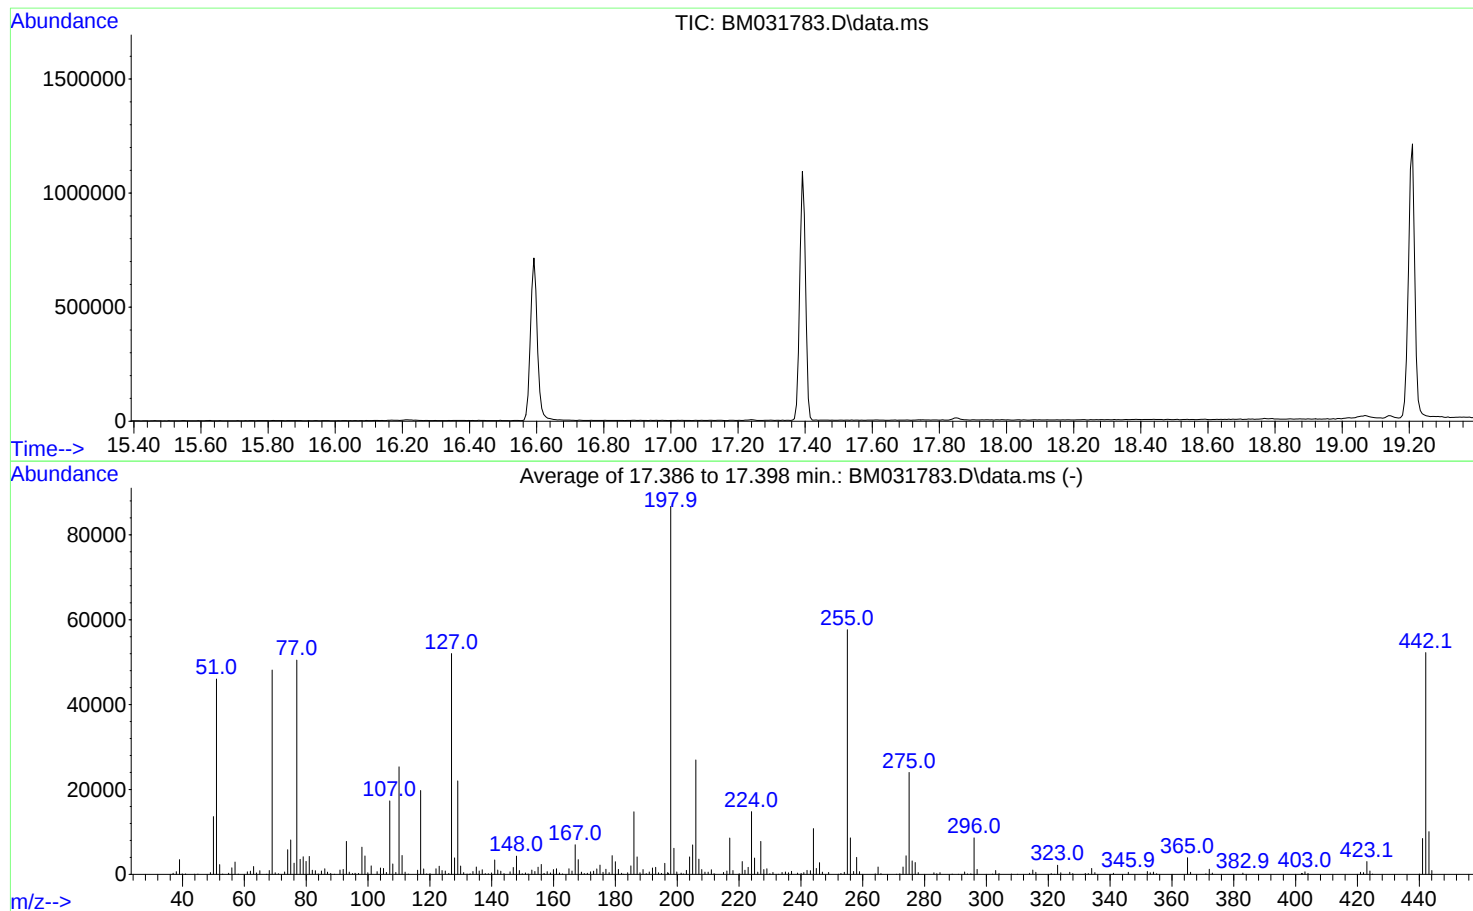




AutoFind: Scans 2431, 2432, 2433; Background Corrected with Scan 2425

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.1	46045	PASS
68	69	0.00	2	1.9	922	PASS
69	198	0.00	100	55.6	48155	PASS
70	69	0.00	2	0.8	362	PASS
127	198	10	80	60.0	52045	PASS
197	198	0.00	2	0.5	401	PASS
198	198	100	100	100.0	86683	PASS
199	198	5	9	7.1	6130	PASS
275	198	10	60	27.7	24011	PASS
365	198	1	100	4.5	3929	PASS
441	198	0.01	100	9.8	8454	PASS
442	442	50	100	100.0	52264	PASS
443	442	15	24	19.3	10068	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081721\
 Data File : BM031783.D
 Acq On : 17 Aug 2021 16:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Aug 17 17:07:46 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 16 16:42:38 2021
 Response via : Initial Calibration

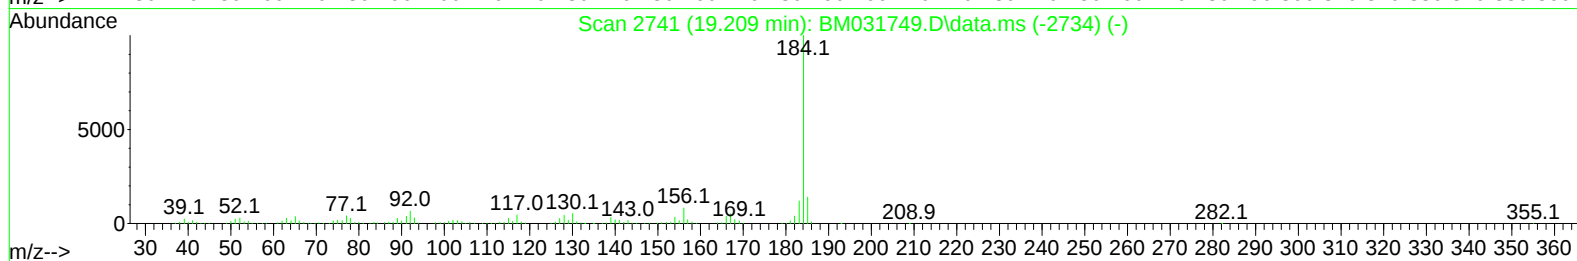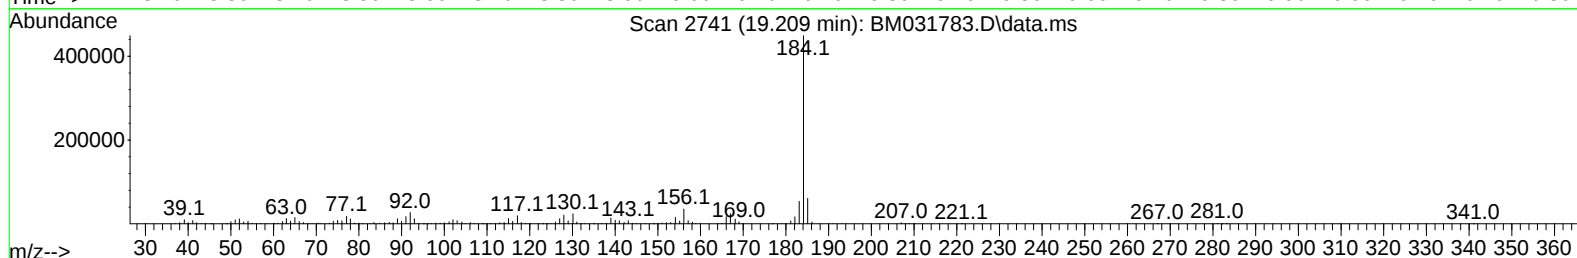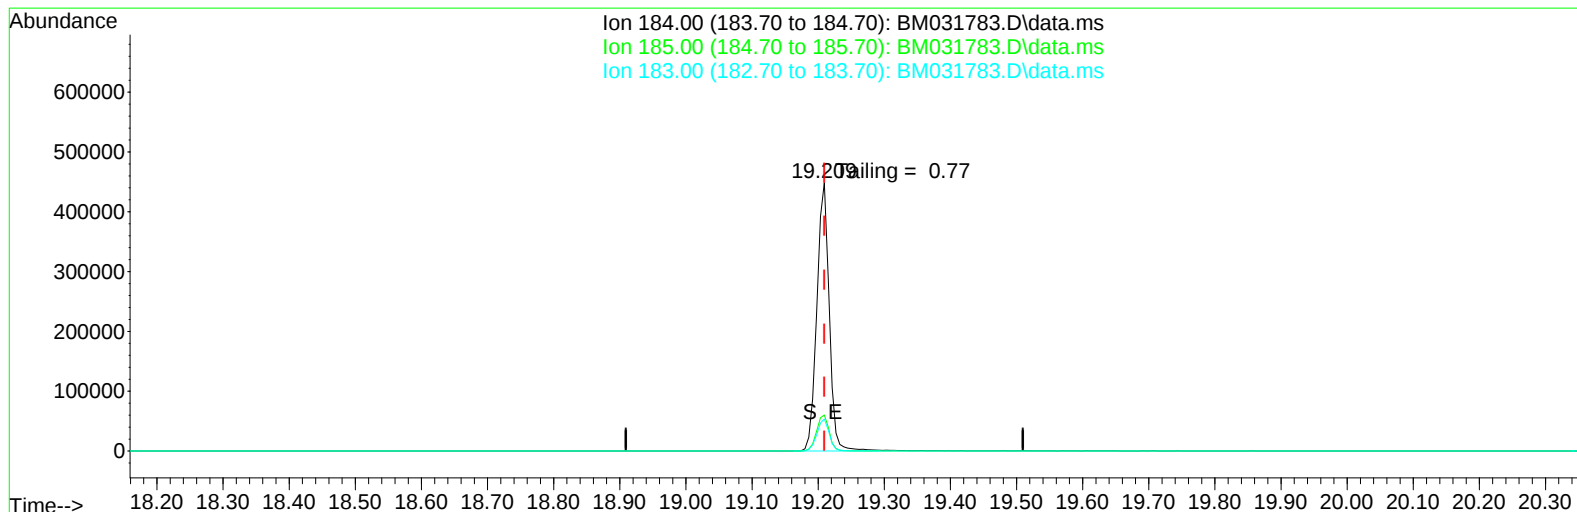

TIC: BM031783.D\data.ms

(77) Benzidine

19.209min (0.000) 131955.97 ng




response 584281

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.45
183.00	12.30	11.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081721\
Data File : BM031783.D
Acq On : 17 Aug 2021 16:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 17 17:07:46 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 16 16:42:38 2021
Response via : Initial Calibration

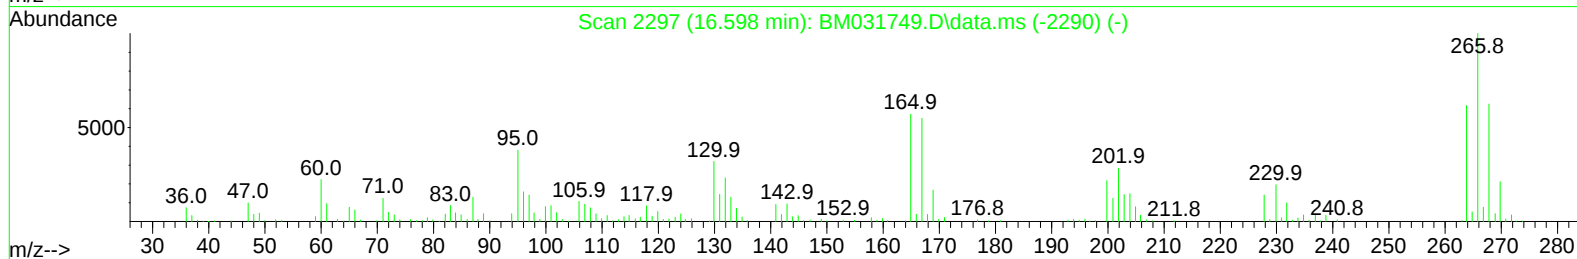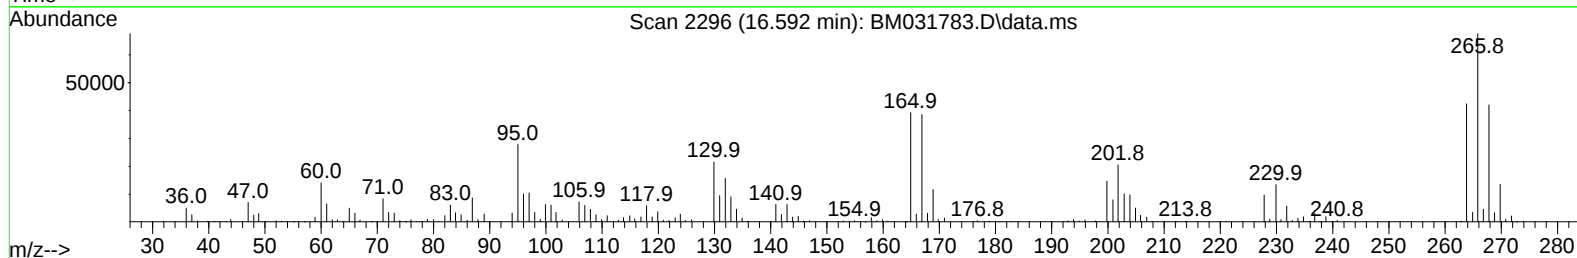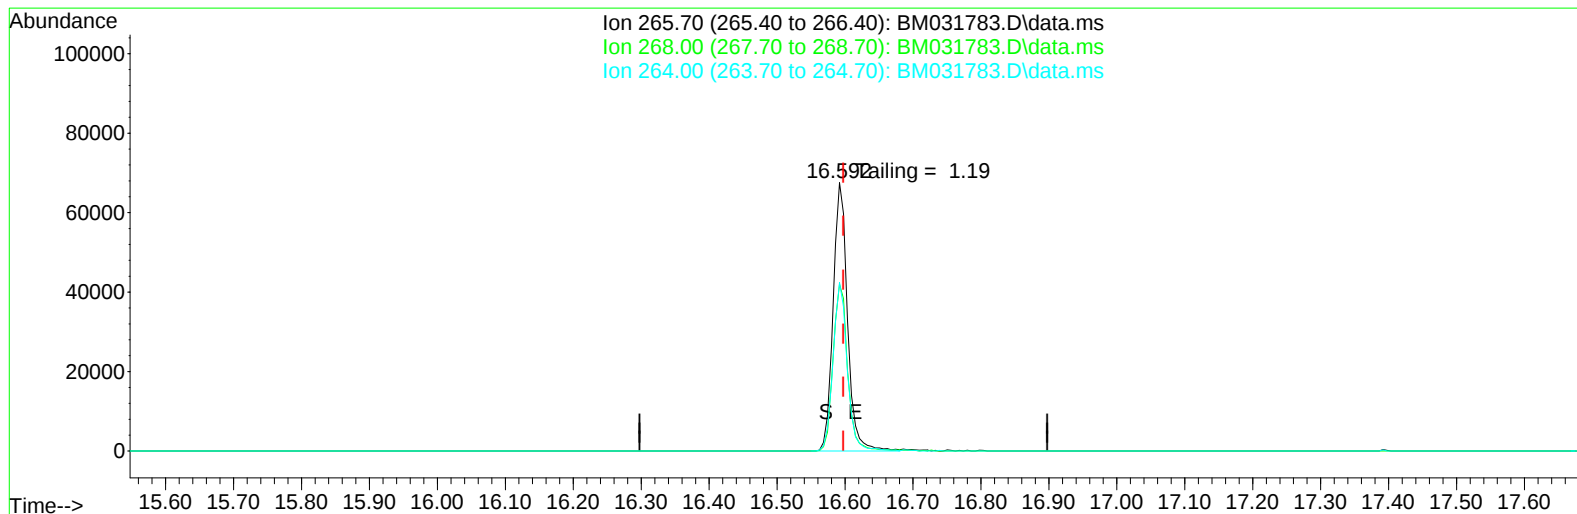

TIC: BM031783.D\data.ms

(70) Pentachlorophenol (C)

16.592min (-0.006) 0.00 ng

response 99464

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	62.21
264.00	64.90	62.79
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/17/2021	BNA_M	<u>BM031783.D</u>
Compound Name	Response	Retention Time
DDT	296791	20.43
DDD	22832	20
DDE	1188	19.48
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24020	320811	7.49

Instrument :
BNA_M
ClientSampleId :
DFTPP