
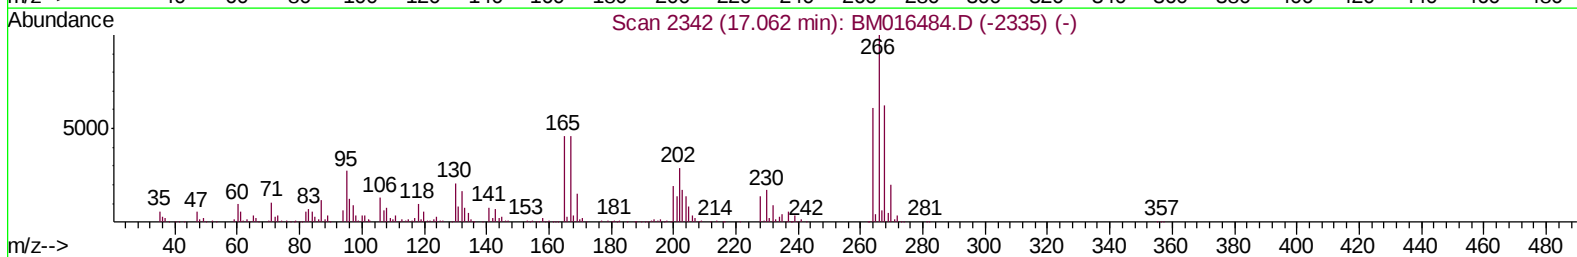
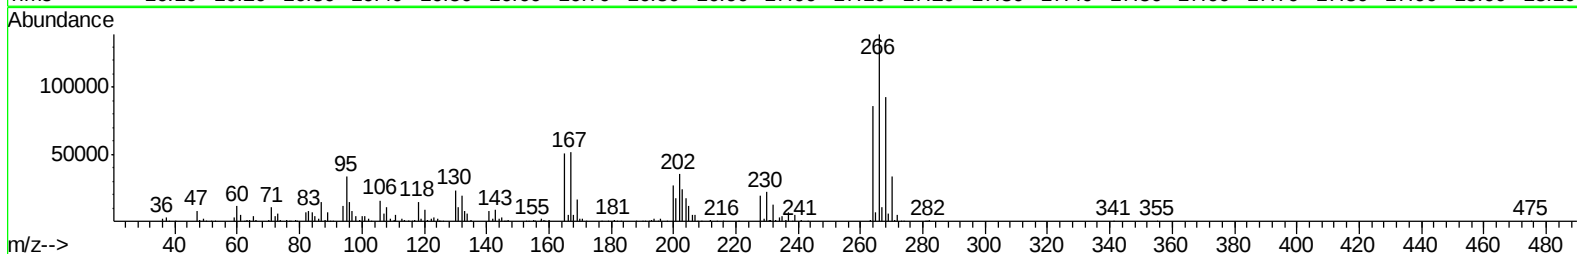


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082218\
Data File : BM016522.D
Acq On : 22 Aug 2018 17:19
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 23 09:21:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 21 16:31:22 2018
Response via : Initial Calibration

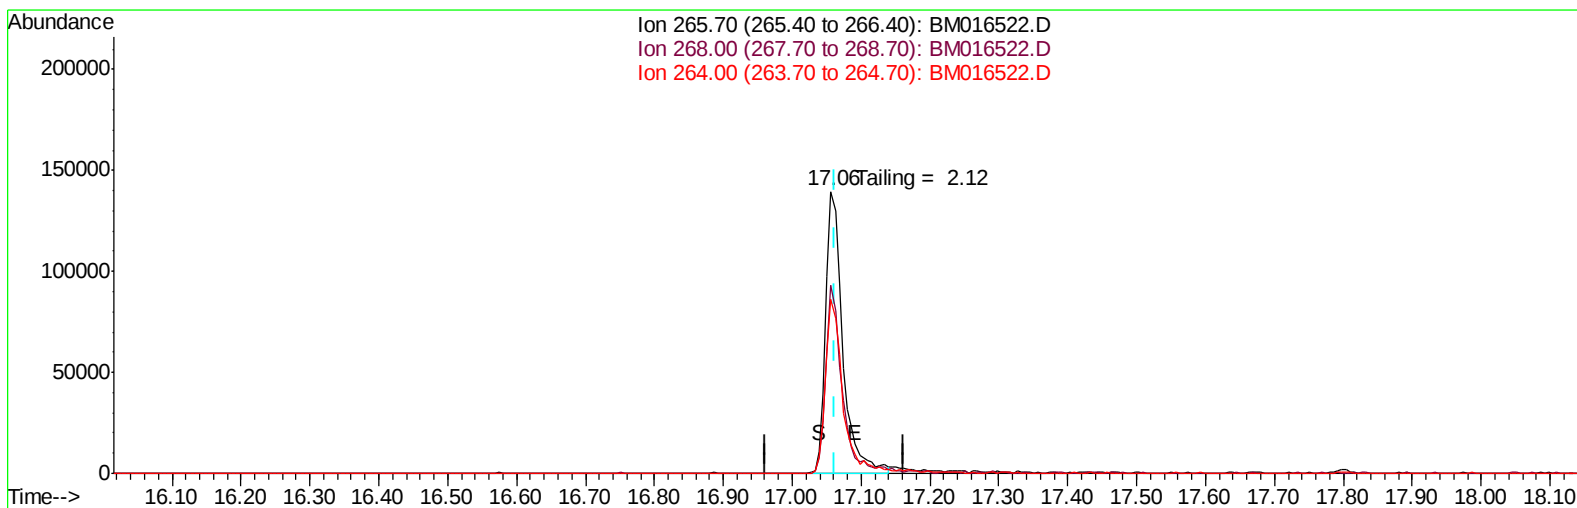

TIC: BM016522.D

(69) Pentachlorophenol (C)




17.057min (-0.006) 0.00ng

response 239607

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	66.82
264.00	61.20	61.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082218\
 Data File : BM016522.D
 Acq On : 22 Aug 2018 17:19
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 23 09:21:20 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 21 16:31:22 2018
 Response via : Initial Calibration

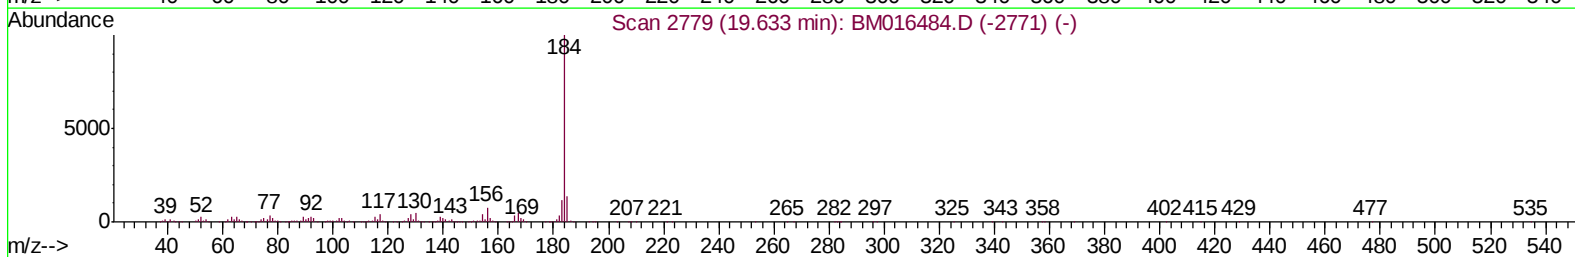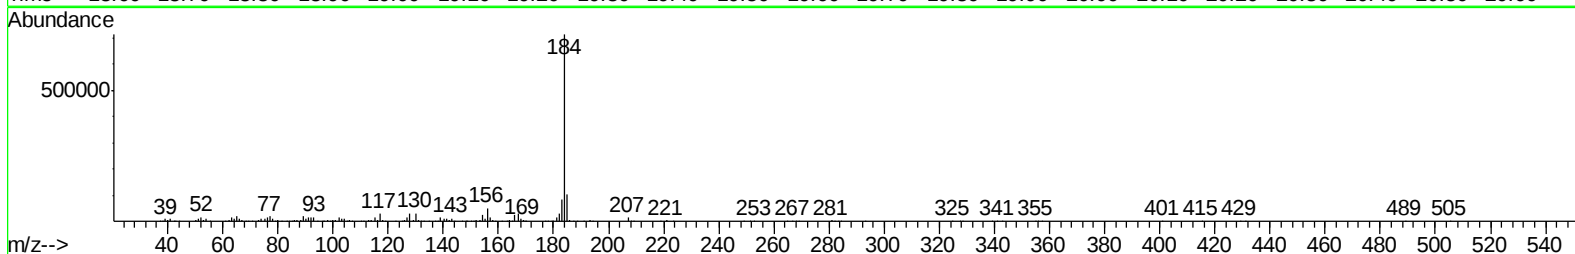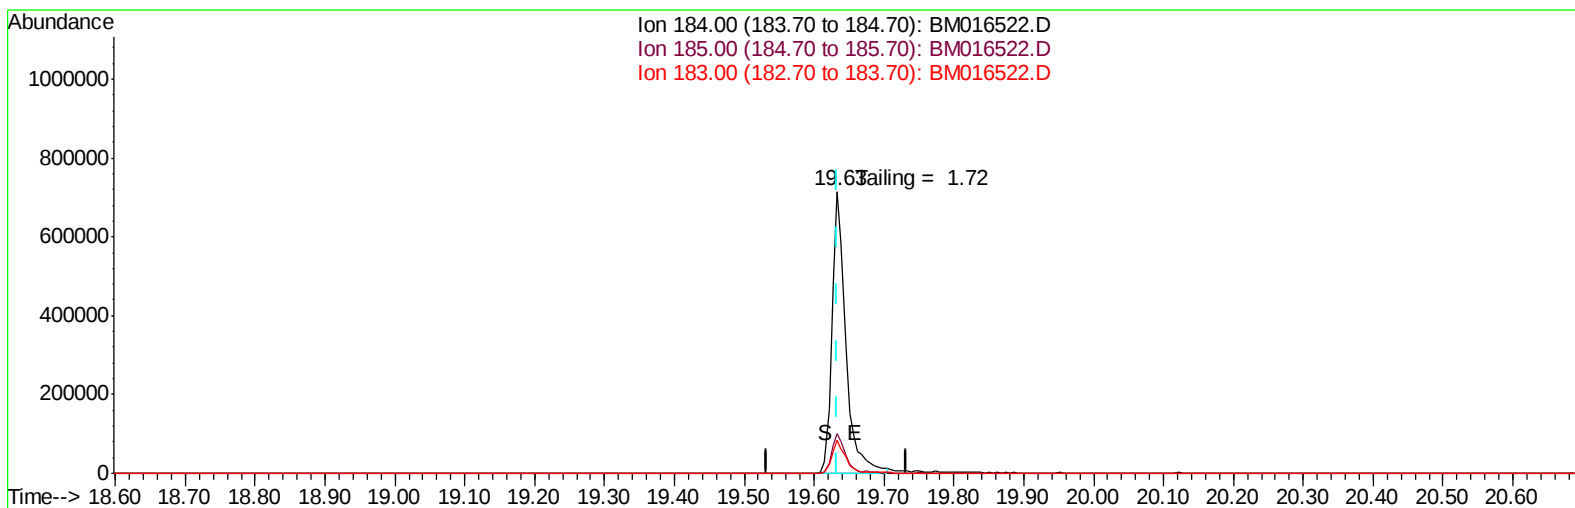

TIC: BM016522.D

(76) Benzidine

19.633min (-0.000) 364836.43ng

response 968235

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.32
183.00	11.10	11.79
0.00	0.00	0.00