
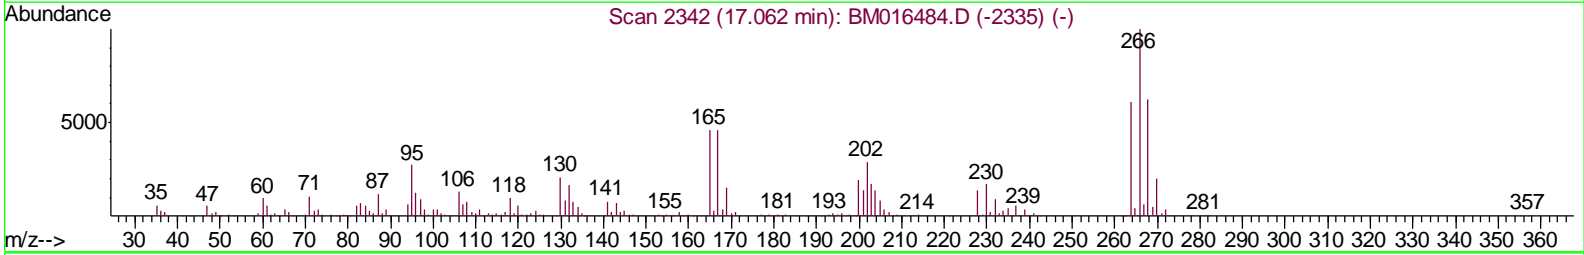
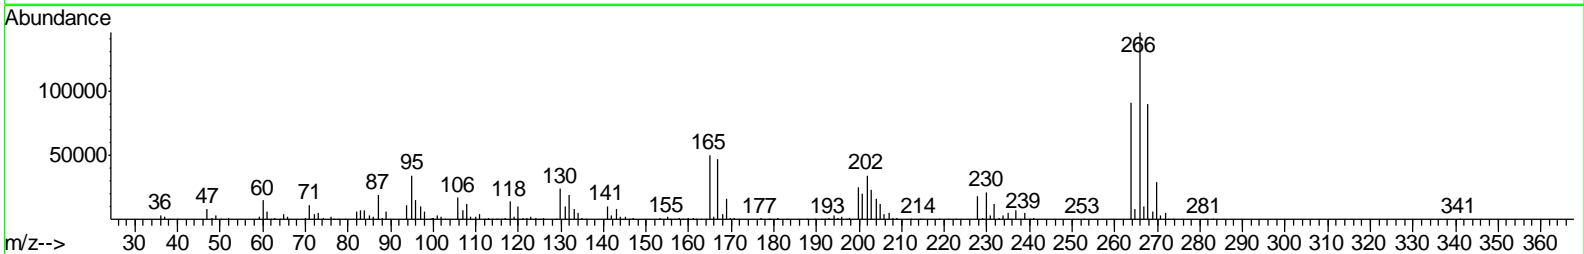


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM082218\  
 Data File : BM016542.D  
 Acq On : 23 Aug 2018 06:38  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 23 09:23:09 2018  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\8270-BM082118.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Aug 21 16:31:22 2018  
 Response via : Initial Calibration

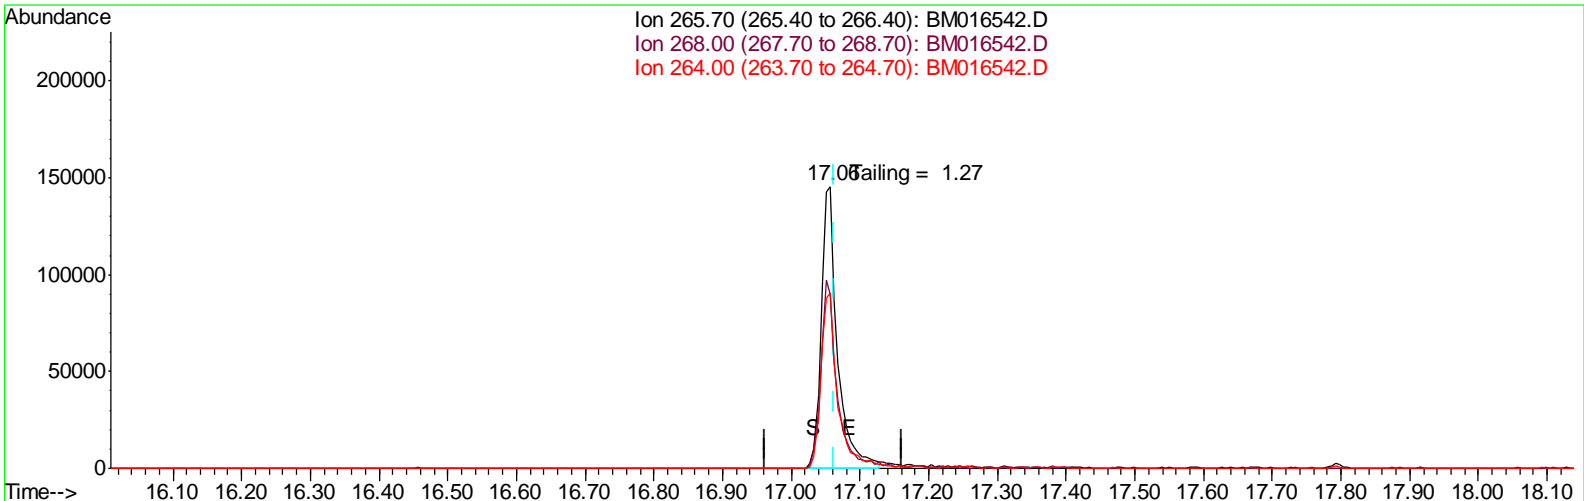

TIC: BM016542.D

(69) Pentachlorophenol (C)




17.057min (-0.006) 0.00ng

response 243783

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	61.82
264.00	61.20	62.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM082218\  
 Data File : BM016542.D  
 Acq On : 23 Aug 2018 06:38  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 23 09:23:09 2018  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\8270-BM082118.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Aug 21 16:31:22 2018  
 Response via : Initial Calibration

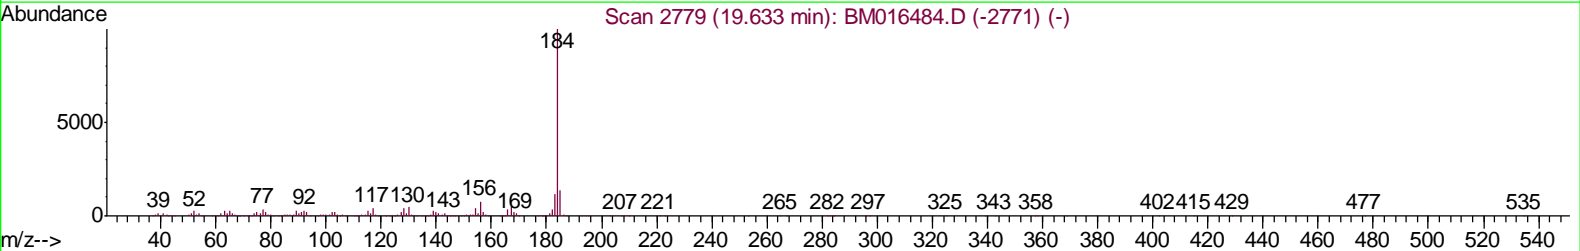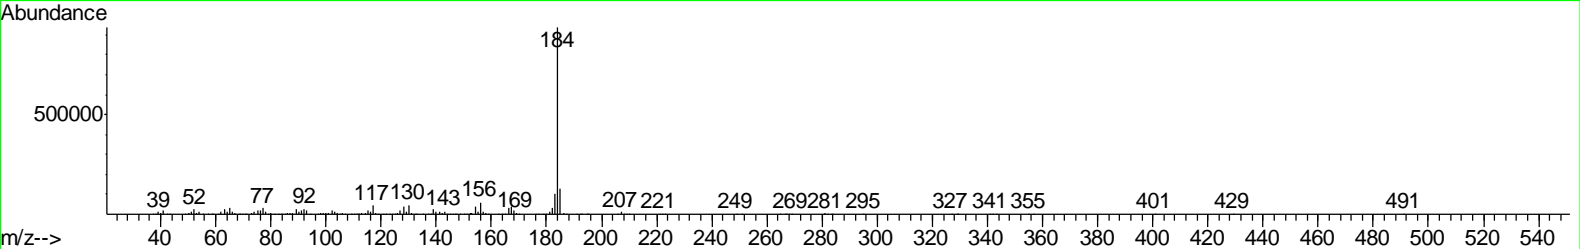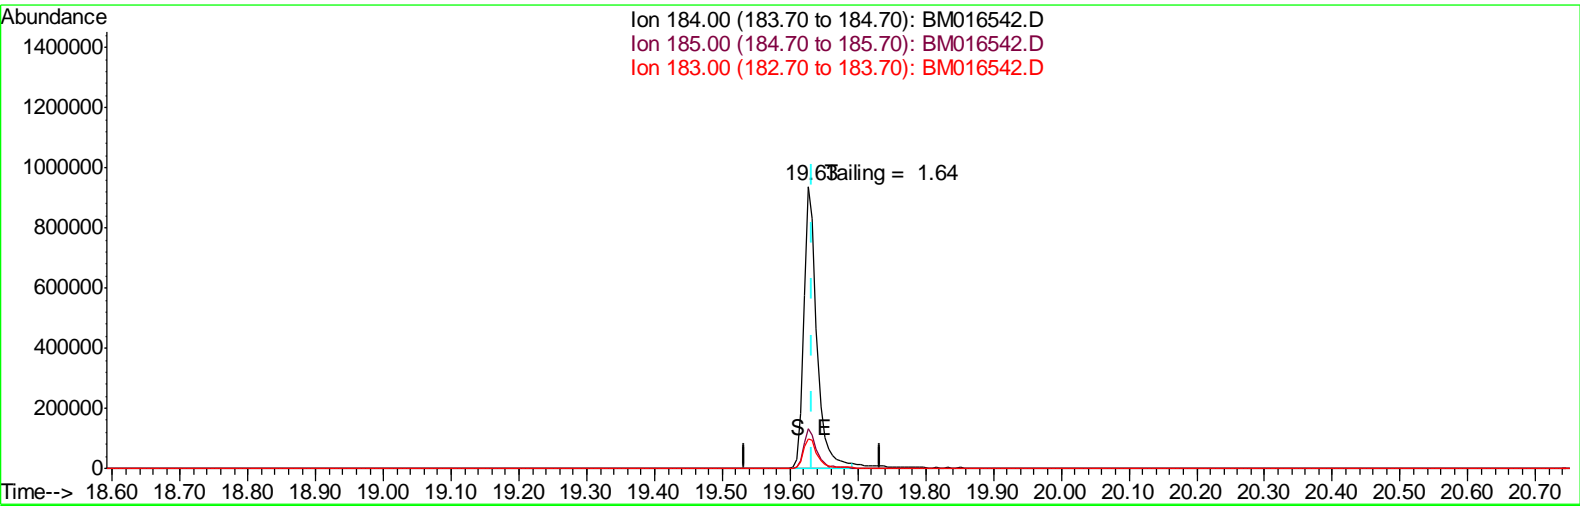

TIC: BM016542.D

(76) Benzidine

19.627min (-0.006) 130038.70ng

response 1282902

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.95
183.00	11.10	10.69
0.00	0.00	0.00