

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082218\
 Data File : BM016530.D
 Acq On : 22 Aug 2018 22:10
 Operator : SJ/JU
 Sample : J4525-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 081518-DBRI-E-D-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.557	381	386	406	rBV	528360	984978	4.30%	1.572%
2	7.192	659	664	684	rBV	301979	598114	2.61%	0.955%
3	7.545	718	724	739	rBV	1407203	2438092	10.64%	3.891%
4	8.016	799	804	824	rBV	438637	826378	3.61%	1.319%
5	8.333	851	858	872	rBV	2648379	4320160	18.85%	6.894%
6	9.204	999	1006	1025	rBV	1506553	2631055	11.48%	4.199%
7	10.827	1276	1282	1299	rBV	469371	922112	4.02%	1.472%
8	13.274	1691	1698	1720	rBV	7634570	9966184	43.49%	15.905%
9	14.657	1925	1933	1944	rBV2	840722	1407520	6.14%	2.246%
10	16.151	2181	2187	2208	rBV	4746968	6469967	28.23%	10.325%
11	17.398	2393	2399	2413	rBV	1440886	2210908	9.65%	3.528%
12	19.992	2834	2840	2848	rBV	21830643	22918425	100.00%	36.574%
13	21.544	3099	3104	3112	rBV	2556770	3505758	15.30%	5.595%
14	23.827	3487	3492	3505	rVB2	1754015	3462763	15.11%	5.526%


Sum of corrected areas: 62662414

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082218\
Data File : BM016530.D
Acq On : 22 Aug 2018 22:10
Operator : SJ/JU
Sample : J4525-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
081518-DBRI-E-D-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

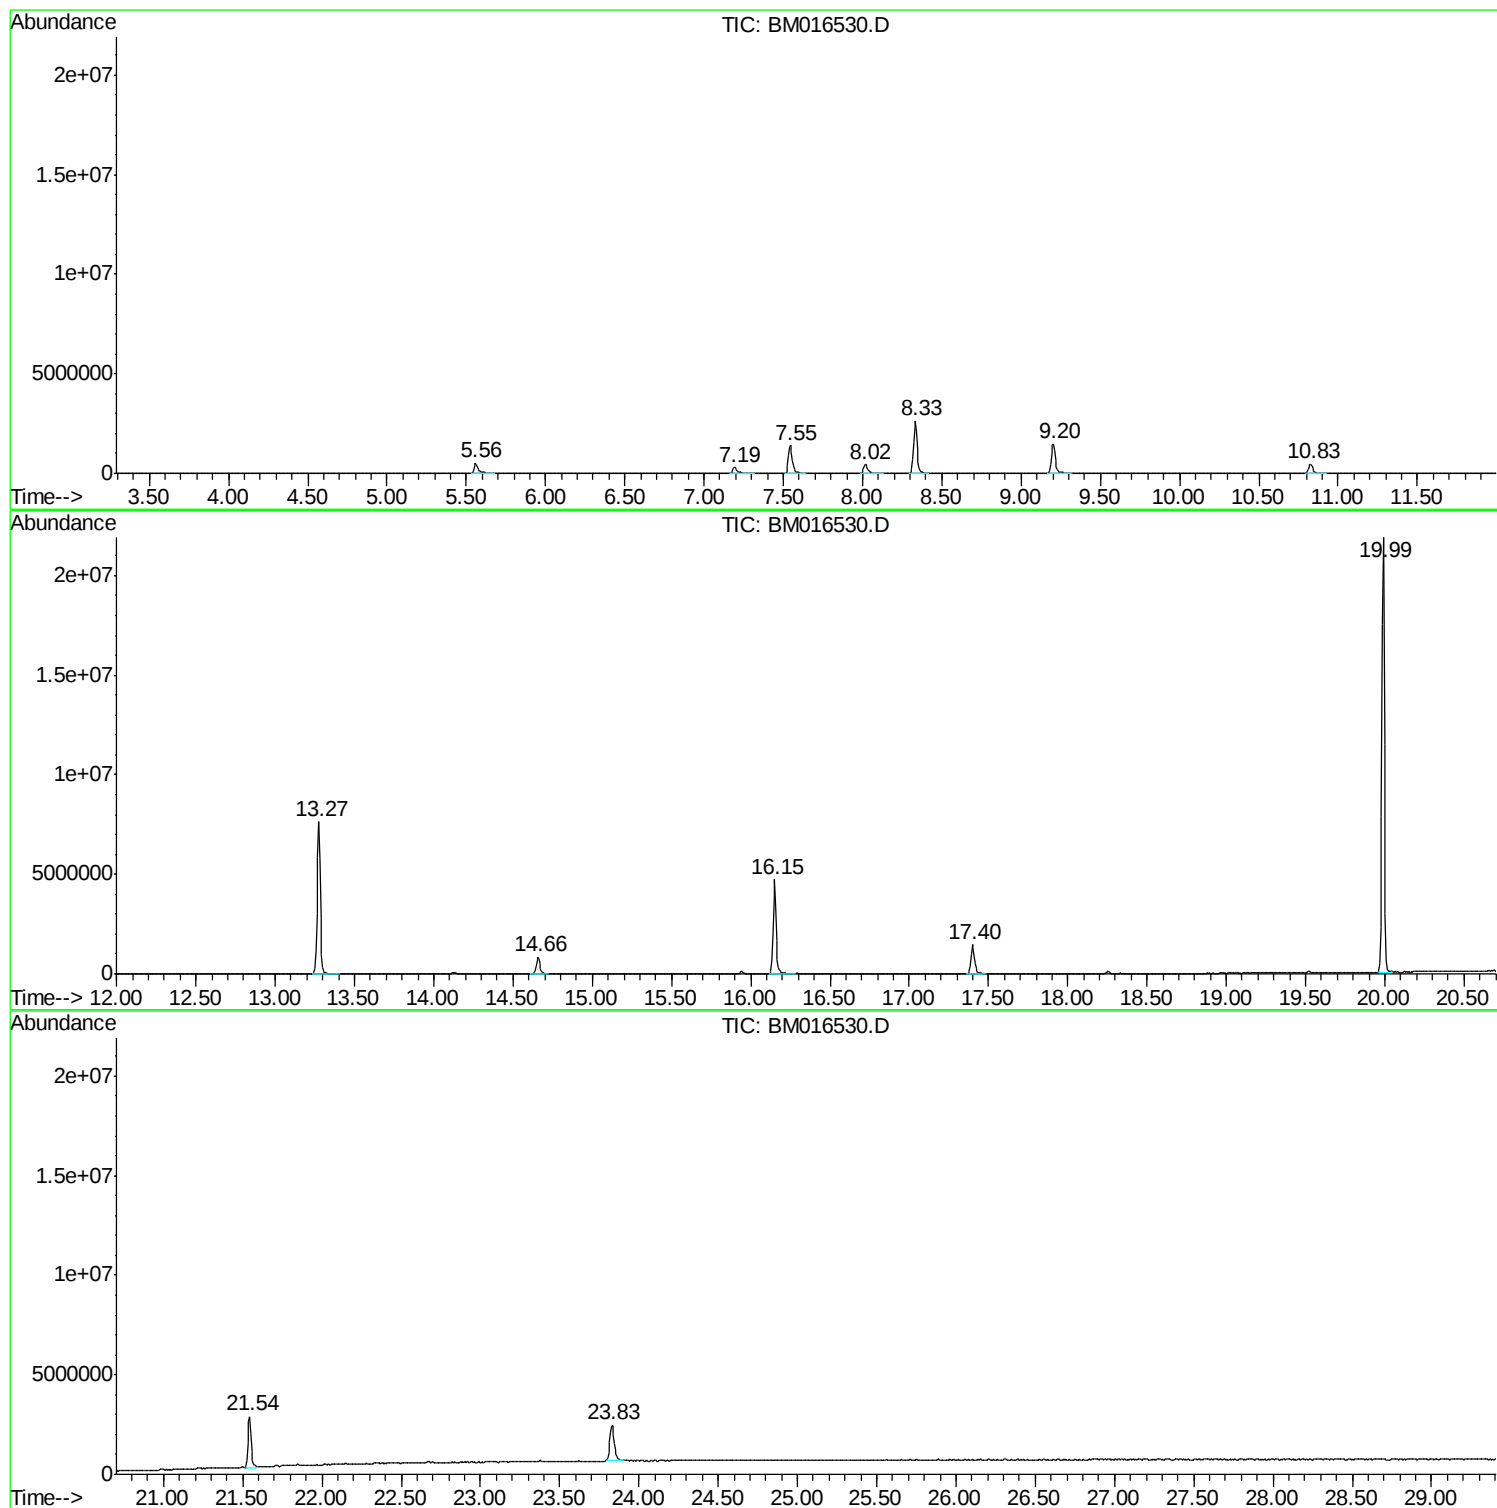

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082218\
Data File : BM016530.D
Acq On : 22 Aug 2018 22:10
Operator : SJ/JU
Sample : J4525-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
081518-DBRI-E-D-B










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.55 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.55	59.01 ng	2438090	1,4-Dichlorobenzene-d4	8.02

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	14
2		3H-1,2-Dithiol-3-one, 5-methyl-	132	C4H4OS2	003620-08-4	14
3		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	11
4		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	10
5		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	10

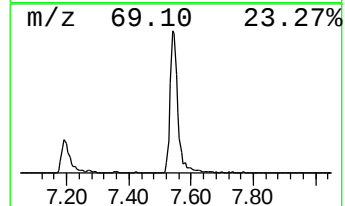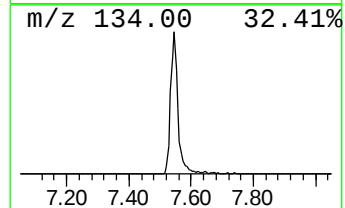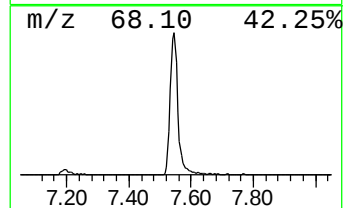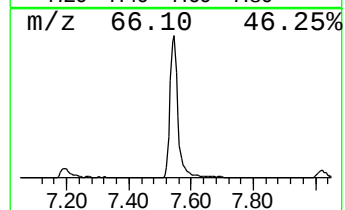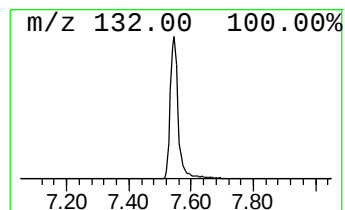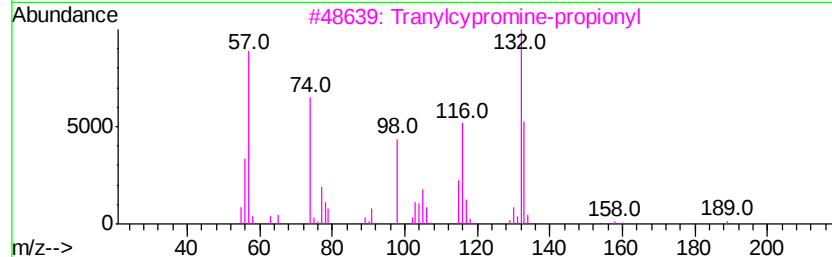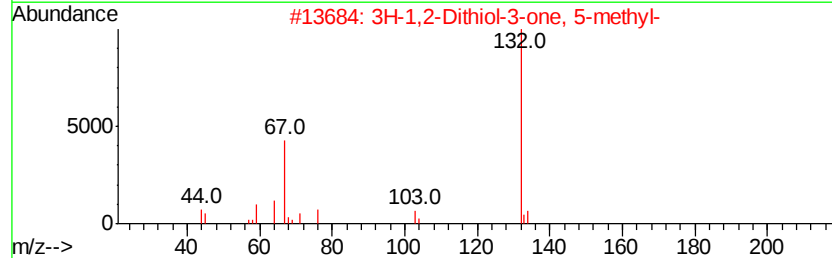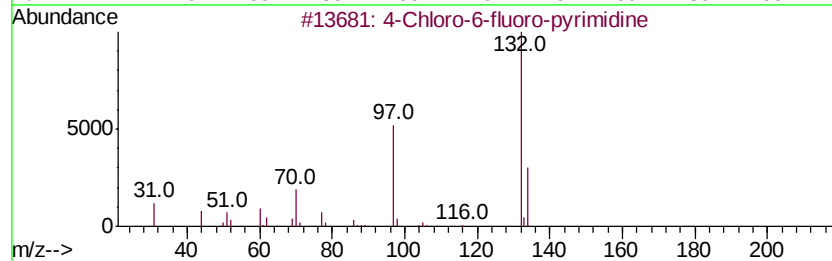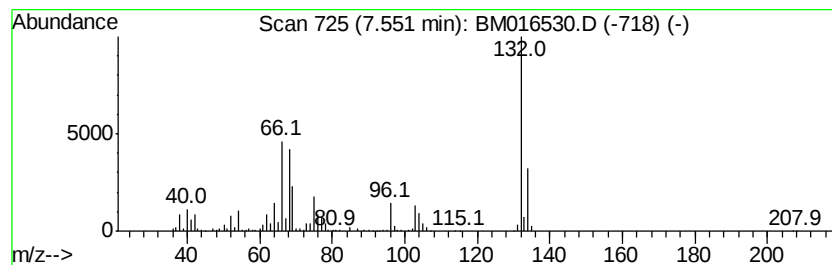

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082218\
Data File : BM016530.D
Acq On : 22 Aug 2018 22:10
Operator : SJ/JU
Sample : J4525-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
081518-DBRI-E-D-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown7.55	7.55	59.0	ng	2438090	1	8.02	826378	20.0