

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082218\
 Data File : BM016535.D
 Acq On : 23 Aug 2018 01:11
 Operator : SJ/JU
 Sample : J4525-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 081518-TIPC-F-D-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.558	381	386	405	rBV	526012	973192	4.12%	1.516%
2	7.193	659	664	680	rBV	319500	597761	2.53%	0.931%
3	7.540	717	723	740	rBV	1397220	2433071	10.31%	3.790%
4	8.016	797	804	819	rBV	449984	832490	3.53%	1.297%
5	8.334	850	858	874	rBV	2536275	4280622	18.13%	6.667%
6	9.198	999	1005	1022	rBV	1504827	2668941	11.31%	4.157%
7	10.822	1275	1281	1295	rBV	497322	933844	3.96%	1.454%
8	13.275	1691	1698	1711	rBV	7419573	10115401	42.85%	15.755%
9	14.657	1923	1933	1946	rBV2	926192	1483153	6.28%	2.310%
10	16.151	2181	2187	2203	rBV	4959923	6970325	29.53%	10.856%
11	17.398	2393	2399	2412	rBV	1518722	2263012	9.59%	3.525%
12	19.986	2834	2839	2846	rBV	20565823	23604524	100.00%	36.764%
13	21.545	3099	3104	3113	rBV	2581519	3472975	14.71%	5.409%
14	23.827	3486	3492	3501	rBV	1826992	3576214	15.15%	5.570%


Sum of corrected areas: 64205525

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082218\
Data File : BM016535.D
Acq On : 23 Aug 2018 01:11
Operator : SJ/JU
Sample : J4525-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
081518-TIPC-F-D-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

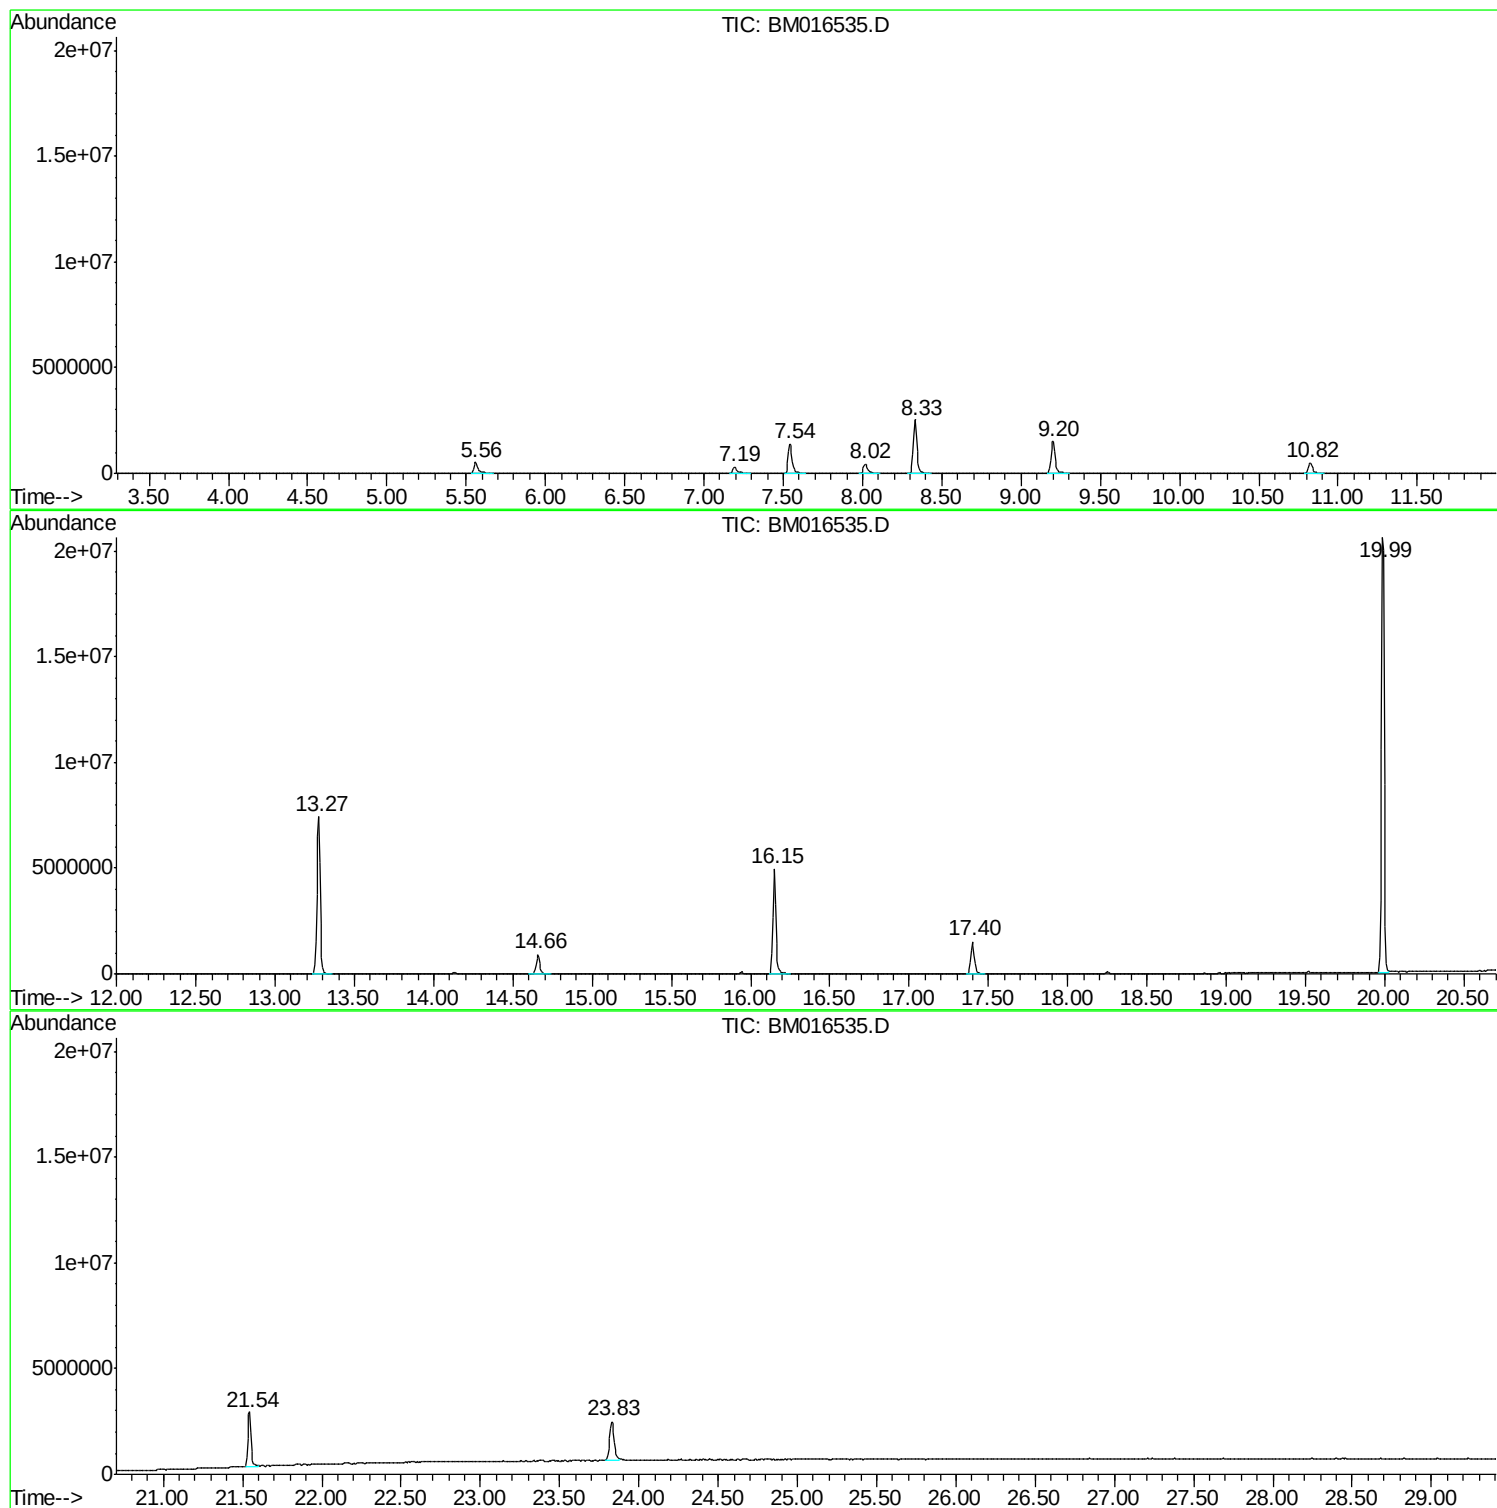

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082218\
Data File : BM016535.D
Acq On : 23 Aug 2018 01:11
Operator : SJ/JU
Sample : J4525-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
081518-TIPC-F-D-S










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.54 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.54	58.45 ng	2433070	1,4-Dichlorobenzene-d4	8.02

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	14
2		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	14
3		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	12
4		3H-1,2-Dithiol-3-one, 5-methyl-	132	C4H4OS2	003620-08-4	12
5		Benzene, 1,2,4-trifluoro-	132	C6H3F3	000367-23-7	10

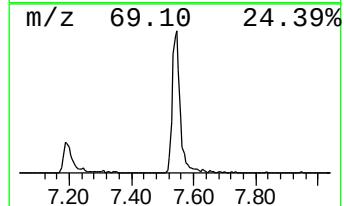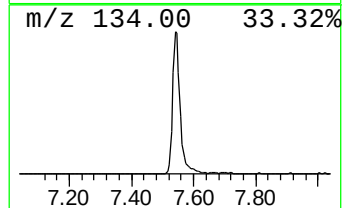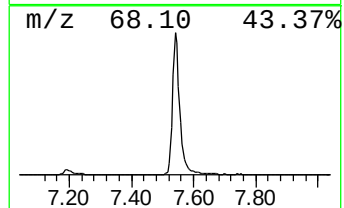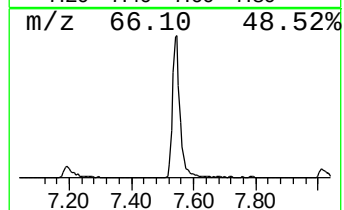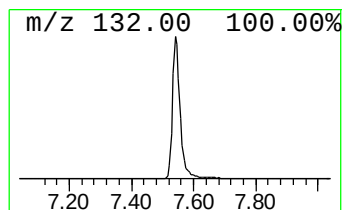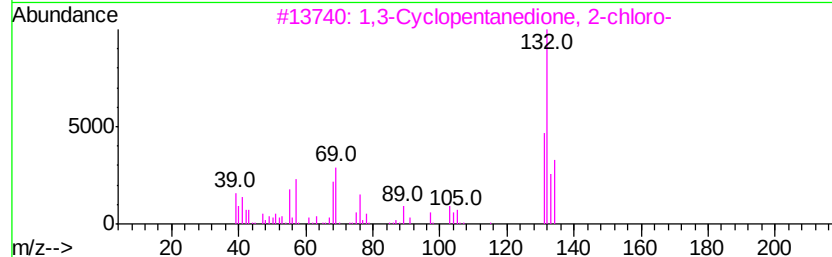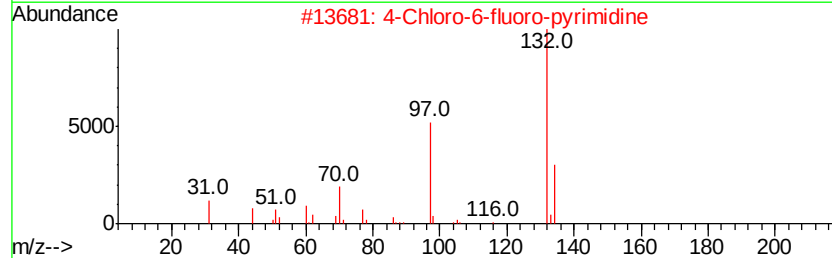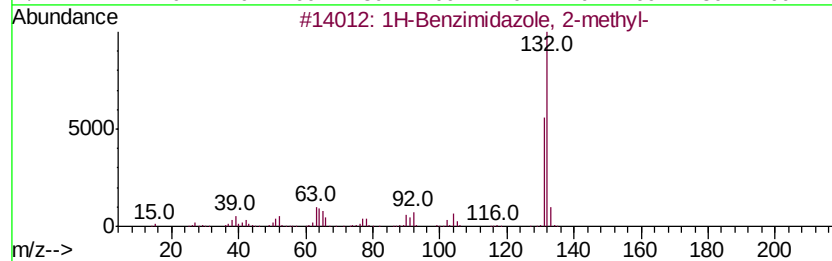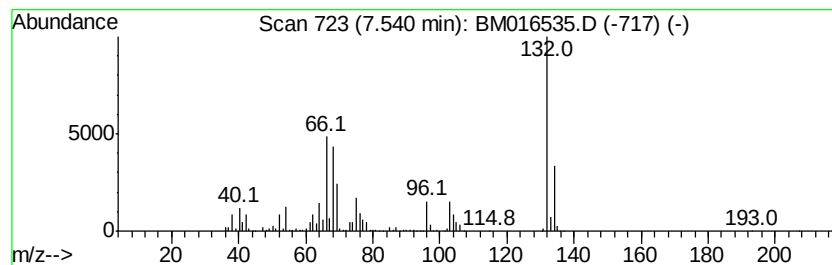

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082218\
Data File : BM016535.D
Acq On : 23 Aug 2018 01:11
Operator : SJ/JU
Sample : J4525-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
081518-TIPC-F-D-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown7.54	7.54	58.5	ng	2433070	1	8.02	832490	20.0