

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082218\
 Data File : BM016536.D
 Acq On : 23 Aug 2018 01:47
 Operator : SJ/JU
 Sample : J4525-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 081518-TIPC-F-U-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.557	381	386	398	rBV	551362	966127	4.48%	1.601%
2	7.193	659	664	681	rBV	316652	621426	2.88%	1.029%
3	7.540	717	723	737	rBV	1365001	2399640	11.12%	3.975%
4	8.016	798	804	819	rBV	441683	810007	3.75%	1.342%
5	8.334	851	858	877	rBV	2457275	4159012	19.28%	6.890%
6	9.198	999	1005	1024	rBV	1399028	2540679	11.77%	4.209%
7	10.822	1275	1281	1299	rBV	462535	886094	4.11%	1.468%
8	13.275	1691	1698	1710	rBV	7343600	9457355	43.83%	15.667%
9	14.657	1924	1933	1947	rBV3	857292	1428498	6.62%	2.366%
10	16.151	2181	2187	2201	rBV	4721390	6640205	30.77%	11.000%
11	17.398	2394	2399	2413	rBV	1434727	2141157	9.92%	3.547%
12	19.992	2834	2840	2847	rBV	19589025	21577191	100.00%	35.745%
13	21.545	3099	3104	3111	rBV	2381147	3261085	15.11%	5.402%
14	23.827	3486	3492	3503	rBV	1755363	3475171	16.11%	5.757%


Sum of corrected areas: 60363647

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082218\
Data File : BM016536.D
Acq On : 23 Aug 2018 01:47
Operator : SJ/JU
Sample : J4525-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
081518-TIPC-F-U-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

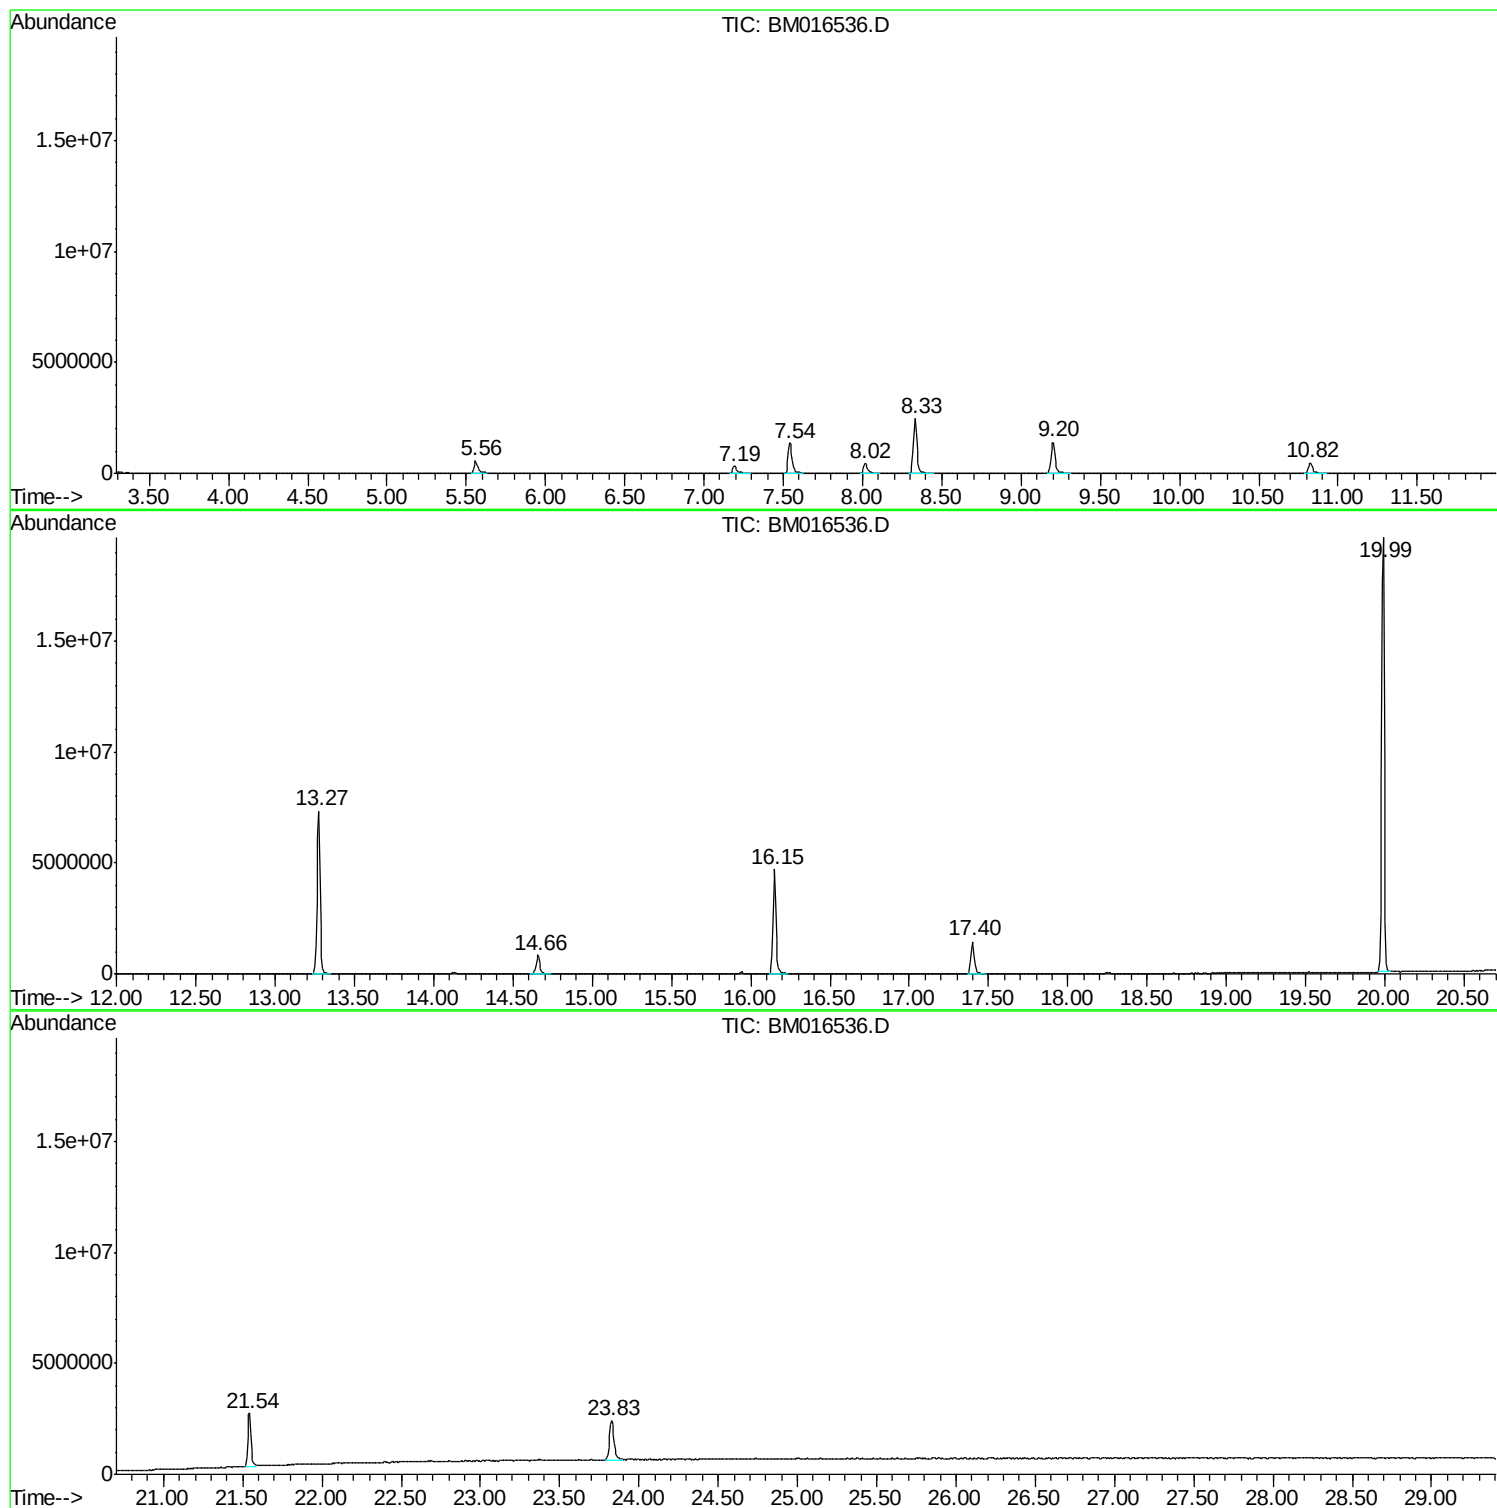

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082218\
Data File : BM016536.D
Acq On : 23 Aug 2018 01:47
Operator : SJ/JU
Sample : J4525-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
081518-TIPC-F-U-B










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.54 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.54	59.25 ng	2399640	1,4-Dichlorobenzene-d4	8.02

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3H-1,2-Dithiol-3-one, 5-methyl-	132	C4H4OS2	003620-08-4	22
2		1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	14
3		Tranvlcypromine-propionyl	189	C12H15NO	1000123-86-3	11
4		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	10
5		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	10

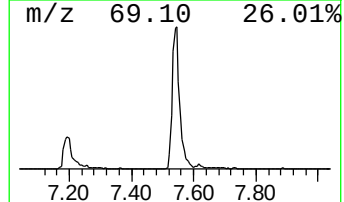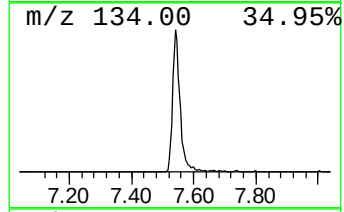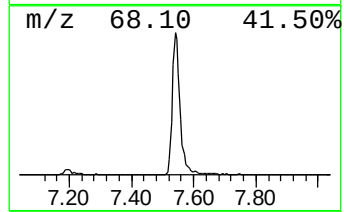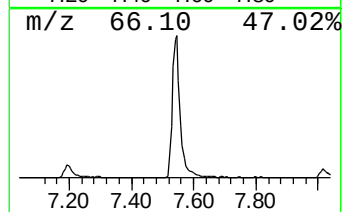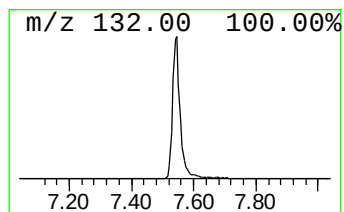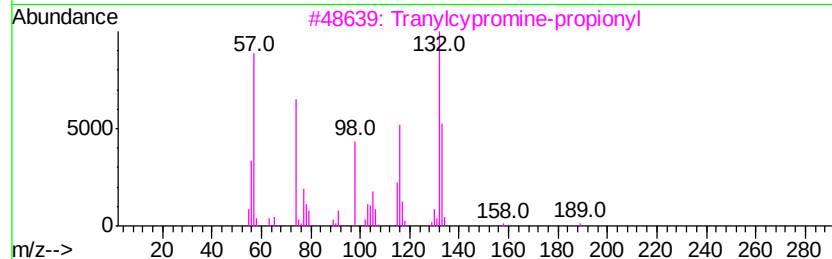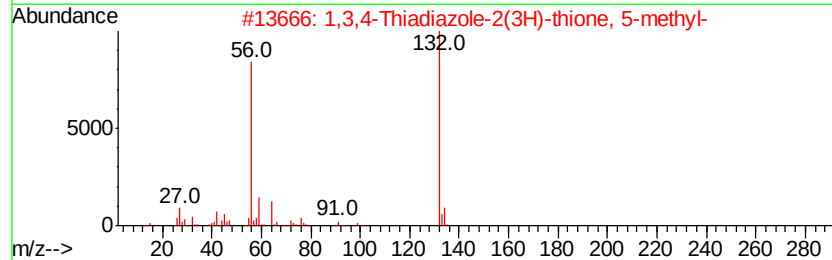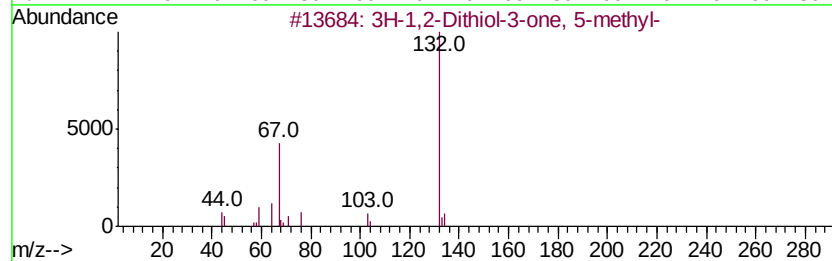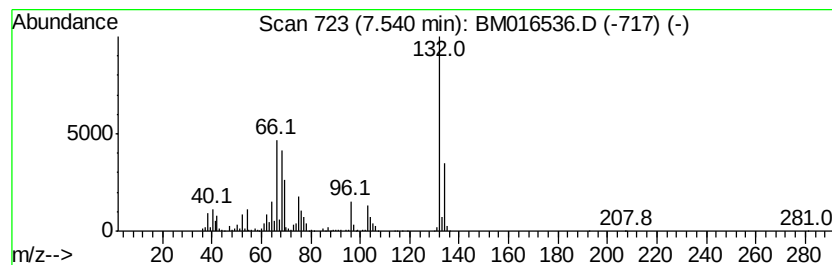

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082218\
Data File : BM016536.D
Acq On : 23 Aug 2018 01:47
Operator : SJ/JU
Sample : J4525-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
081518-TIPC-F-U-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown7.54	7.54	59.3	ng	2399640	1	8.02	810007	20.0