

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082218\
 Data File : BM016537.D
 Acq On : 23 Aug 2018 02:23
 Operator : SJ/JU
 Sample : J4525-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 081518-TIPC-F-U-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.557	381	386	405	rBV	462985	902812	4.60%	1.593%
2	7.193	659	664	679	rBV	278363	526692	2.68%	0.929%
3	7.540	718	723	741	rBV	1268983	2245166	11.44%	3.961%
4	8.016	796	804	817	rBV	437858	798729	4.07%	1.409%
5	8.328	851	857	872	rBV	2306166	3909914	19.93%	6.897%
6	9.198	999	1005	1021	rBV	1327878	2378370	12.12%	4.196%
7	10.822	1274	1281	1295	rBV	492491	902683	4.60%	1.592%
8	13.275	1691	1698	1714	rBV	6376772	8825817	44.98%	15.569%
9	14.657	1924	1933	1947	rBV2	900247	1467451	7.48%	2.589%
10	16.151	2181	2187	2203	rBV	4363374	6123476	31.21%	10.802%
11	17.398	2393	2399	2413	rBV	1440498	2196308	11.19%	3.874%
12	19.986	2833	2839	2849	rBV	16770615	19621136	100.00%	34.613%
13	21.539	3099	3103	3112	rBV	2376945	3335566	17.00%	5.884%
14	23.827	3486	3492	3504	rBV2	1745062	3453855	17.60%	6.093%


Sum of corrected areas: 56687975

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082218\
Data File : BM016537.D
Acq On : 23 Aug 2018 02:23
Operator : SJ/JU
Sample : J4525-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
081518-TIPC-F-U-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

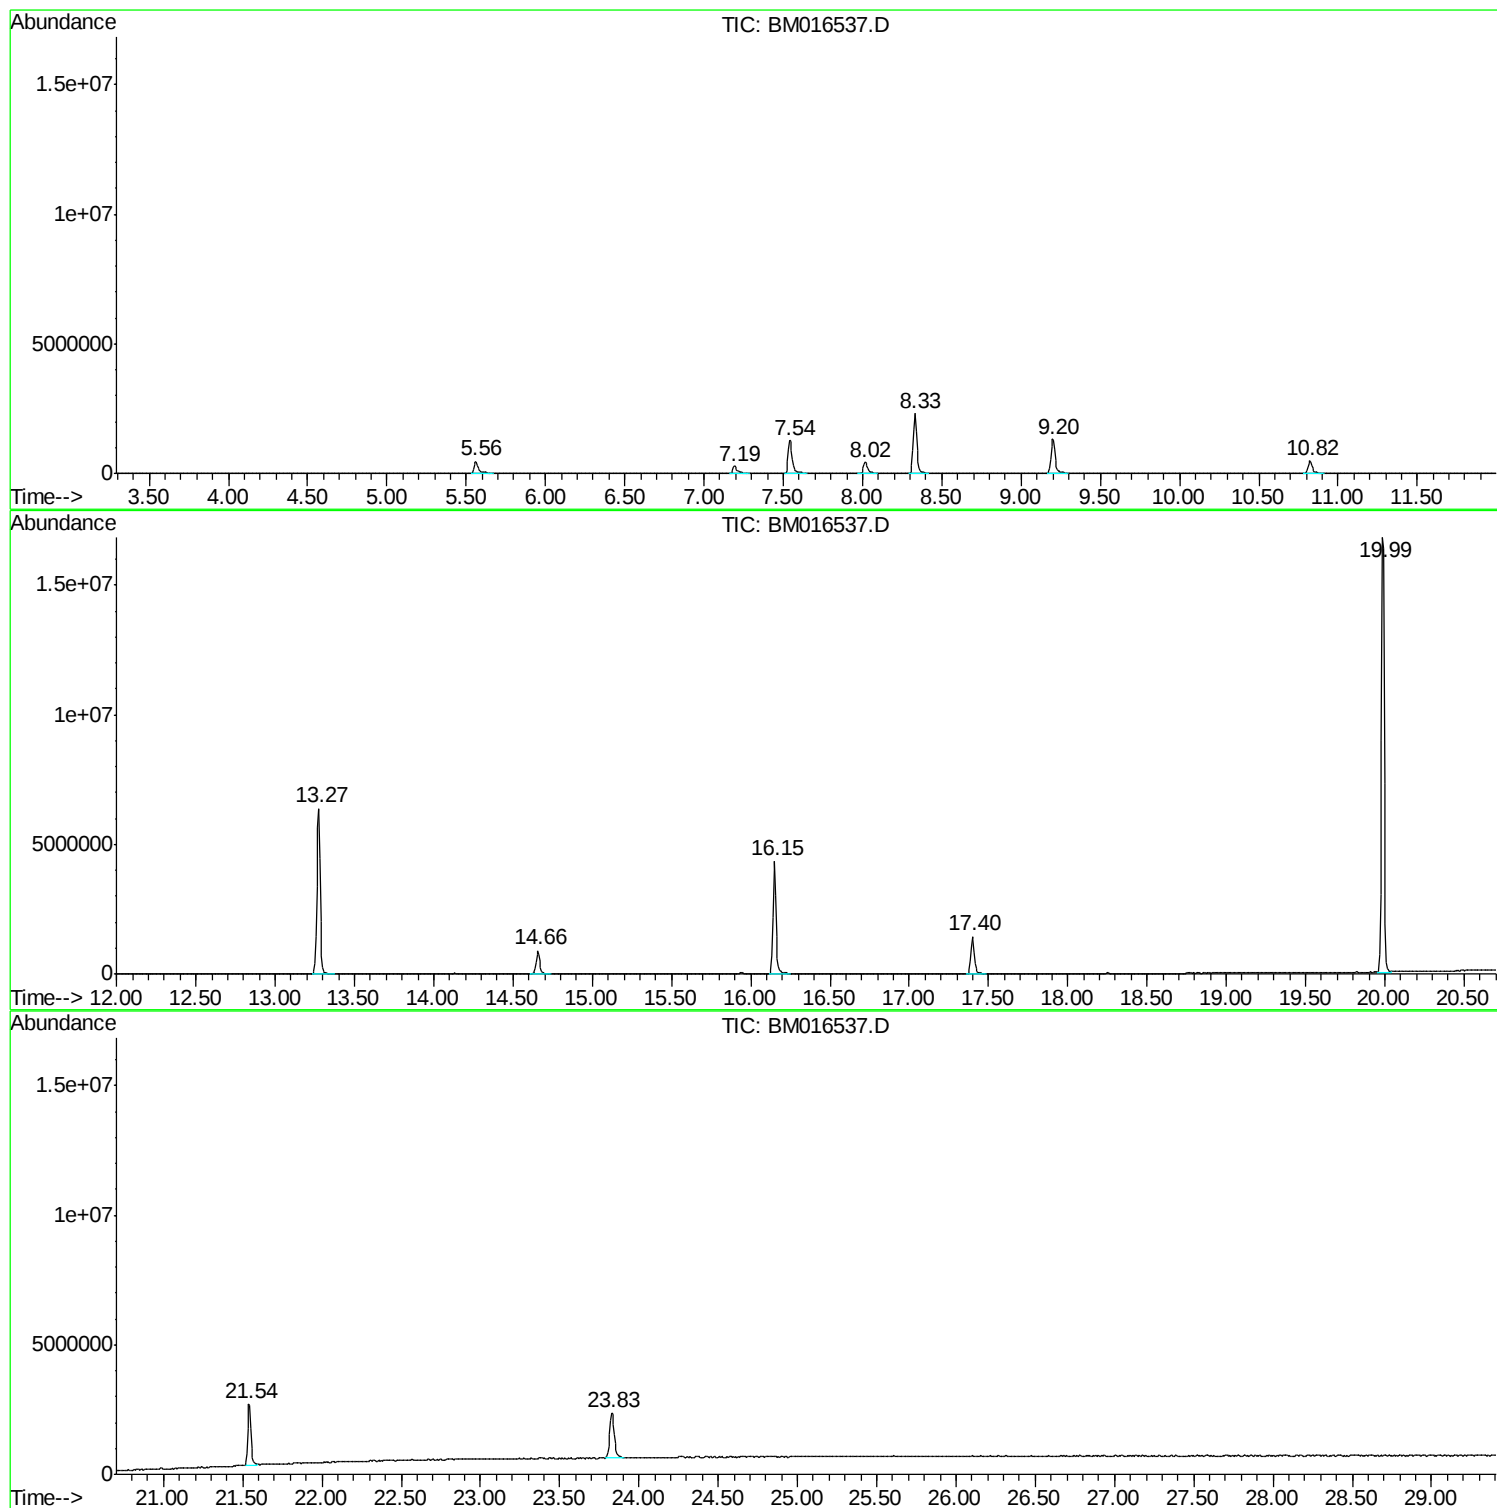

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082218\
Data File : BM016537.D
Acq On : 23 Aug 2018 02:23
Operator : SJ/JU
Sample : J4525-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
081518-TIPC-F-U-S










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.54 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.54	56.22 ng	2245170	1,4-Dichlorobenzene-d4	8.02

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3H-1,2-Dithiol-3-one, 5-methyl-	132	C4H4OS2	003620-08-4	22
2		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	14
3		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	10
4		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	10
5		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9

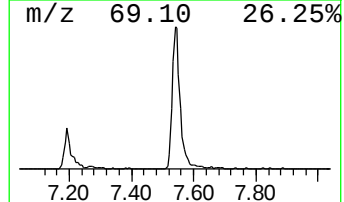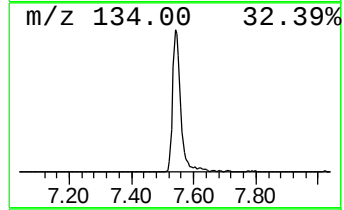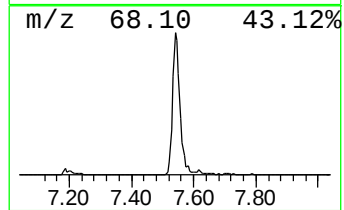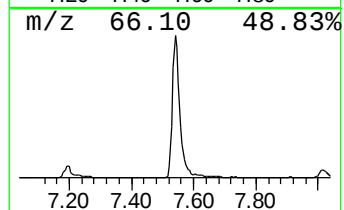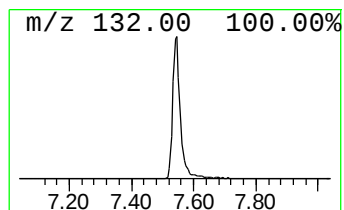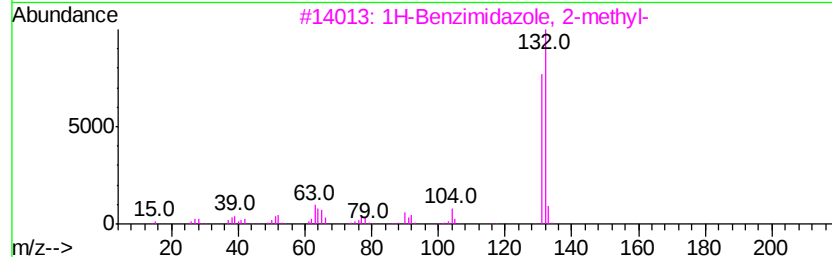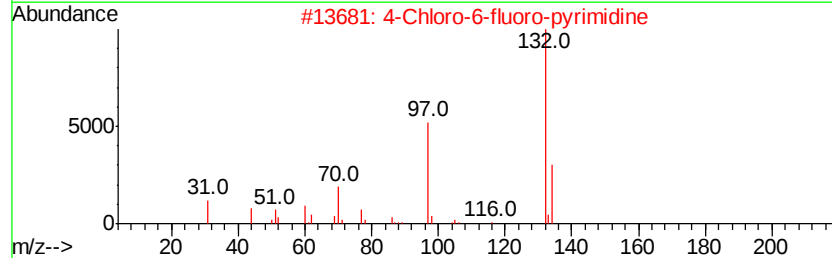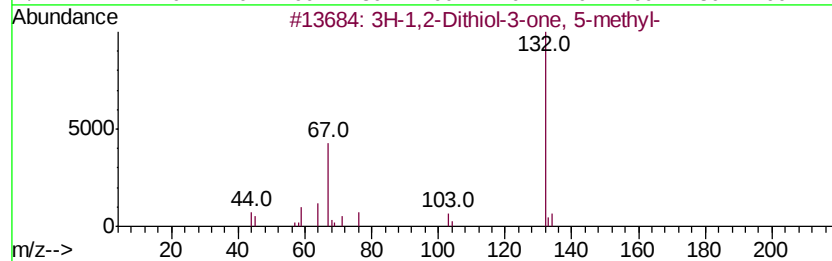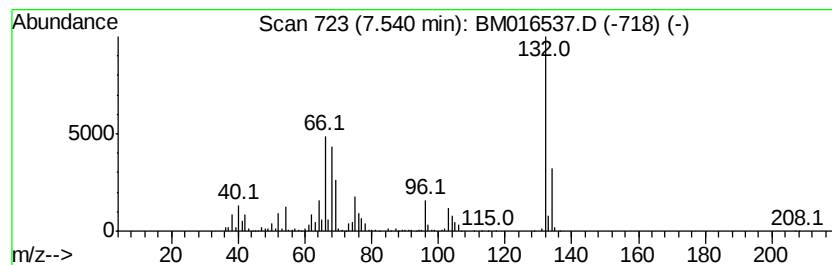

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082218\
Data File : BM016537.D
Acq On : 23 Aug 2018 02:23
Operator : SJ/JU
Sample : J4525-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
081518-TIPC-F-U-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown7.54	7.54	56.2	ng	2245170	1	8.02	798729	20.0