

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082218\
 Data File : BM016539.D
 Acq On : 23 Aug 2018 03:36
 Operator : SJ/JU
 Sample : PB112247BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB112247BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.551	380	385	404	rBV	2398585	3757341	18.93%	5.259%
2	7.192	657	664	684	rBV	2326555	3745013	18.86%	5.242%
3	7.540	717	723	738	rBV	2852572	4658626	23.47%	6.521%
4	8.016	798	804	819	rBV	641811	1112224	5.60%	1.557%
5	8.334	850	858	878	rBV	2438557	4096533	20.63%	5.734%
6	9.198	999	1005	1016	rBV	1345684	2312790	11.65%	3.237%
7	10.822	1275	1281	1300	rBV	667730	1230498	6.20%	1.722%
8	13.274	1691	1698	1710	rBV	6191692	8806294	44.36%	12.327%
9	14.657	1927	1933	1947	rBV2	1192394	1853347	9.34%	2.594%
10	16.151	2180	2187	2203	rBV	6925371	9345598	47.07%	13.082%
11	17.398	2393	2399	2417	rBV	1957481	2860055	14.41%	4.003%
12	19.986	2834	2839	2847	rBV	17064464	19853160	100.00%	27.790%
13	21.544	3099	3104	3115	rBV	2995961	3893031	19.61%	5.449%
14	23.827	3486	3492	3504	rBV	1916355	3915581	19.72%	5.481%


Sum of corrected areas: 71440091

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082218\
Data File : BM016539.D
Acq On : 23 Aug 2018 03:36
Operator : SJ/JU
Sample : PB112247BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB112247BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

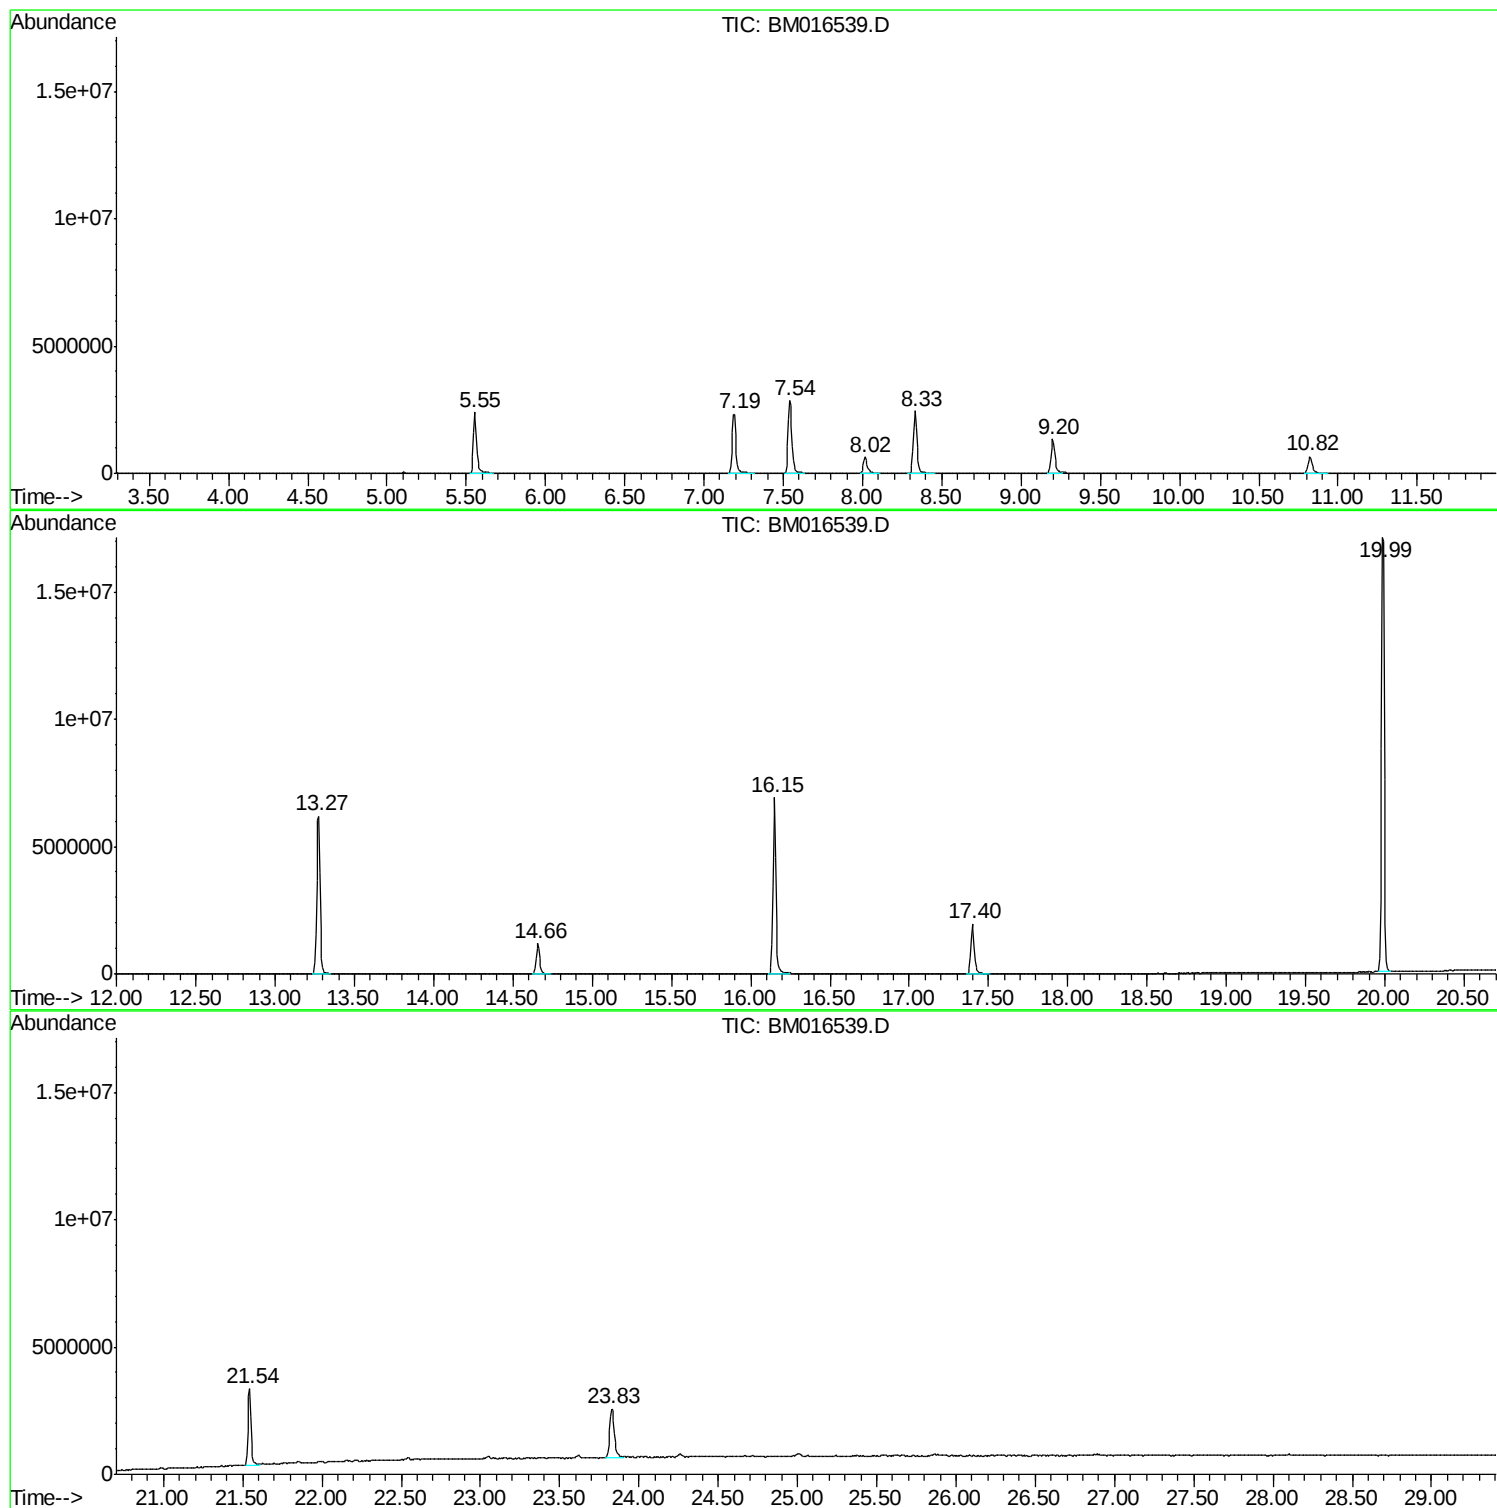

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082218\
Data File : BM016539.D
Acq On : 23 Aug 2018 03:36
Operator : SJ/JU
Sample : PB112247BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB112247BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.54 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.54	83.77 ng	4658630	1,4-Dichlorobenzene-d4	8.02

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	14
2		1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	14
3		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	12
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
5		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	10

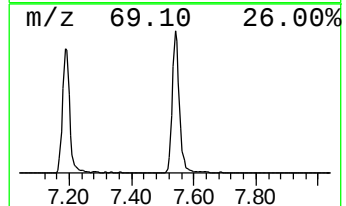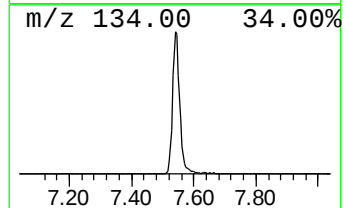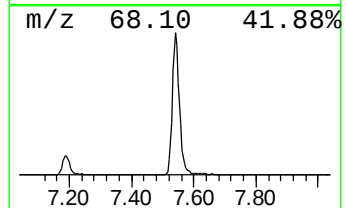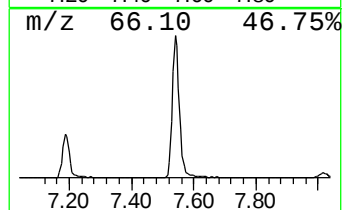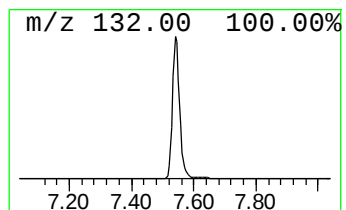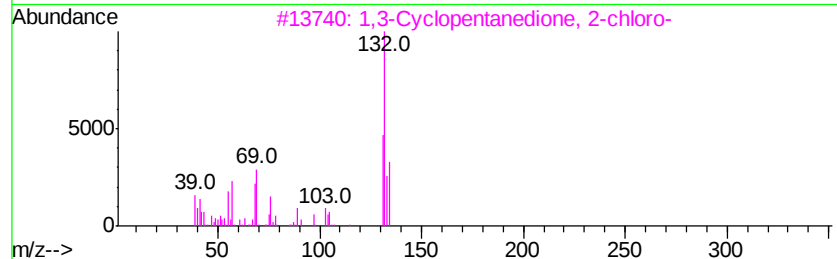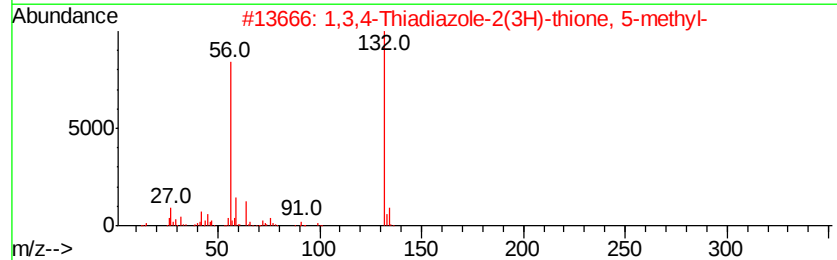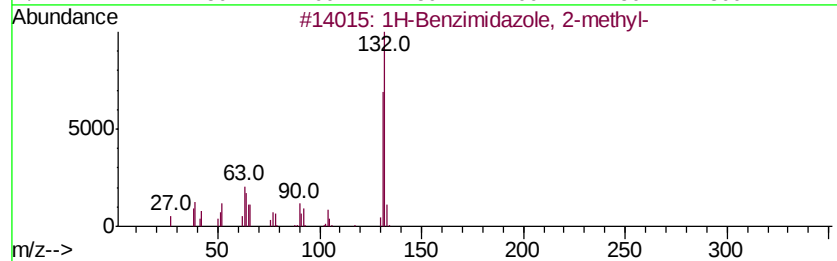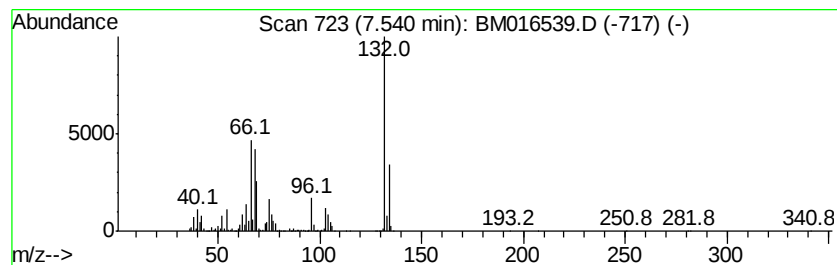

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM082218\
Data File : BM016539.D
Acq On : 23 Aug 2018 03:36
Operator : SJ/JU
Sample : PB112247BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB112247BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.54	7.54	83.8	ng	4658630	1	8.02	1112220	20.0