


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082218\
 Data File : BM016522.D
 Acq On : 22 Aug 2018 17:19
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 21 16:31:22 2018

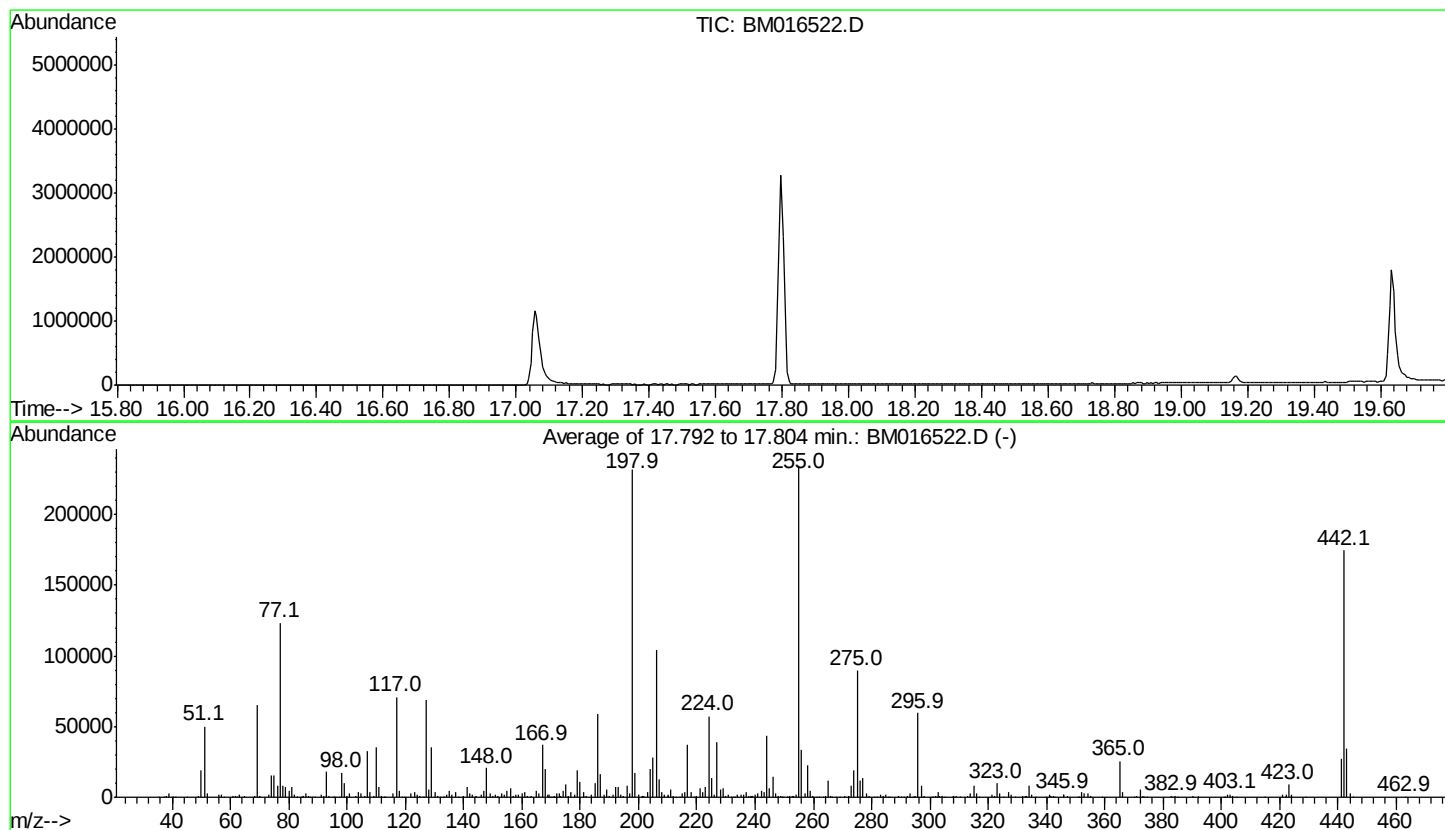

AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.6	50021	PASS
68	69	0.00	2	1.4	940	PASS
69	198	0.00	100	28.0	64976	PASS
70	69	0.00	2	0.8	536	PASS
127	198	10	80	29.6	68736	PASS
197	198	0.00	2	1.2	2682	PASS
198	198	100	100	100.0	231914	PASS
199	198	5	9	7.6	17512	PASS
275	198	10	60	38.6	89565	PASS
365	198	1	100	11.1	25728	PASS
441	198	0.01	100	11.8	27384	PASS
442	198	50	100	75.2	174402	PASS
443	442	15	24	19.9	34680	PASS