


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM082218\
 Data File : BM016542.D
 Acq On : 23 Aug 2018 06:38
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM082118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 21 16:31:22 2018

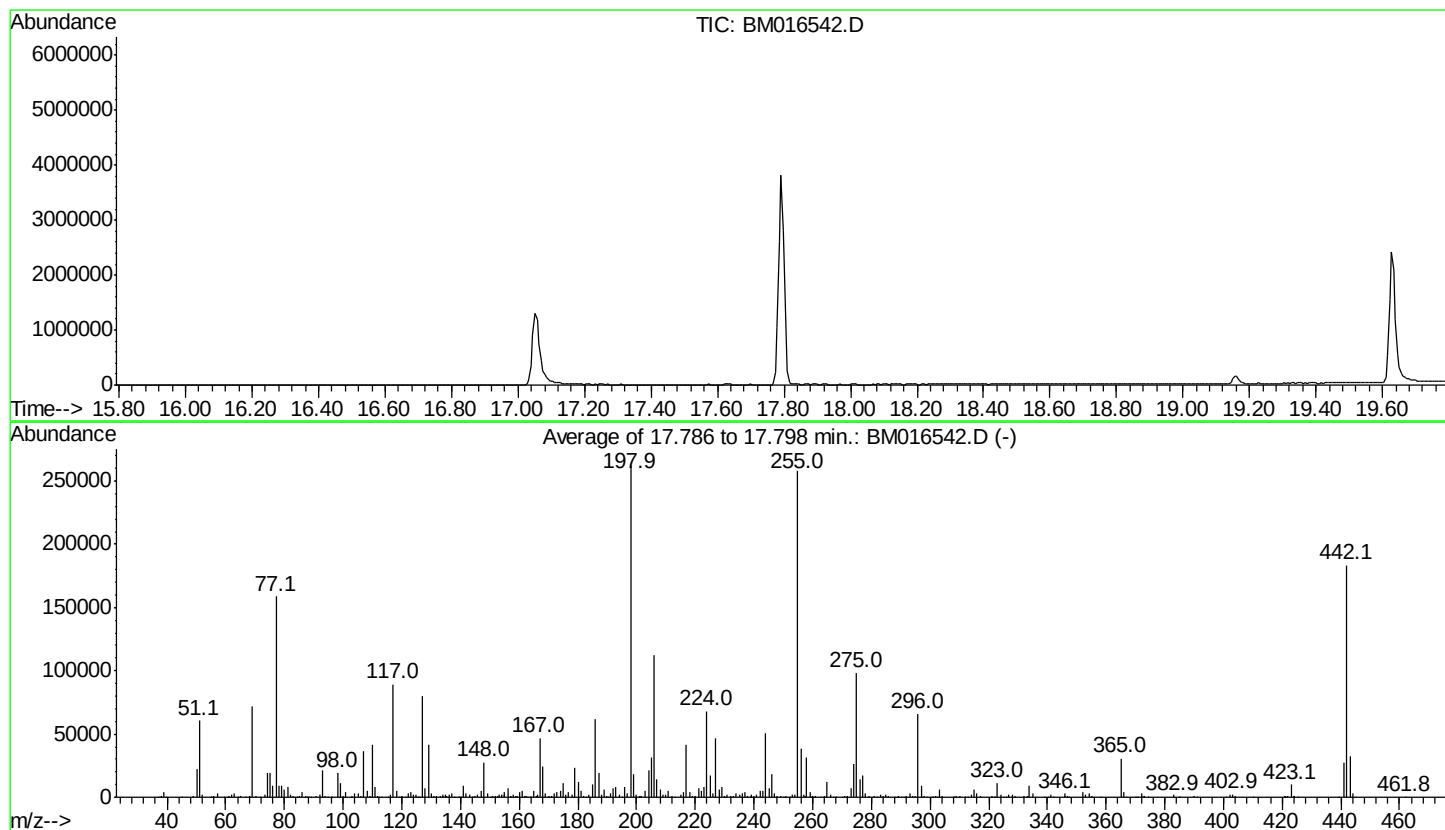

AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.1	60552	PASS
68	69	0.00	2	1.7	1203	PASS
69	198	0.00	100	27.4	71917	PASS
70	69	0.00	2	1.1	817	PASS
127	198	10	80	30.6	80173	PASS
197	198	0.00	2	1.2	3047	PASS
198	198	100	100	100.0	262229	PASS
199	198	5	9	7.0	18328	PASS
275	198	10	60	37.5	98362	PASS
365	198	1	100	11.7	30770	PASS
441	198	0.01	100	10.4	27197	PASS
442	198	50	100	70.1	183757	PASS
443	442	15	24	17.8	32666	PASS