
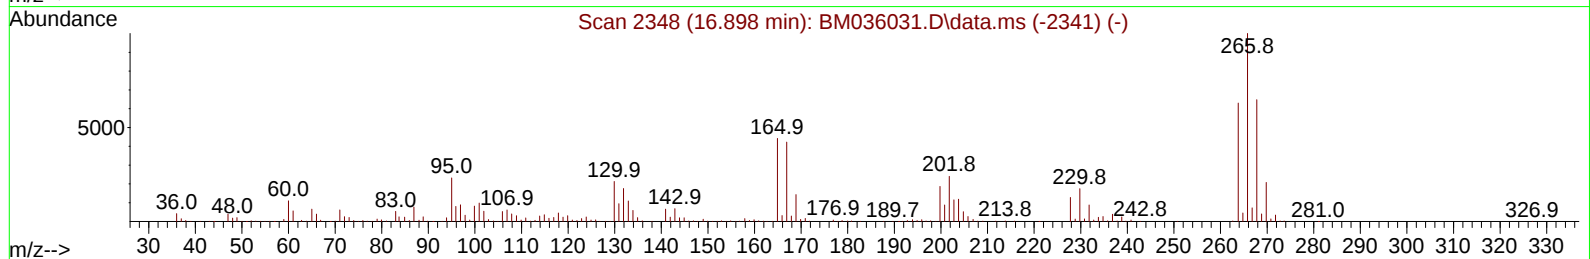
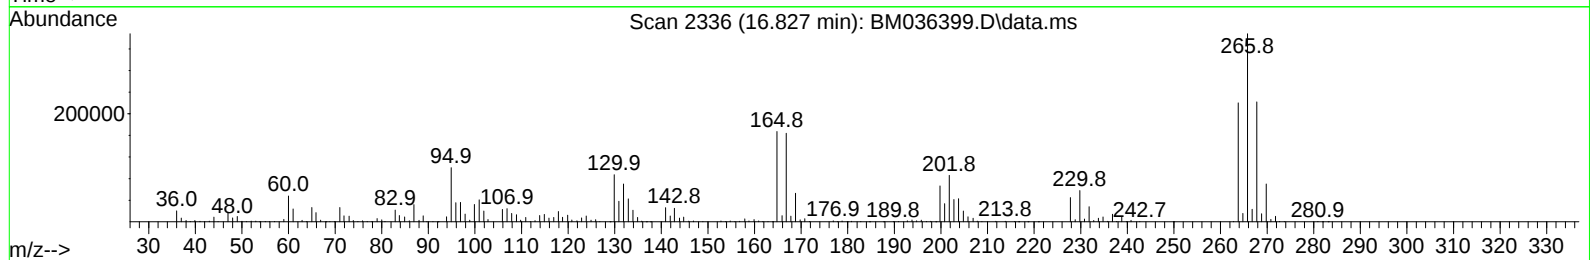


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082522\
 Data File : BM036399.D
 Acq On : 25 Aug 2022 10:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 26 07:19:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 25 15:21:00 2022
 Response via : Initial Calibration

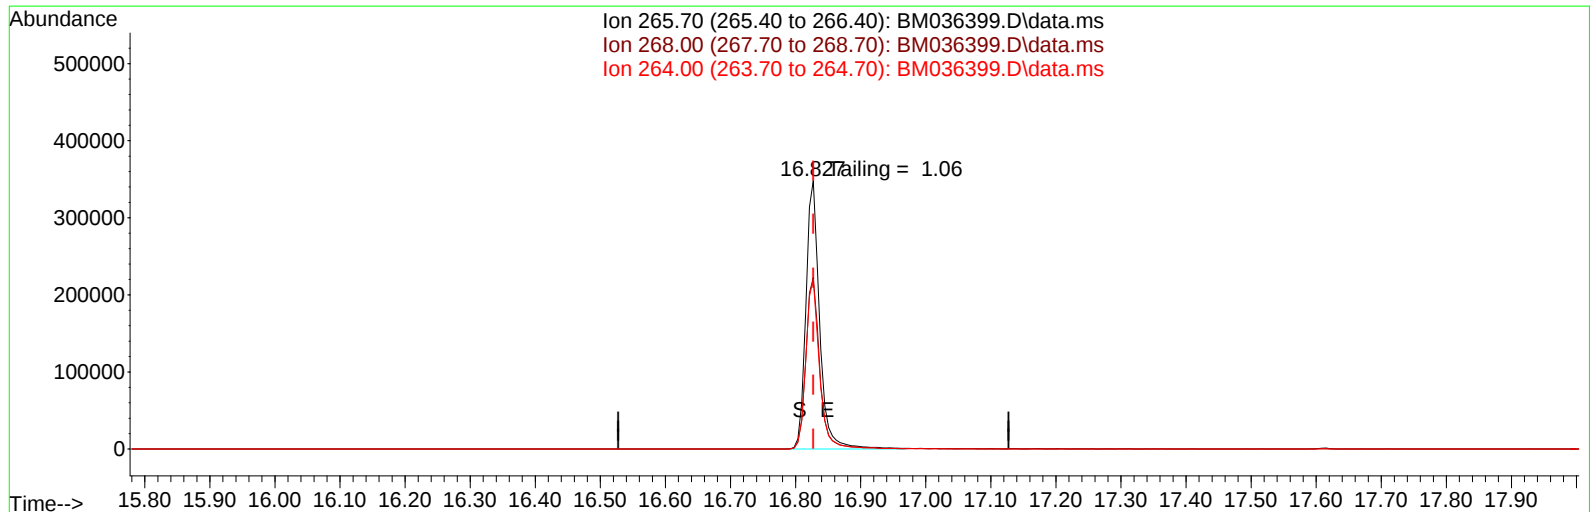

TIC: BM036399.D\data.ms

(70) Pentachlorophenol (C)




16.827min (-0.000) 1122501.82 ng

response 513060

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.79
264.00	63.30	63.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082522\
Data File : BM036399.D
Acq On : 25 Aug 2022 10:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 26 07:19:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 15:21:00 2022
Response via : Initial Calibration

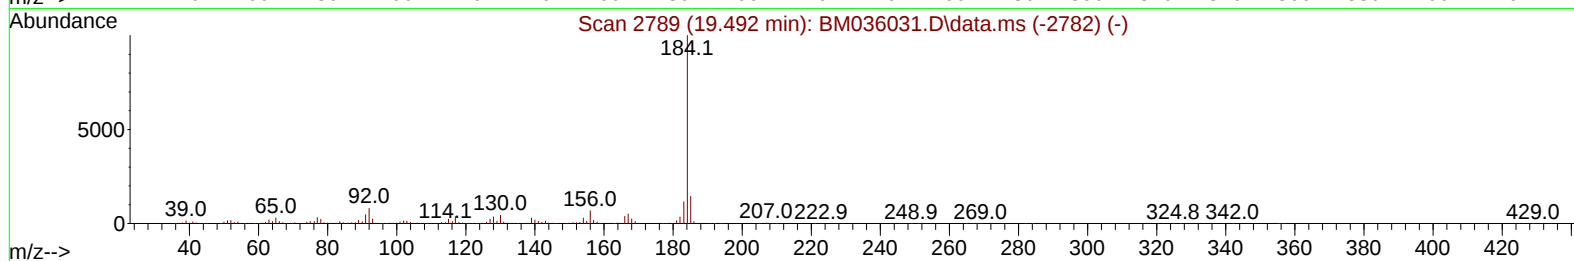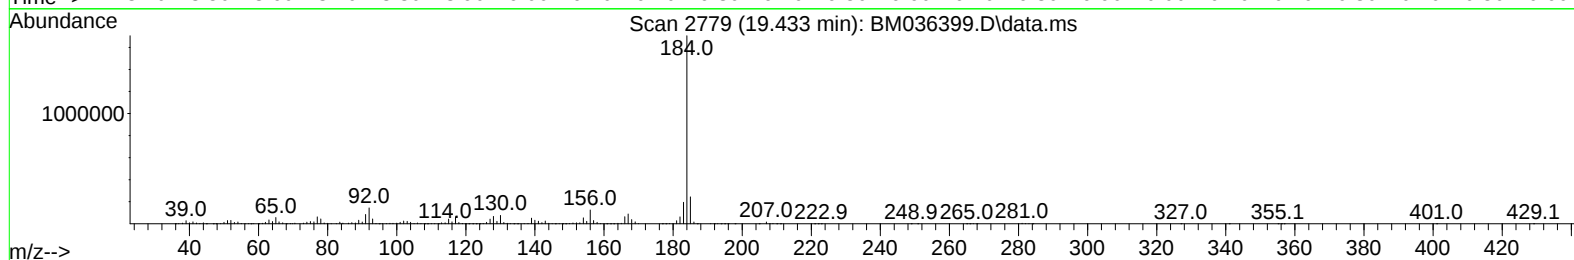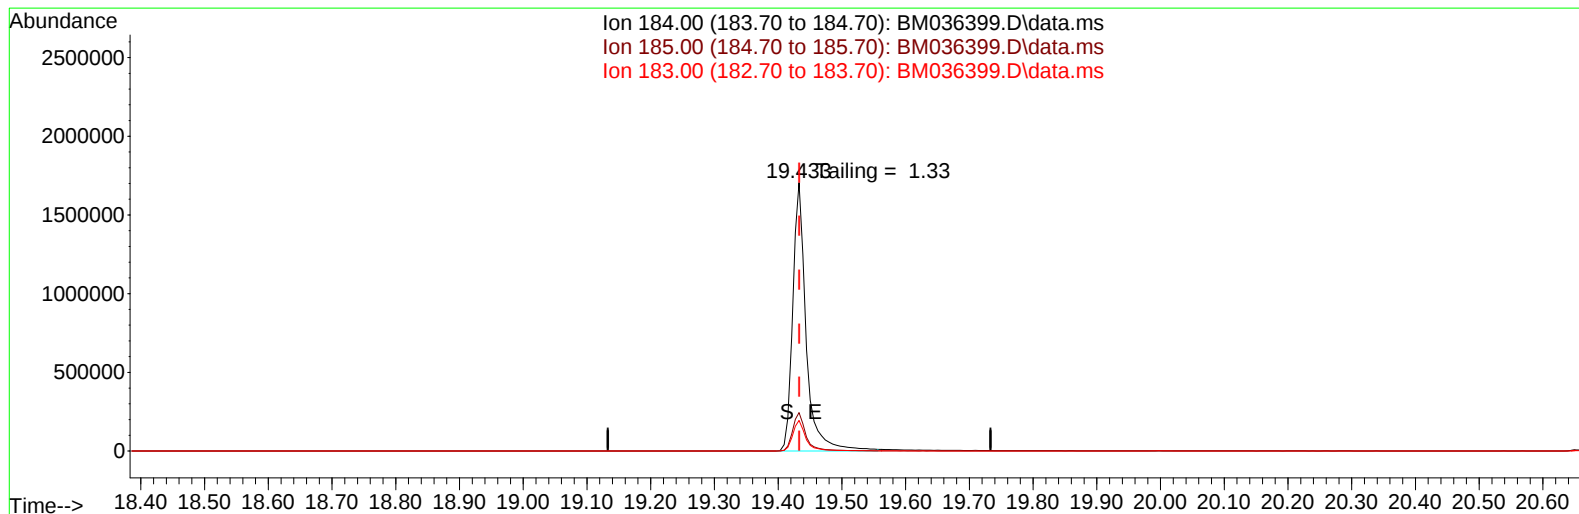

TIC: BM036399.D\data.ms

(77) Benzidine**19.433min (-0.000) 312081.71 ng****response 2550766**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.30
183.00	11.90	11.42
0.00	0.00	0.00