

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082522\
 Data File : BM036401.D
 Acq On : 25 Aug 2022 11:51
 Operator : CG/JU
 Sample : PB147203BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB147203BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM036401.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.357	380	386	402	rBV	4158907	6119823	44.29%	9.511%
2	6.969	653	660	677	rBV	4044494	6235738	45.13%	9.691%
3	7.787	791	799	810	rBV	1009580	1565562	11.33%	2.433%
4	8.957	988	998	1017	rBV	3530412	5899209	42.70%	9.168%
5	10.586	1268	1275	1296	rBV	1294607	2270044	16.43%	3.528%
6	13.057	1688	1695	1718	rBV	8835218	12753709	92.31%	19.821%
7	14.433	1922	1929	1943	rBV	1875450	2816030	20.38%	4.376%
8	15.921	2176	2182	2202	rBV	3860286	5512791	39.90%	8.568%
9	17.180	2389	2396	2412	rBV	1955907	2956625	21.40%	4.595%
10	19.809	2837	2843	2852	rBV	11493874	13816308	100.00%	21.472%
11	21.362	3102	3107	3115	rBV	1750802	2363893	17.11%	3.674%
12	23.686	3496	3502	3516	rVB2	1035984	2035619	14.73%	3.164%




Sum of corrected areas: 64345351

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082522\
Data File : BM036401.D
Acq On : 25 Aug 2022 11:51
Operator : CG/JU
Sample : PB147203BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB147203BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

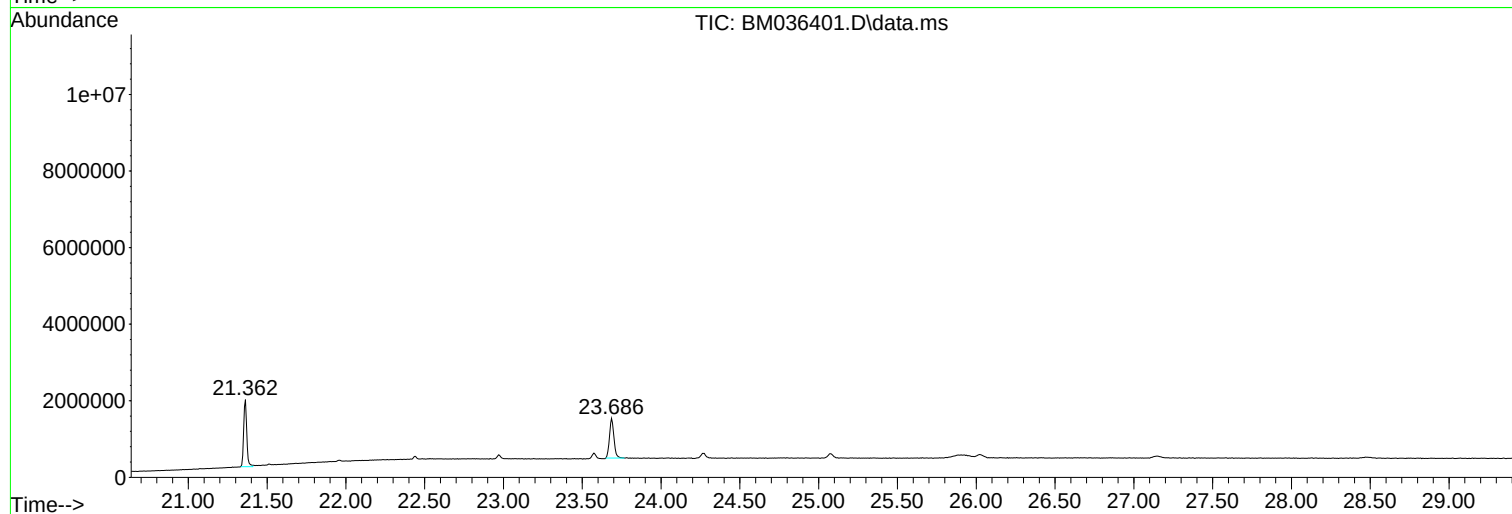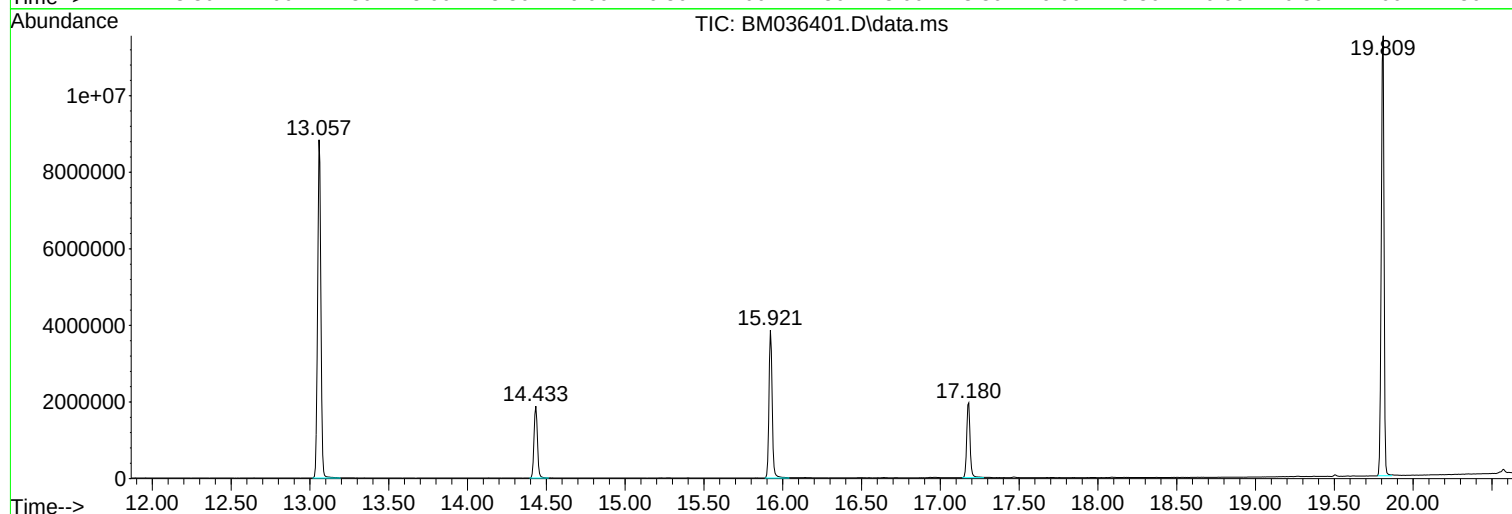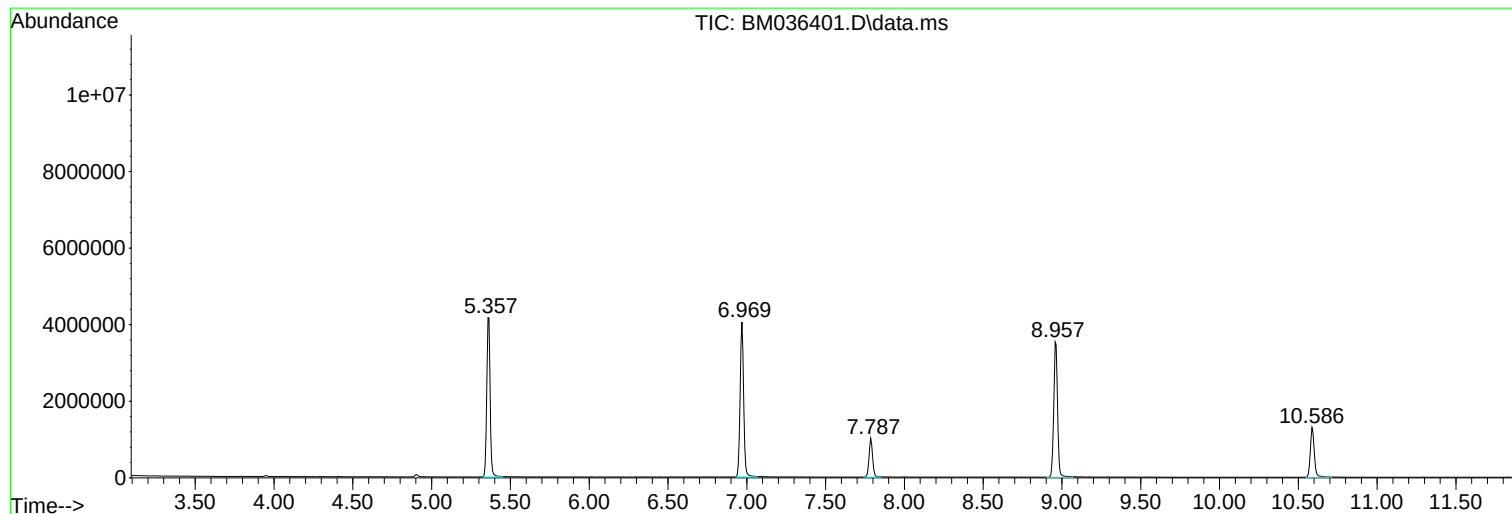

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082522\
Data File : BM036401.D
Acq On : 25 Aug 2022 11:51
Operator : CG/JU
Sample : PB147203BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB147203BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082522\
Data File : BM036401.D
Acq On : 25 Aug 2022 11:51
Operator : CG/JU
Sample : PB147203BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB147203BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------