
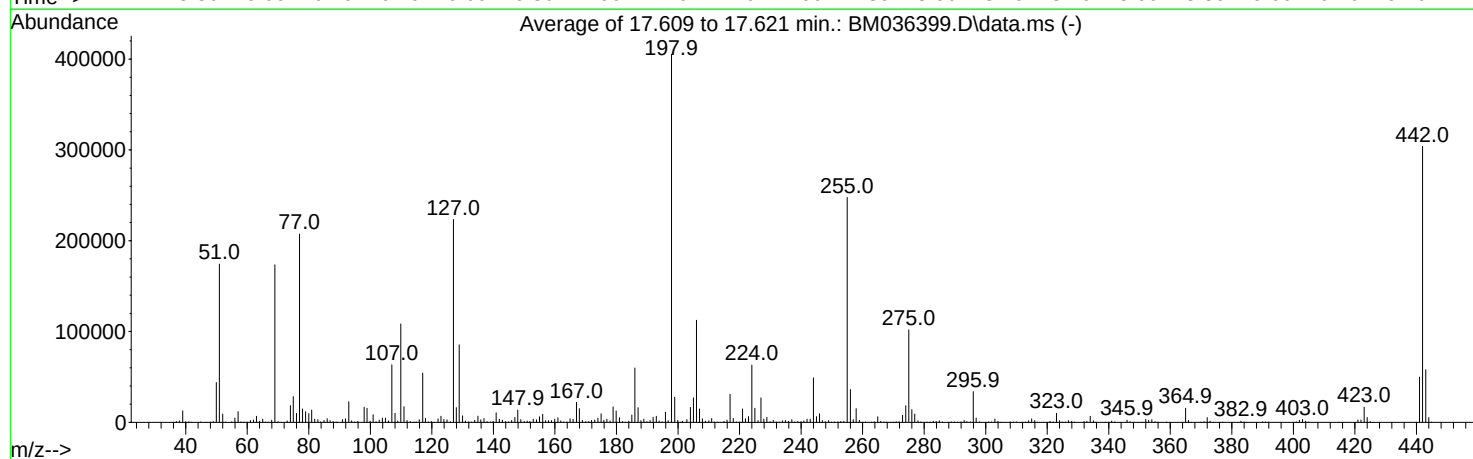


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082522\
 Data File : BM036399.D
 Acq On : 25 Aug 2022 10:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 25 15:21:00 2022

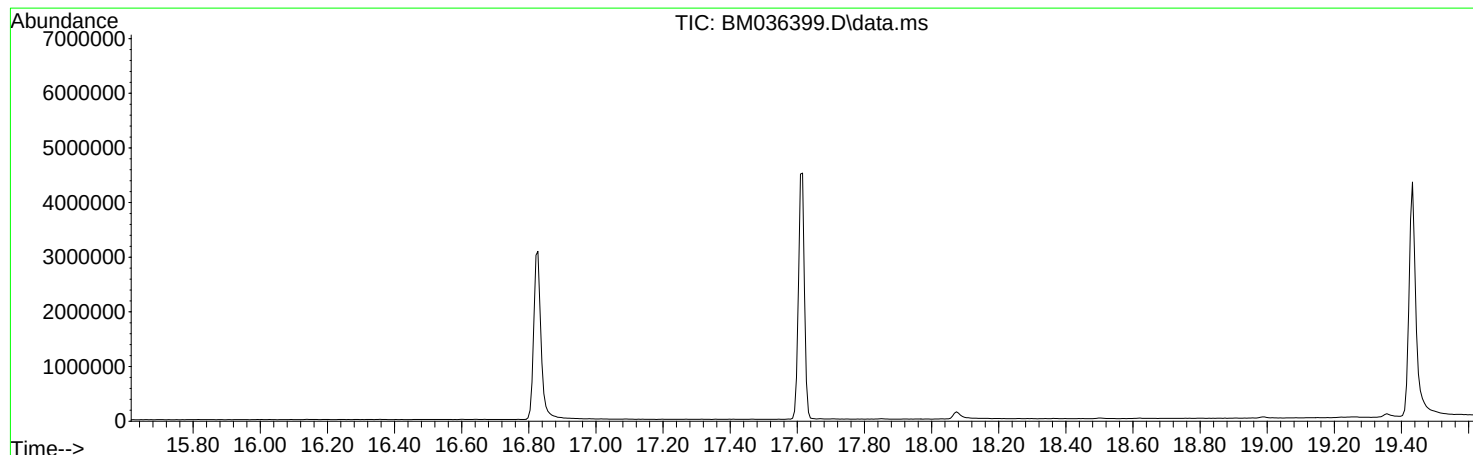




AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.0	174203	PASS
68	69	0.00	2	1.4	2449	PASS
69	198	0.00	100	42.8	173574	PASS
70	69	0.00	2	0.4	763	PASS
127	198	10	80	55.1	223363	PASS
197	198	0.00	2	0.4	1783	PASS
198	198	100	100	100.0	405205	PASS
199	198	5	9	6.8	27670	PASS
275	198	10	60	25.1	101805	PASS
365	198	1	100	3.8	15405	PASS
441	198	0.01	100	12.3	49755	PASS
442	442	50	100	100.0	303893	PASS
443	442	15	24	19.1	57968	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082522\
 Data File : BM036399.D
 Acq On : 25 Aug 2022 10:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Aug 26 07:19:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 25 15:21:00 2022
 Response via : Initial Calibration

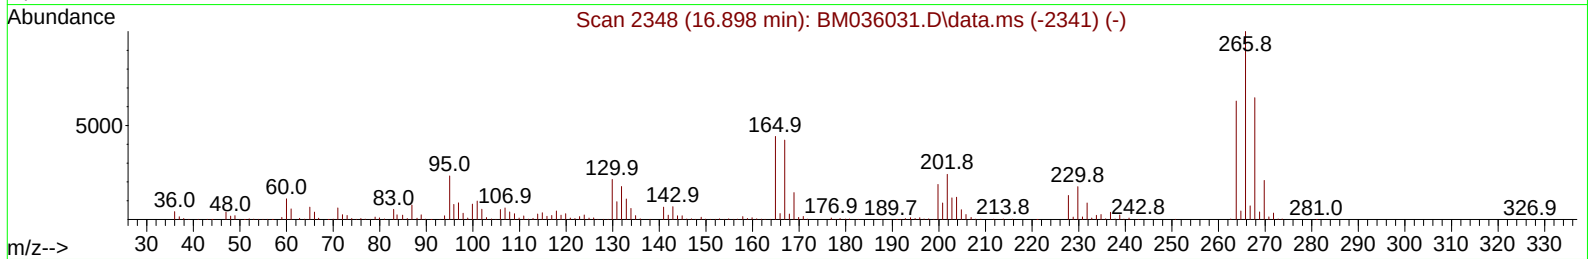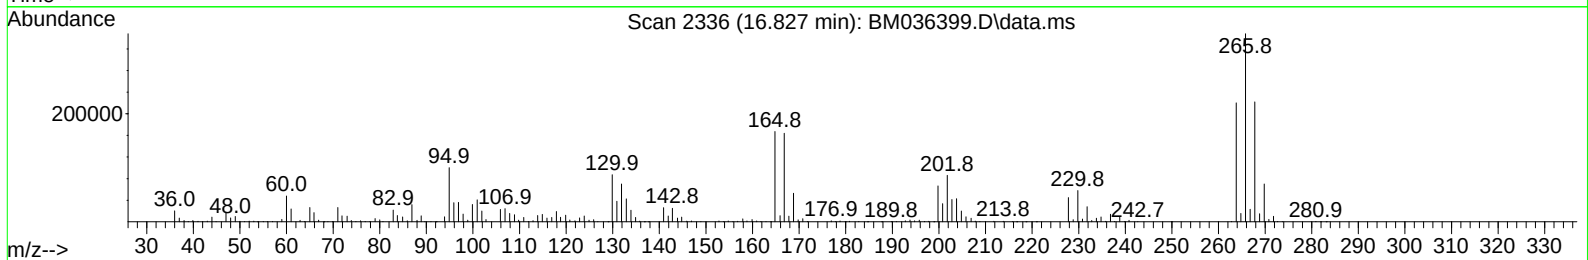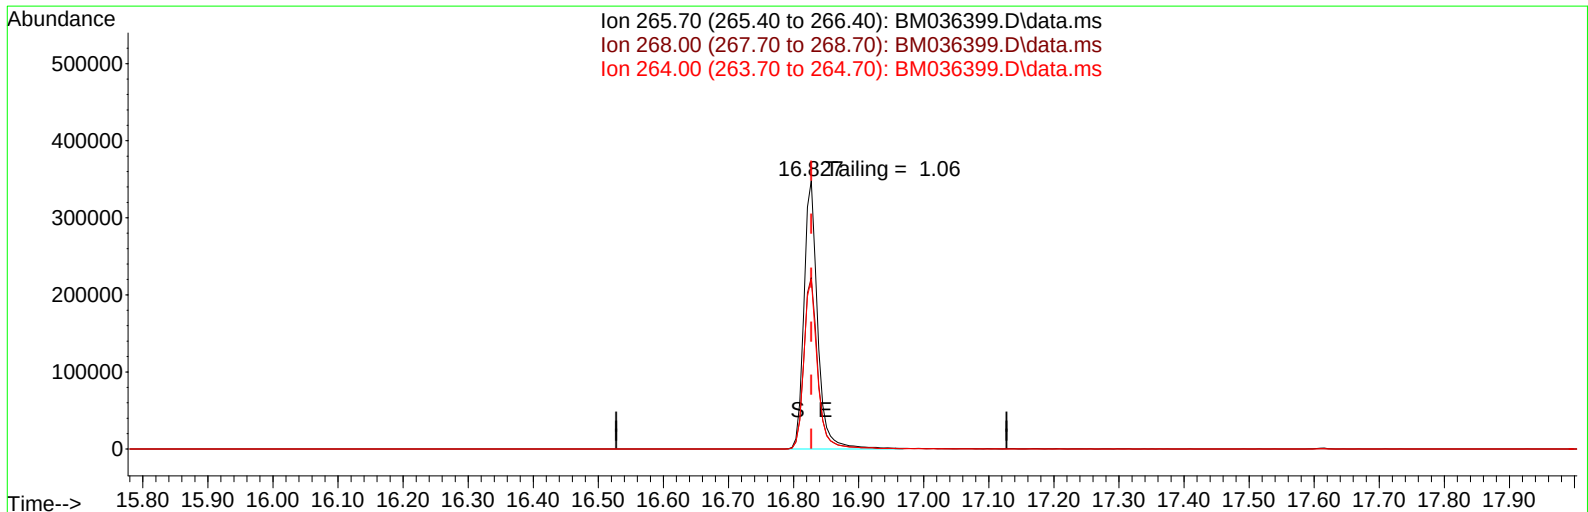

TIC: BM036399.D\data.ms

(70) Pentachlorophenol (C)

16.827min (-0.000) 1122501.82 ng




response 513060

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.79
264.00	63.30	63.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM082522\
 Data File : BM036399.D
 Acq On : 25 Aug 2022 10:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Aug 26 07:19:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 25 15:21:00 2022
 Response via : Initial Calibration

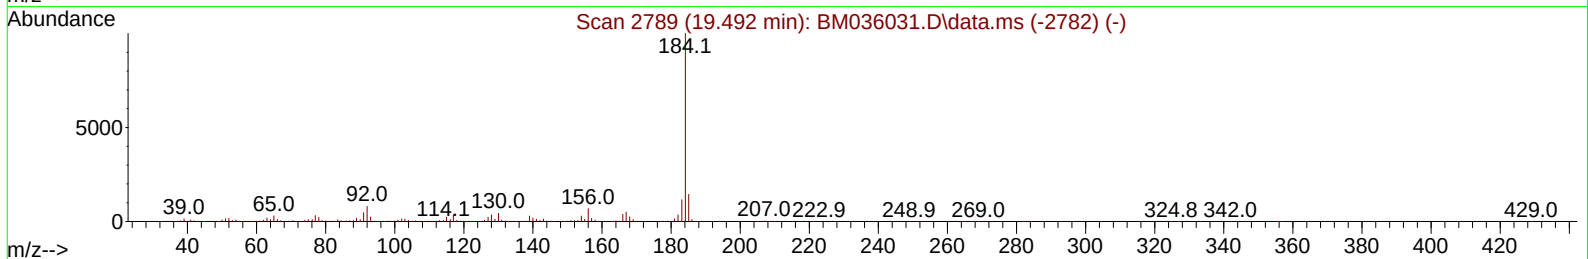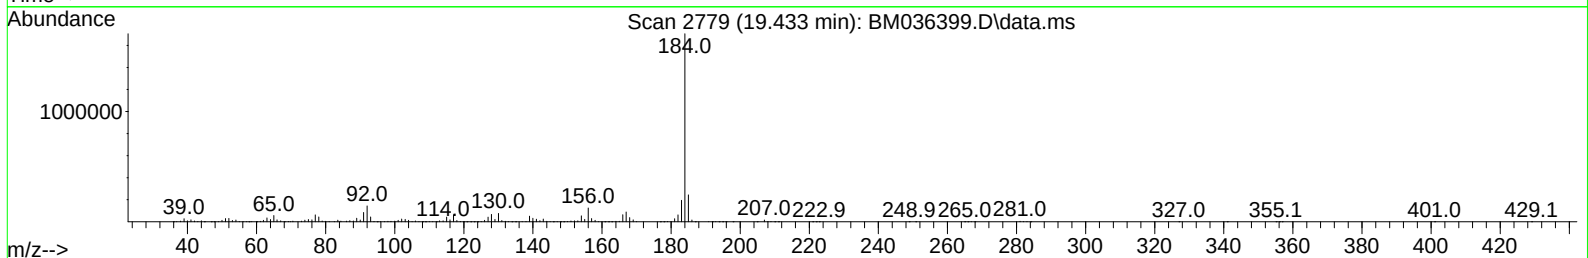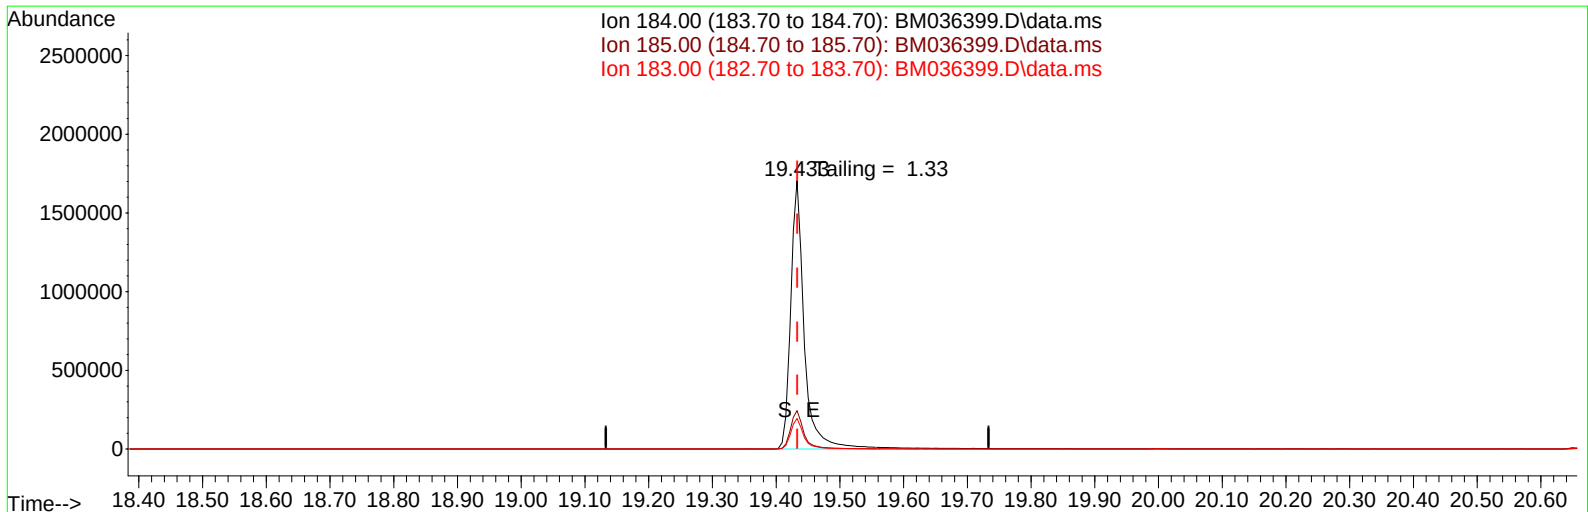

TIC: BM036399.D\data.ms

(77) Benzidine

19.433min (-0.000) 312081.71 ng

response 2550766

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.30
183.00	11.90	11.42
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/25/2022	BNA_M	<u>BM036399.D</u>
Compound Name	Response	Retention Time
DDT	1424175	20.656
DDD	7608	20.262
DDE	419	19.709
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8027	1432202	0.56

Instrument :
BNA_M
ClientSampleId :
DFTPP