



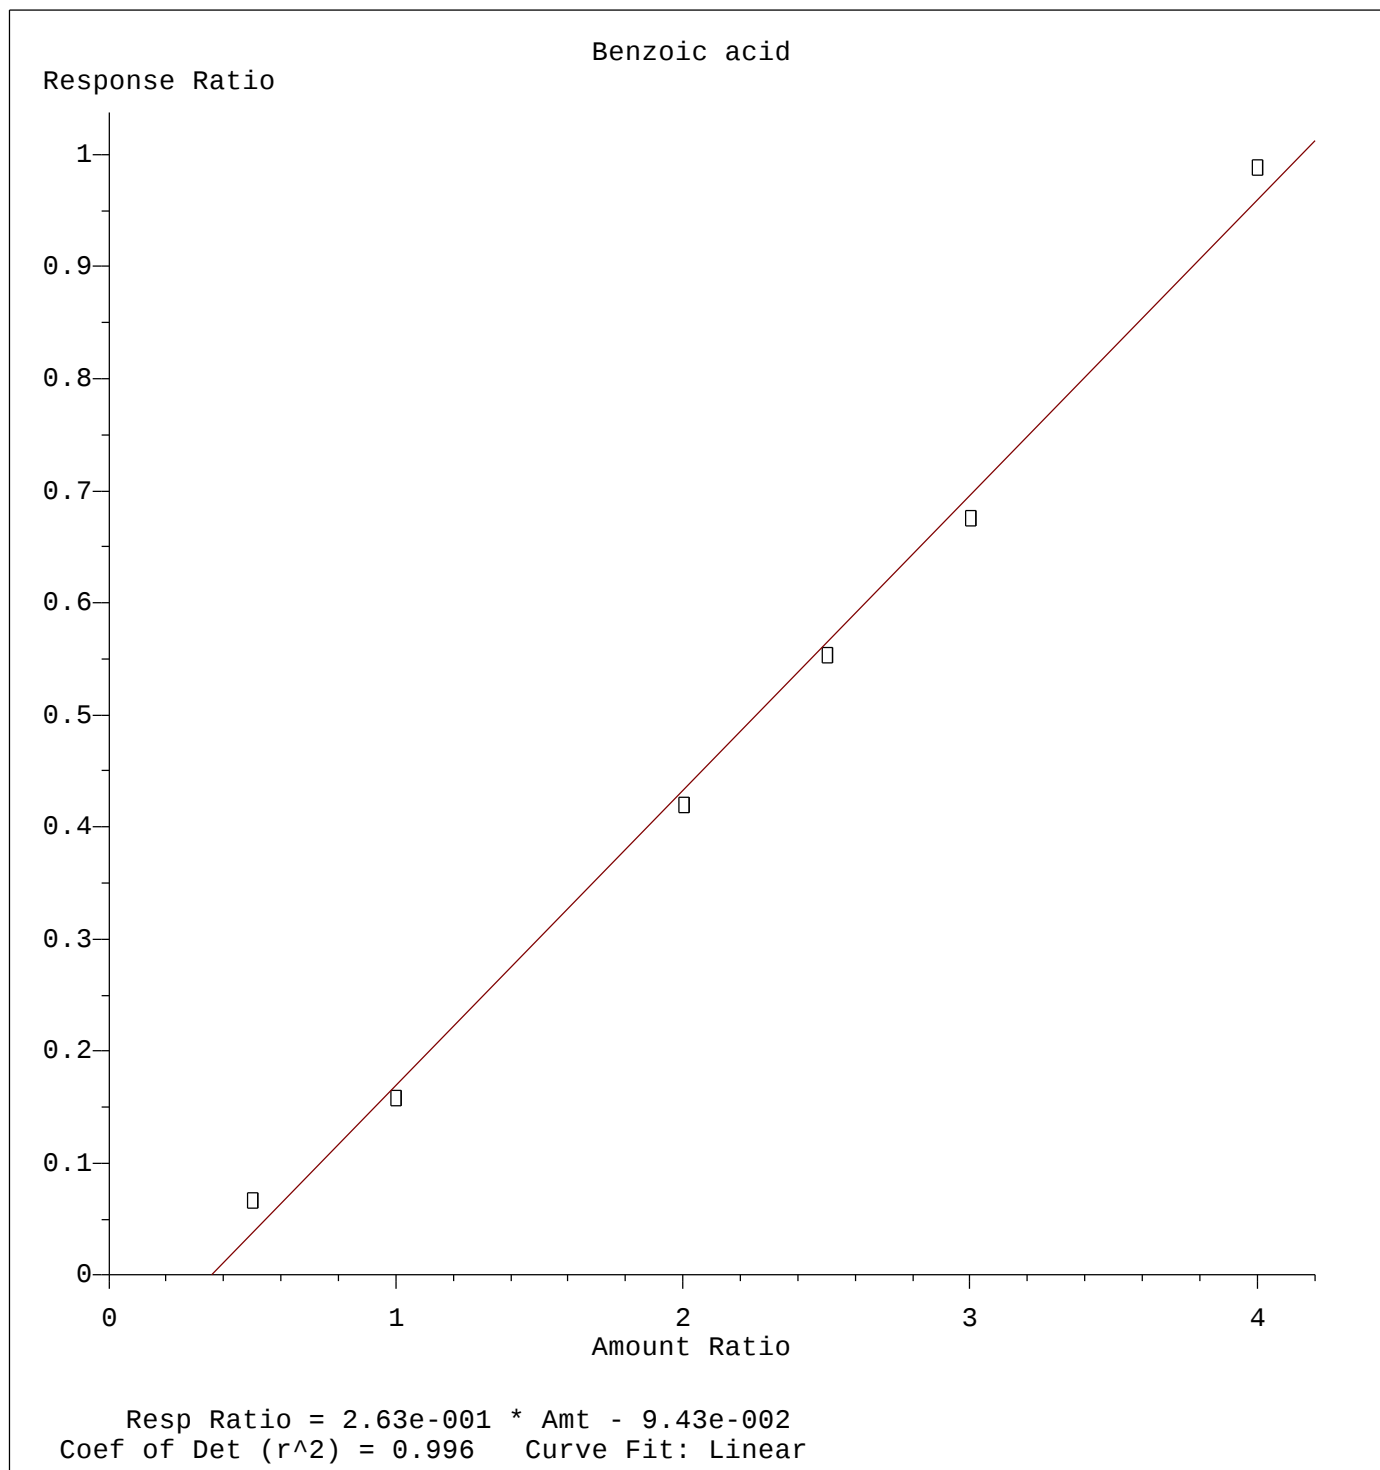

Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM090220.M
Calibration Table Last Updated: Wed Sep 02 18:43:48 2020

3-Nitroaniline

Response Ratio

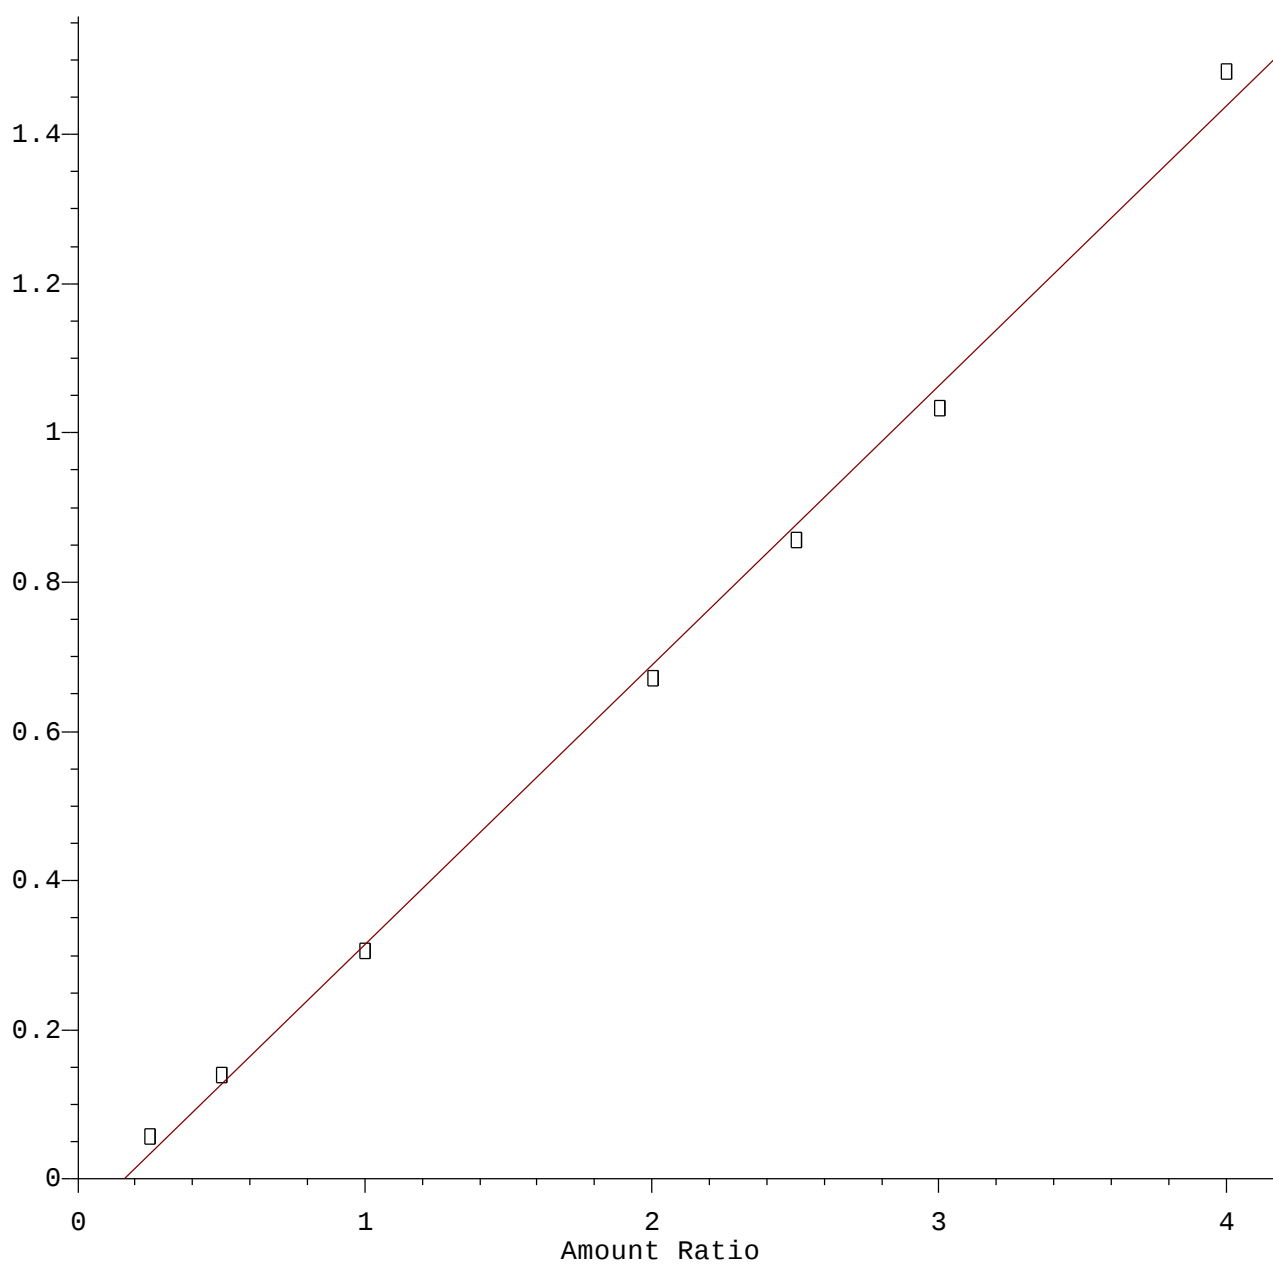


Resp Ratio = $3.74 \times 10^{-1} \times \text{Amt} - 5.96 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM090220.M
Calibration Table Last Updated: Wed Sep 02 18:43:48 2020

2,4-Dinitrophenol

Response Ratio

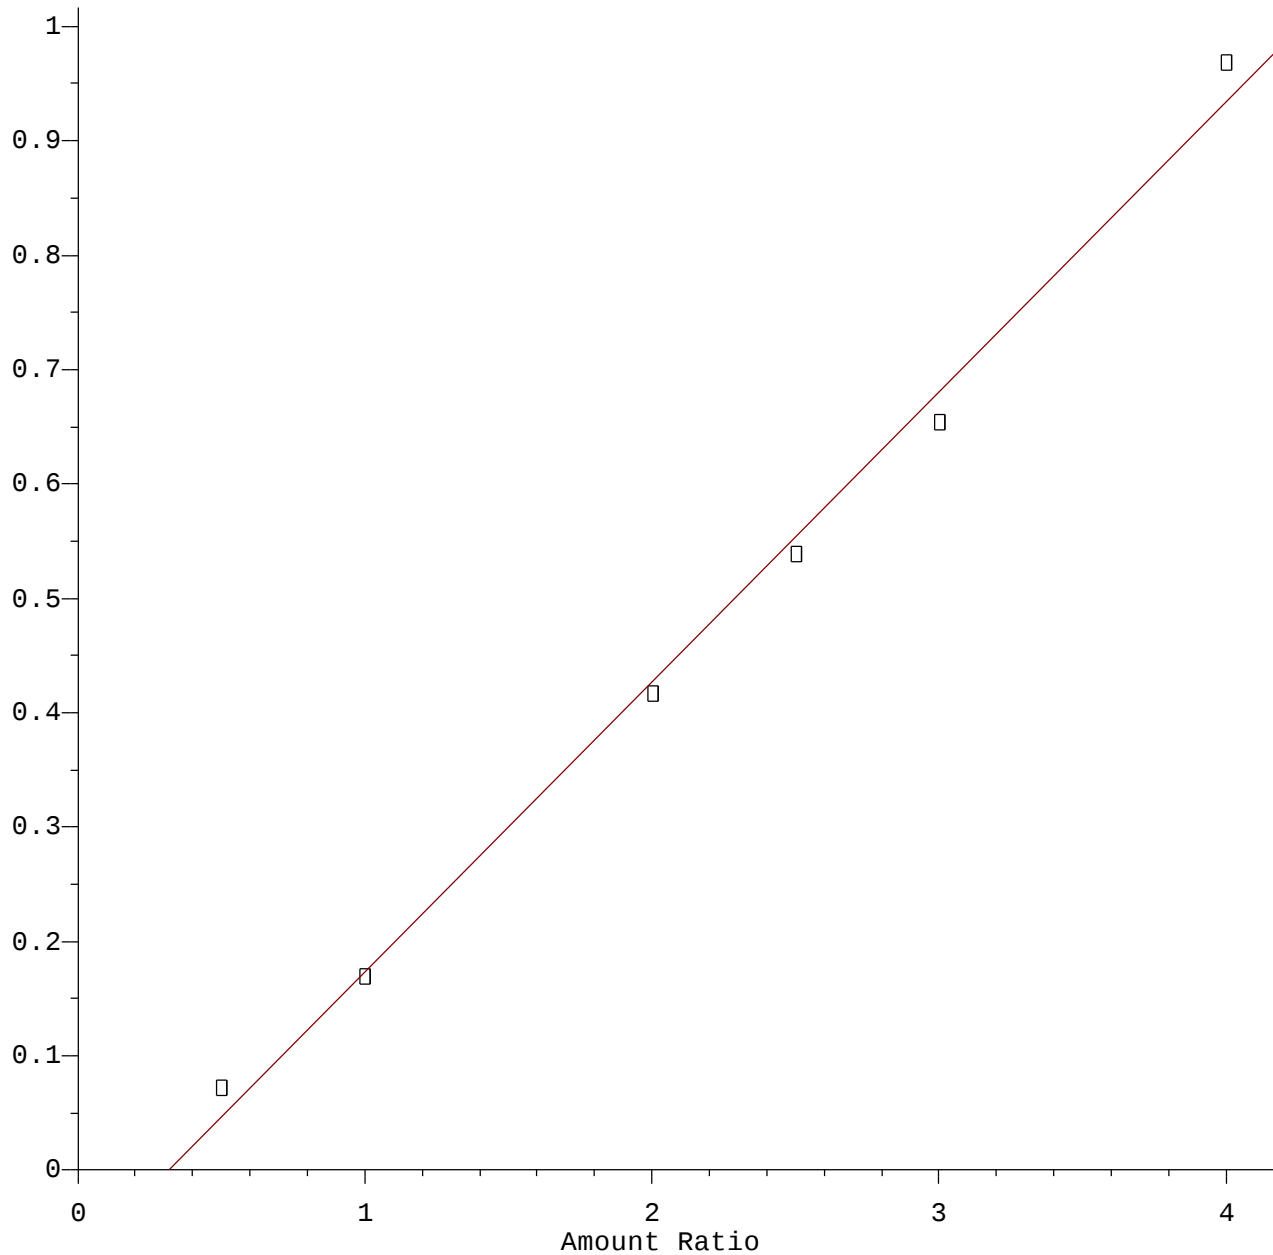


Resp Ratio = $2.54 \times 10^{-1} \times \text{Amt} - 8.01 \times 10^{-2}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM090220.M
Calibration Table Last Updated: Wed Sep 02 18:43:48 2020


4-Nitroaniline

Response Ratio

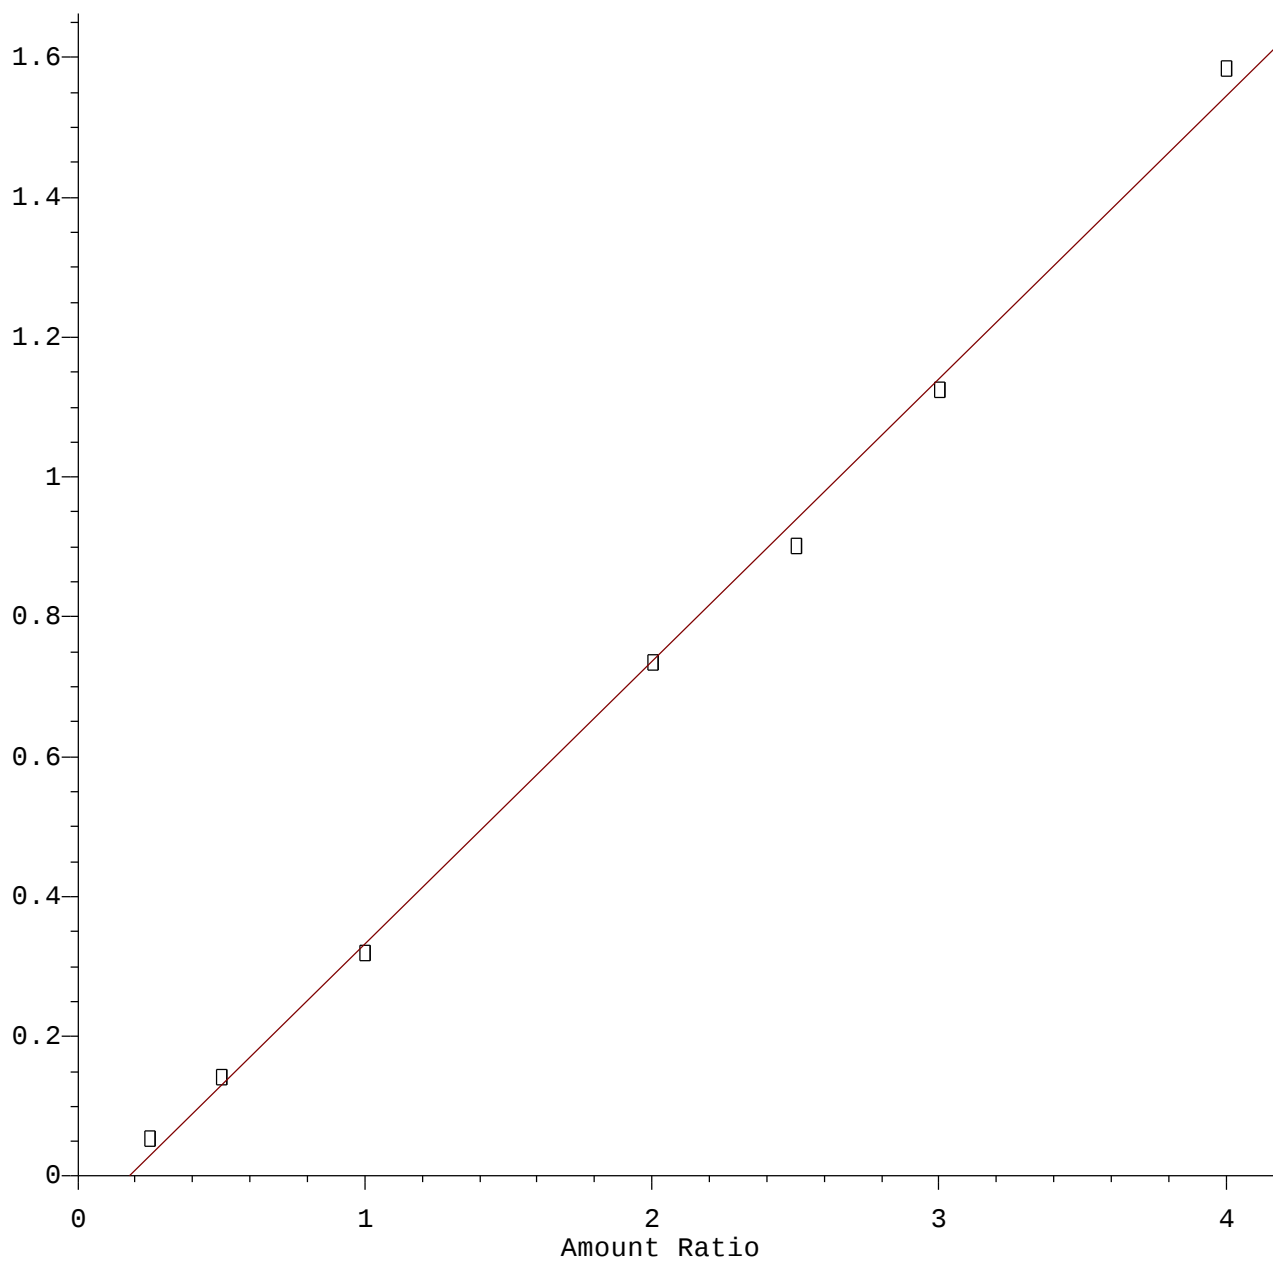


Resp Ratio = $4.04 \times 10^{-1} \times \text{Amt} - 7.10 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM090220.M
Calibration Table Last Updated: Wed Sep 02 18:43:48 2020

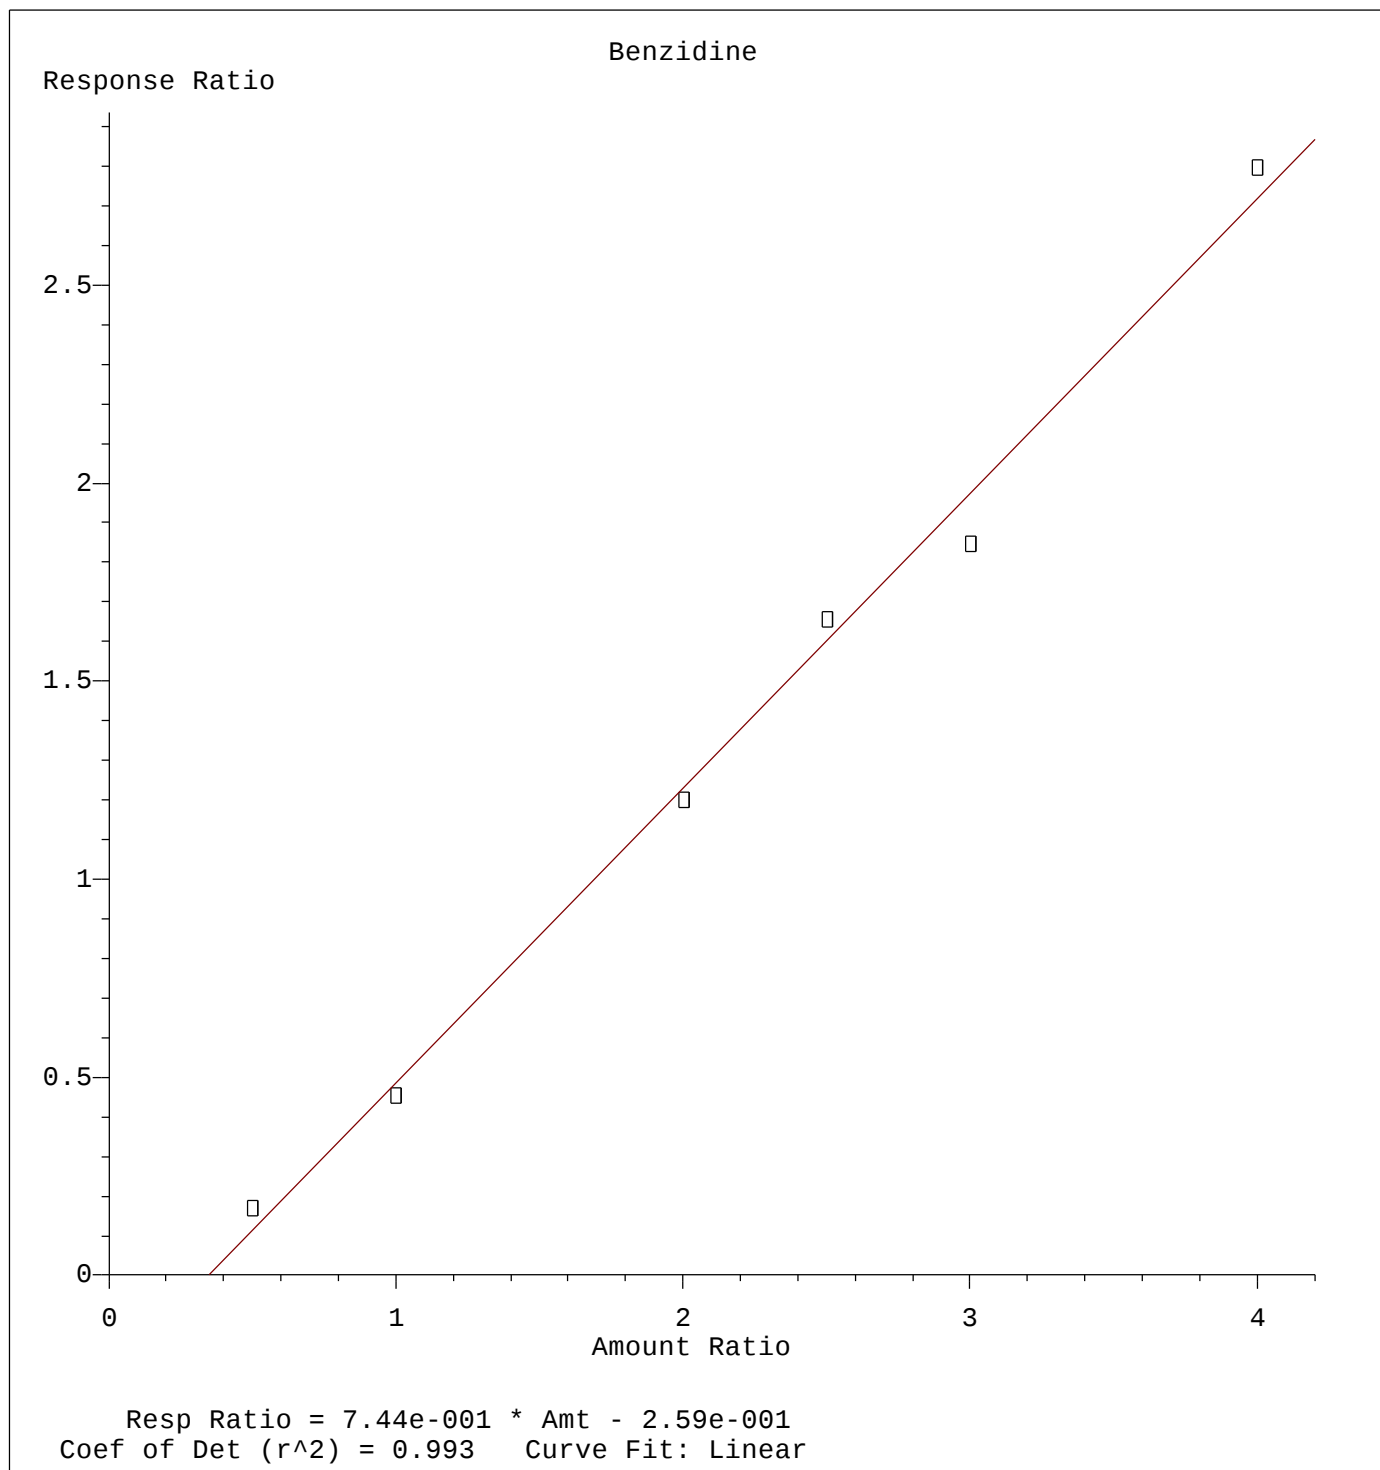


Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM090220.M
Calibration Table Last Updated: Wed Sep 02 18:43:48 2020

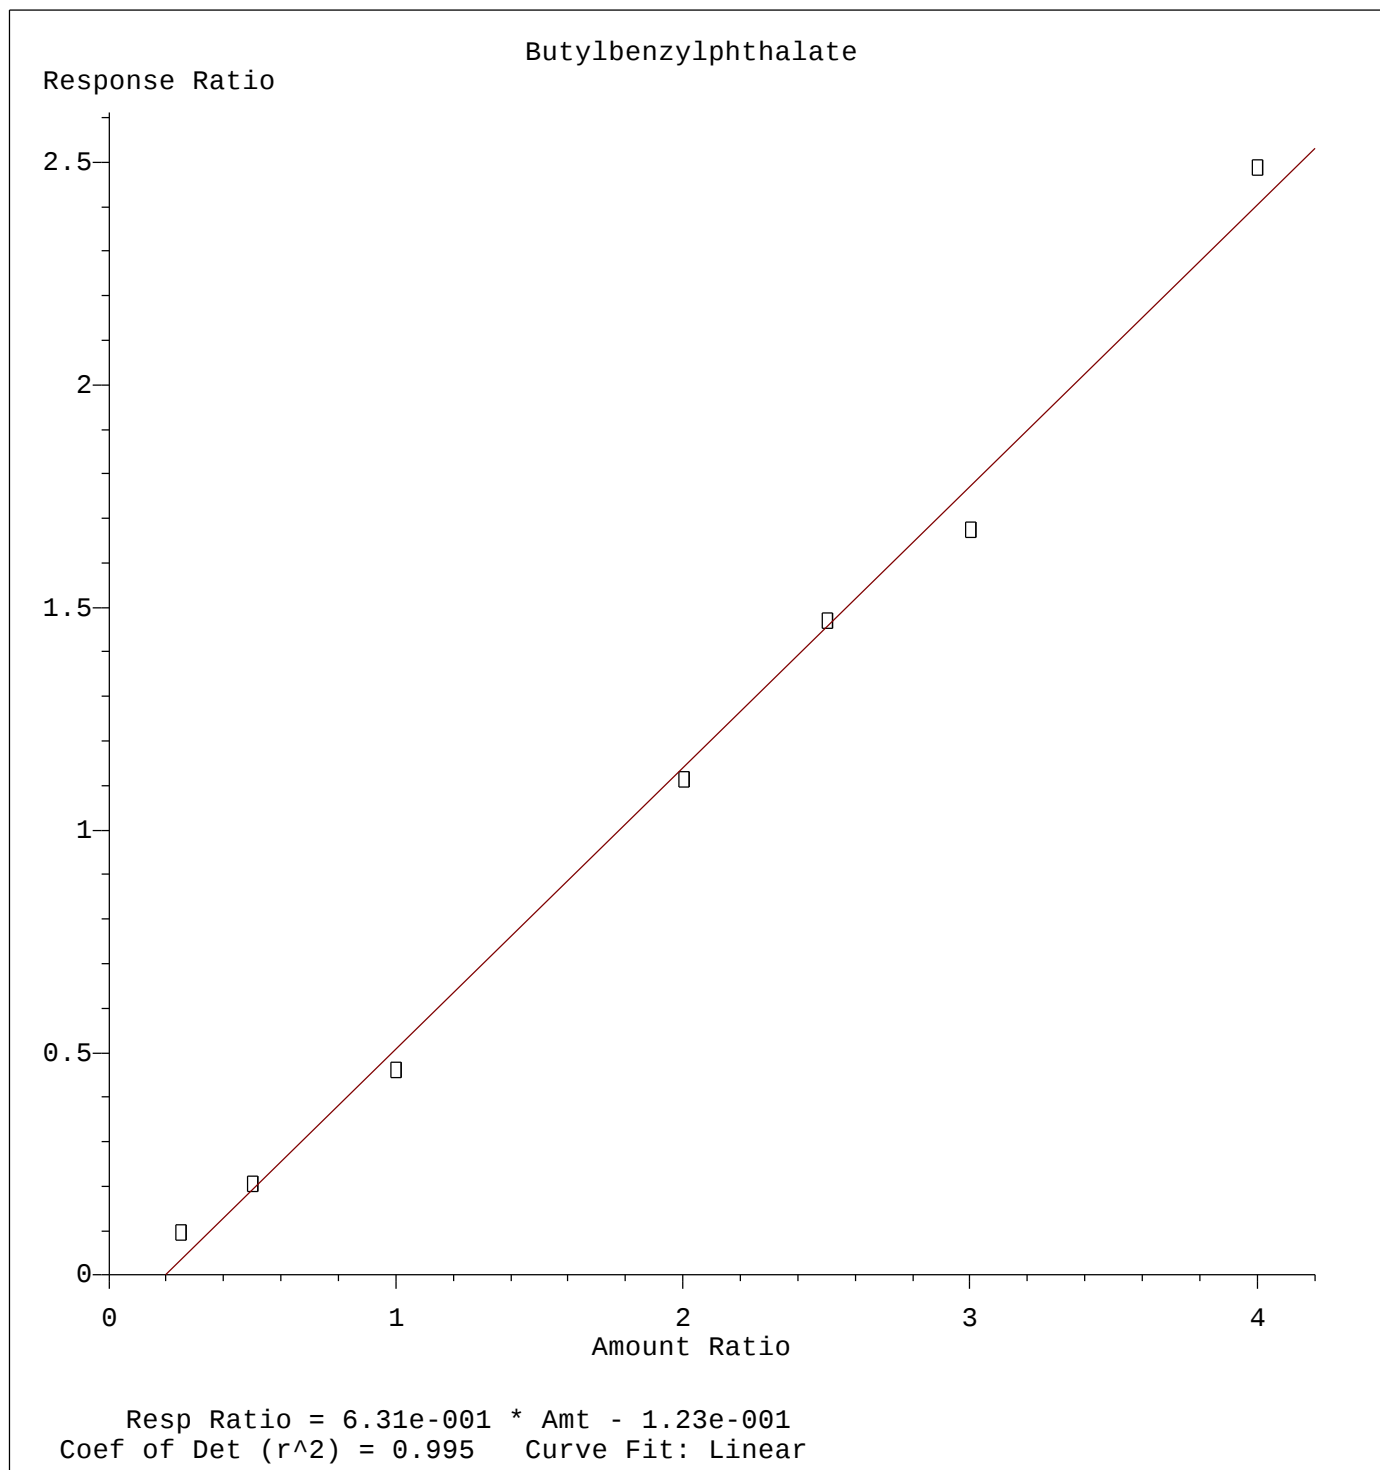

Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM090220.M
Calibration Table Last Updated: Wed Sep 02 18:43:48 2020

3,3'-Dichlorobenzidine

Response Ratio

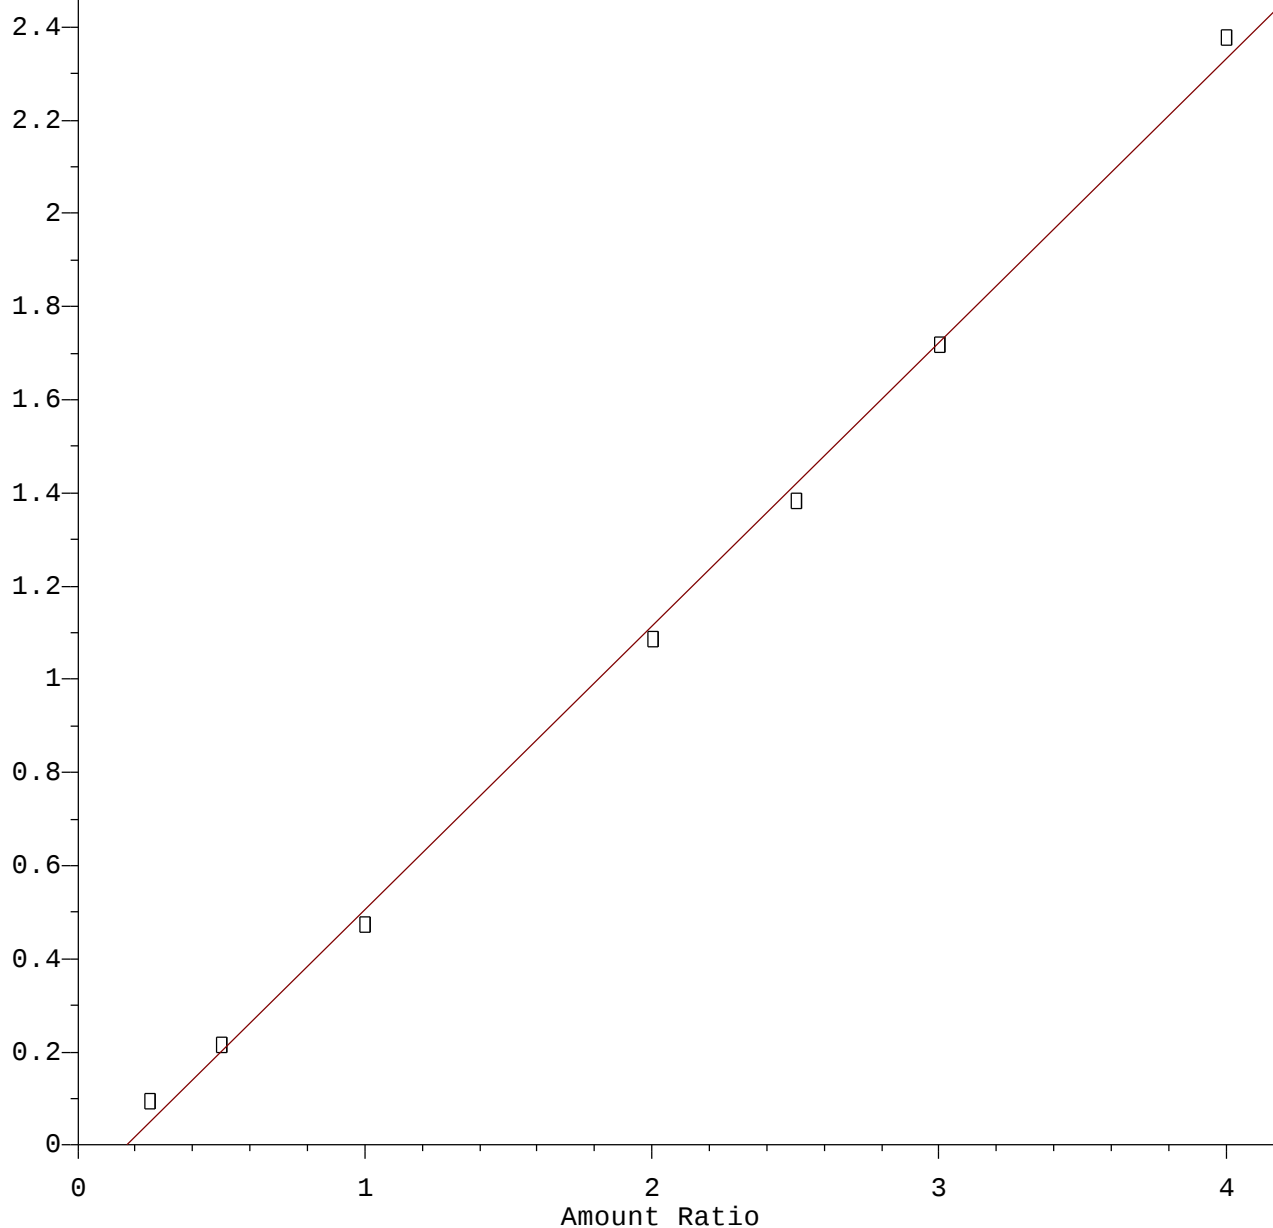

Resp Ratio = $6.08 \times 10^{-1} \times \text{Amt} - 1.03 \times 10^{-1}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM090220.M
Calibration Table Last Updated: Wed Sep 02 18:43:48 2020