
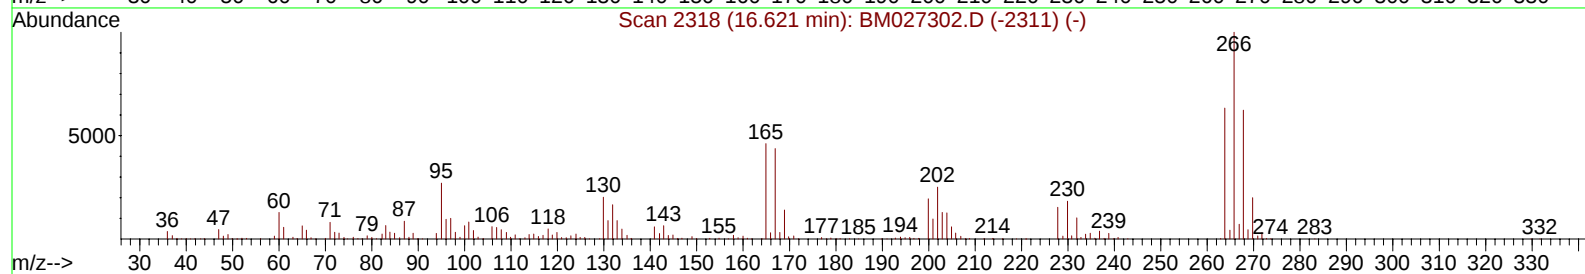
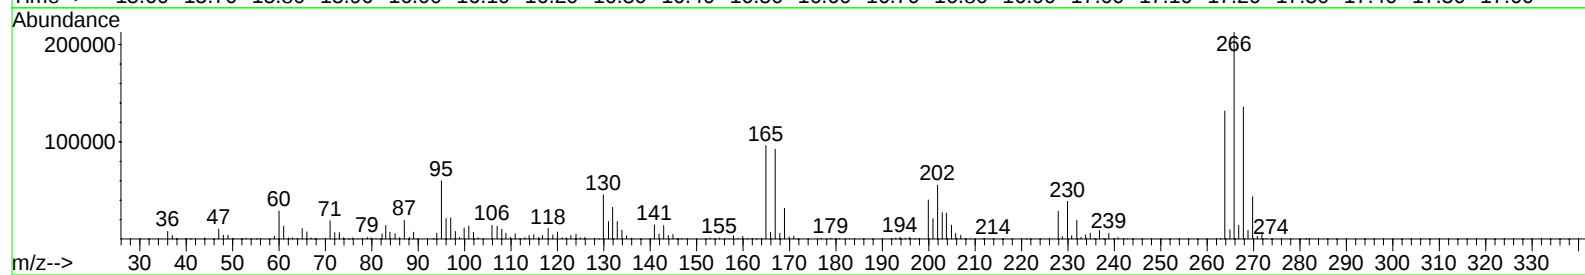


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090220\
Data File : BM027298.D
Acq On : 02 Sep 2020 10:16
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 02 18:37:31 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM090220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 02 16:21:29 2020
Response via : Initial Calibration

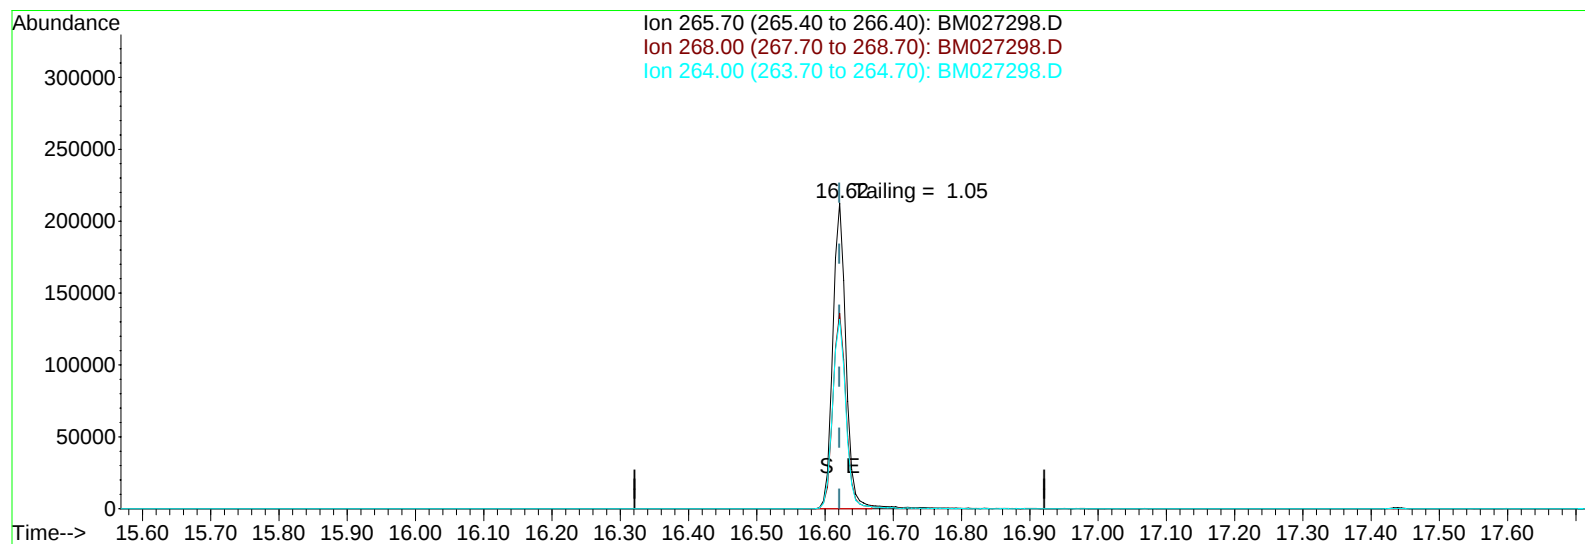

TIC: BM027298.D

(70) Pentachlorophenol (C)




16.621min (+0.000) 0.00ng

response 284377

Ion	Exp%	Act%
265.70	100	100
268.00	62.40	63.89
264.00	63.30	61.84
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090220\
Data File : BM027298.D
Acq On : 02 Sep 2020 10:16
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 02 18:37:31 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM090220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 02 16:21:29 2020
Response via : Initial Calibration

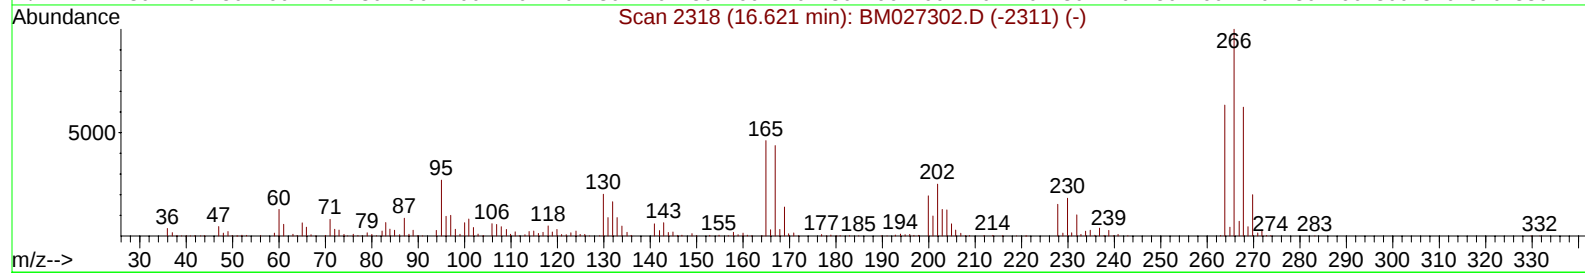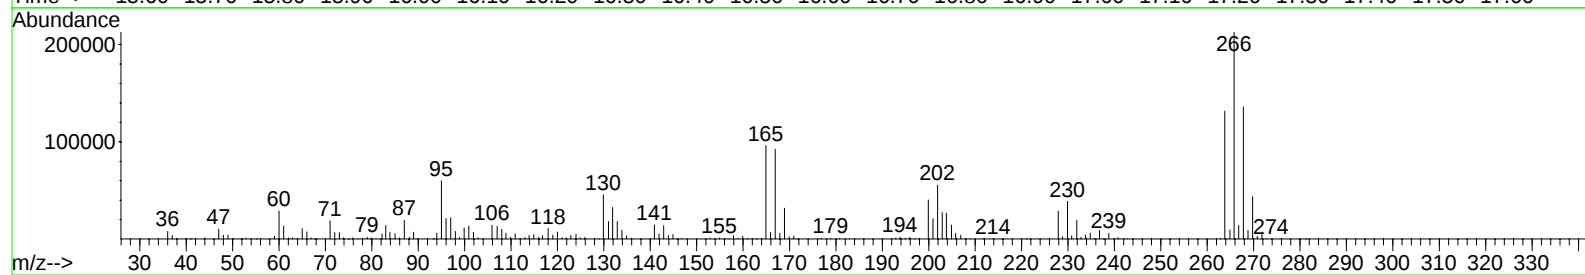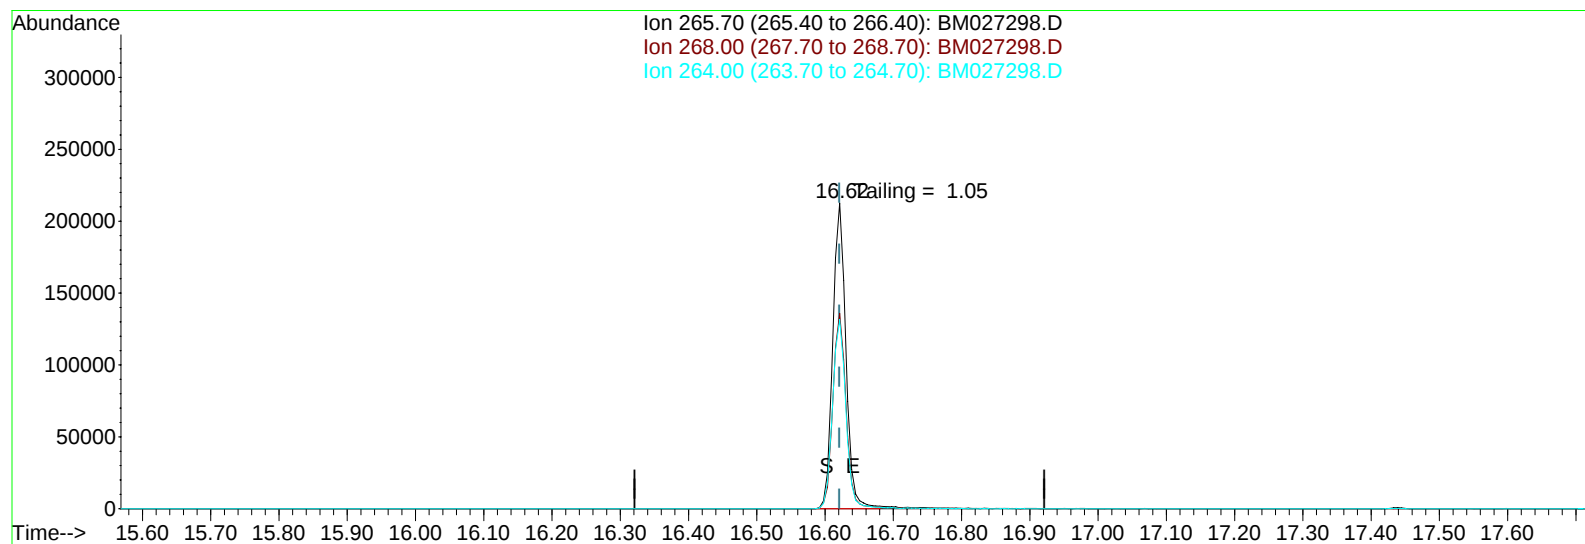

TIC: BM027298.D

(70) Pentachlorophenol (C)

16.621min (+0.000) 0.00ng

response 284377

Ion	Exp%	Act%
265.70	100	100
268.00	62.40	63.89
264.00	63.30	61.84
0.00	0.00	0.00