

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM090220\
 Data File : BM027307.D
 Acq On : 02 Sep 2020 17:13
 Operator : JU/CG
 Sample : PB131374BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB131374BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM090220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.199	370	376	392	rBV	3383058	4999741	29.96%	8.835%
2	6.769	635	643	657	rBV	3296441	5081709	30.45%	8.980%
3	7.575	774	780	790	rVB	566783	888595	5.32%	1.570%
4	8.722	966	975	989	rBV	2210051	3566754	21.37%	6.303%
5	10.345	1244	1251	1262	rBV	676960	1124023	6.73%	1.986%
6	12.839	1667	1675	1686	rBV	5843558	8505706	50.96%	15.031%
7	14.216	1902	1909	1922	rVB	1122226	1646857	9.87%	2.910%
8	15.710	2156	2163	2182	rBV	5350595	7464324	44.72%	13.191%
9	16.963	2370	2376	2389	rBV	1493323	2034948	12.19%	3.596%
10	19.615	2820	2827	2838	rBV	13922748	16690371	100.00%	29.495%
11	21.162	3085	3090	3098	rBV	1810058	2365776	14.17%	4.181%
12	23.339	3454	3460	3472	rVB	1276654	2218819	13.29%	3.921%


Sum of corrected areas: 56587623

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM090220\
Data File : BM027307.D
Acq On : 02 Sep 2020 17:13
Operator : JU/CG
Sample : PB131374BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB131374BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM090220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

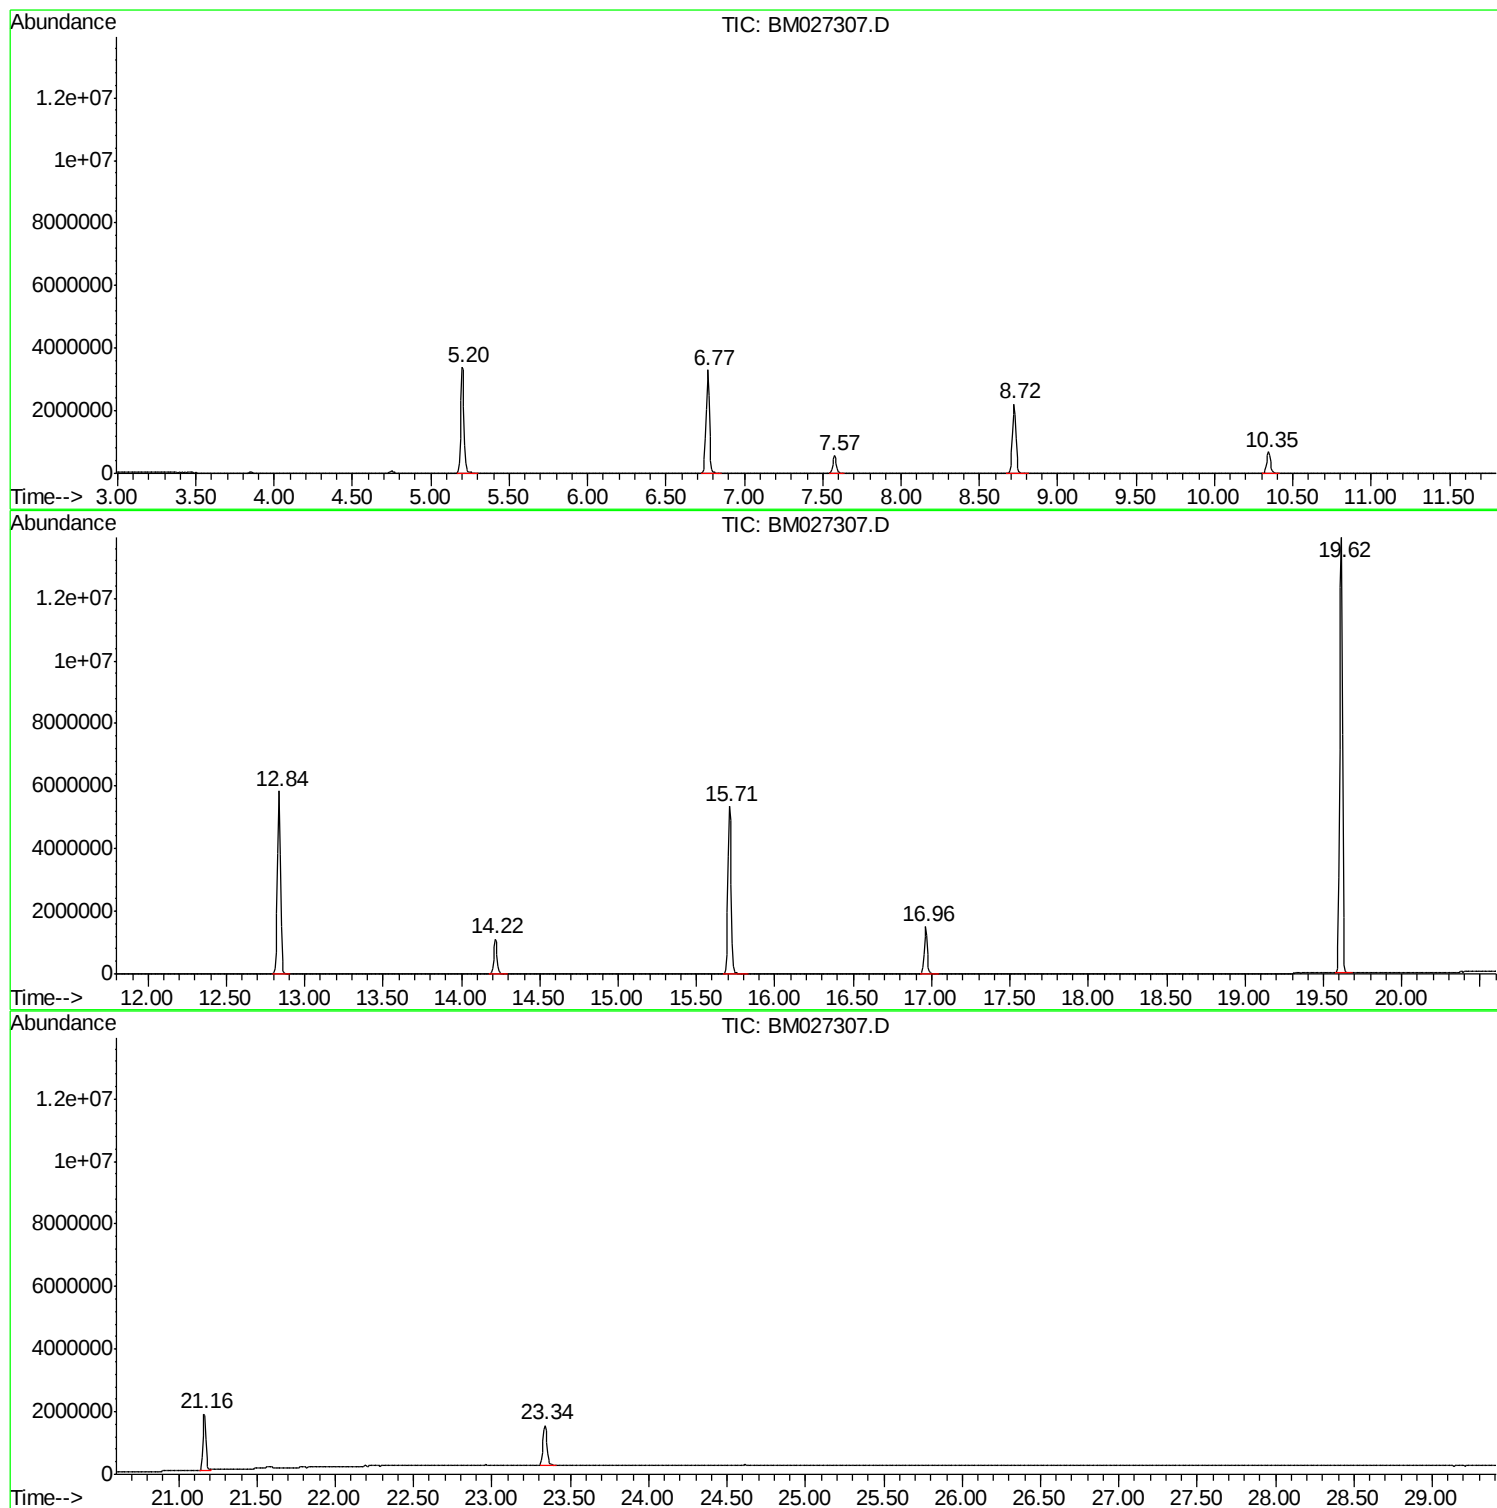

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090220\
Data File : BM027307.D
Acq On : 02 Sep 2020 17:13
Operator : JU/CG
Sample : PB131374BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB131374BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM090220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090220\
Data File : BM027307.D
Acq On : 02 Sep 2020 17:13
Operator : JU/CG
Sample : PB131374BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB131374BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM090220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc