


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM090220\
 Data File : BM027298.D
 Acq On : 02 Sep 2020 10:16
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM090220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 02 16:21:29 2020

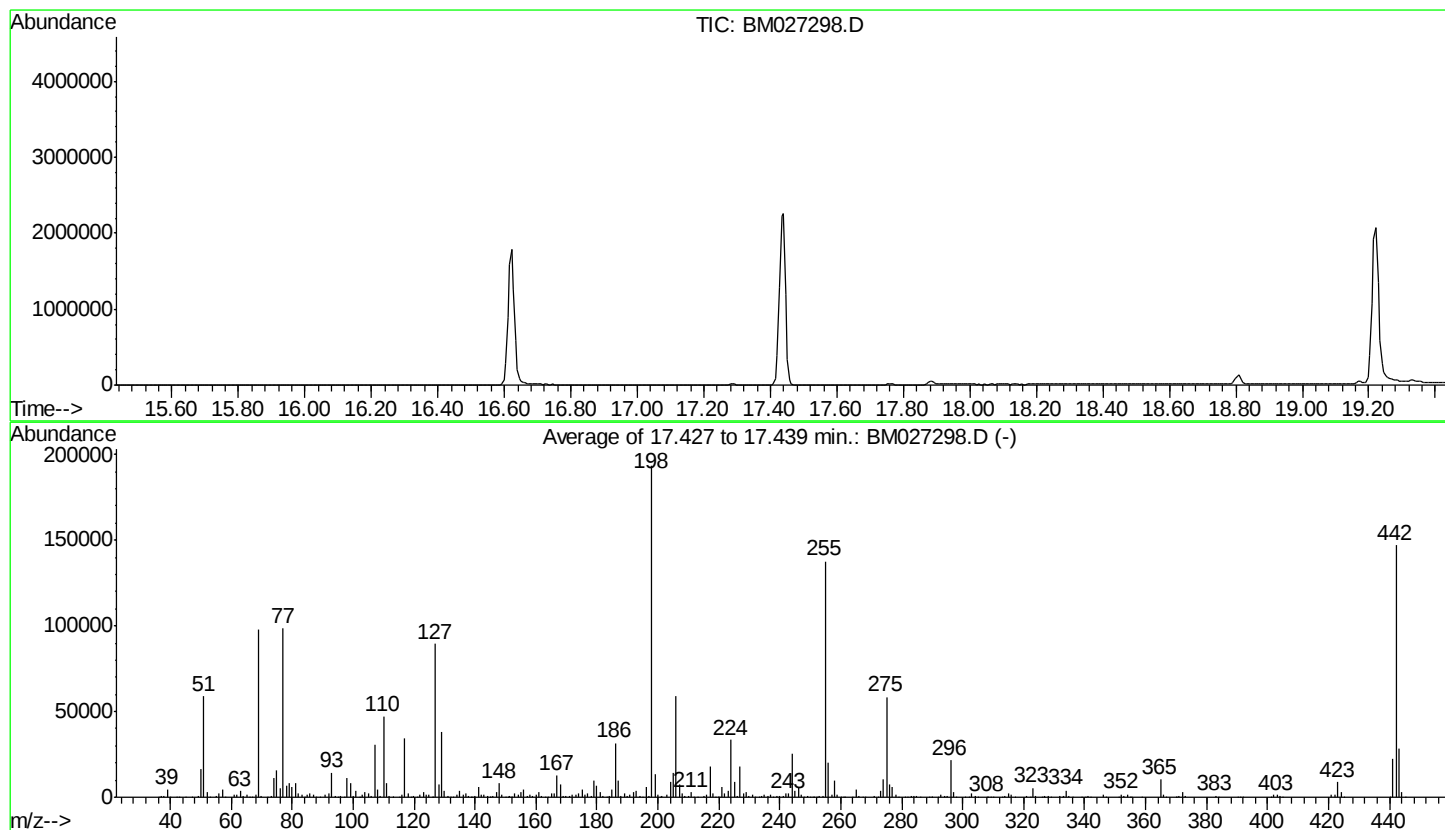

AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	58920	PASS
68	69	0.00	2	1.8	1761	PASS
69	198	0.00	100	50.8	98185	PASS
70	69	0.00	2	0.6	546	PASS
127	198	10	80	46.3	89576	PASS
197	198	0.00	2	0.6	1104	PASS
198	198	100	100	100.0	193450	PASS
199	198	5	9	7.1	13782	PASS
275	198	10	60	30.2	58445	PASS
365	198	1	100	5.3	10166	PASS
441	198	0.01	100	11.8	22746	PASS
442	198	50	100	75.9	146810	PASS
443	442	15	24	19.5	28616	PASS