

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091424\
 Data File : BM047520.D
 Acq On : 14 Sep 2024 11:57
 Operator : RC/JU
 Sample : SSTDICC2.5
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC2.5

Quant Time: Sep 15 08:16:42 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 08:15:39 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	331818	20.000	ng	0.00
21) Naphthalene-d8	10.645	136	1431277	20.000	ng	0.00
39) Acenaphthene-d10	14.480	164	860230	20.000	ng	0.00
64) Phenanthrene-d10	17.215	188	1698459	20.000	ng	0.00
76) Chrysene-d12	21.439	240	1448703	20.000	ng	0.00
86) Perylene-d12	24.468	264	1514067	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	0.000	112	0d	0.000	ng	
7) Phenol-d6	0.000	99	0d	0.000	ng	
23) Nitrobenzene-d5	0.000	82	0d	0.000	ng	
42) 2,4,6-Tribromophenol	0.000	330	0d	0.000	ng	
45) 2-Fluorobiphenyl	0.000	172	0d	0.000	ng	
79) Terphenyl-d14	0.000	244	0d	0.000	ng	
Target Compounds						
19) n-Nitroso-di-n-propyla...	8.651	70	44249	2.927	ng	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091424\
Data File : BM047520.D
Acq On : 14 Sep 2024 11:57
Operator : RC/JU
Sample : SSTDICC2.5
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTDICC2.5

Quant Time: Sep 15 08:16:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 08:15:39 2024
Response via : Initial Calibration

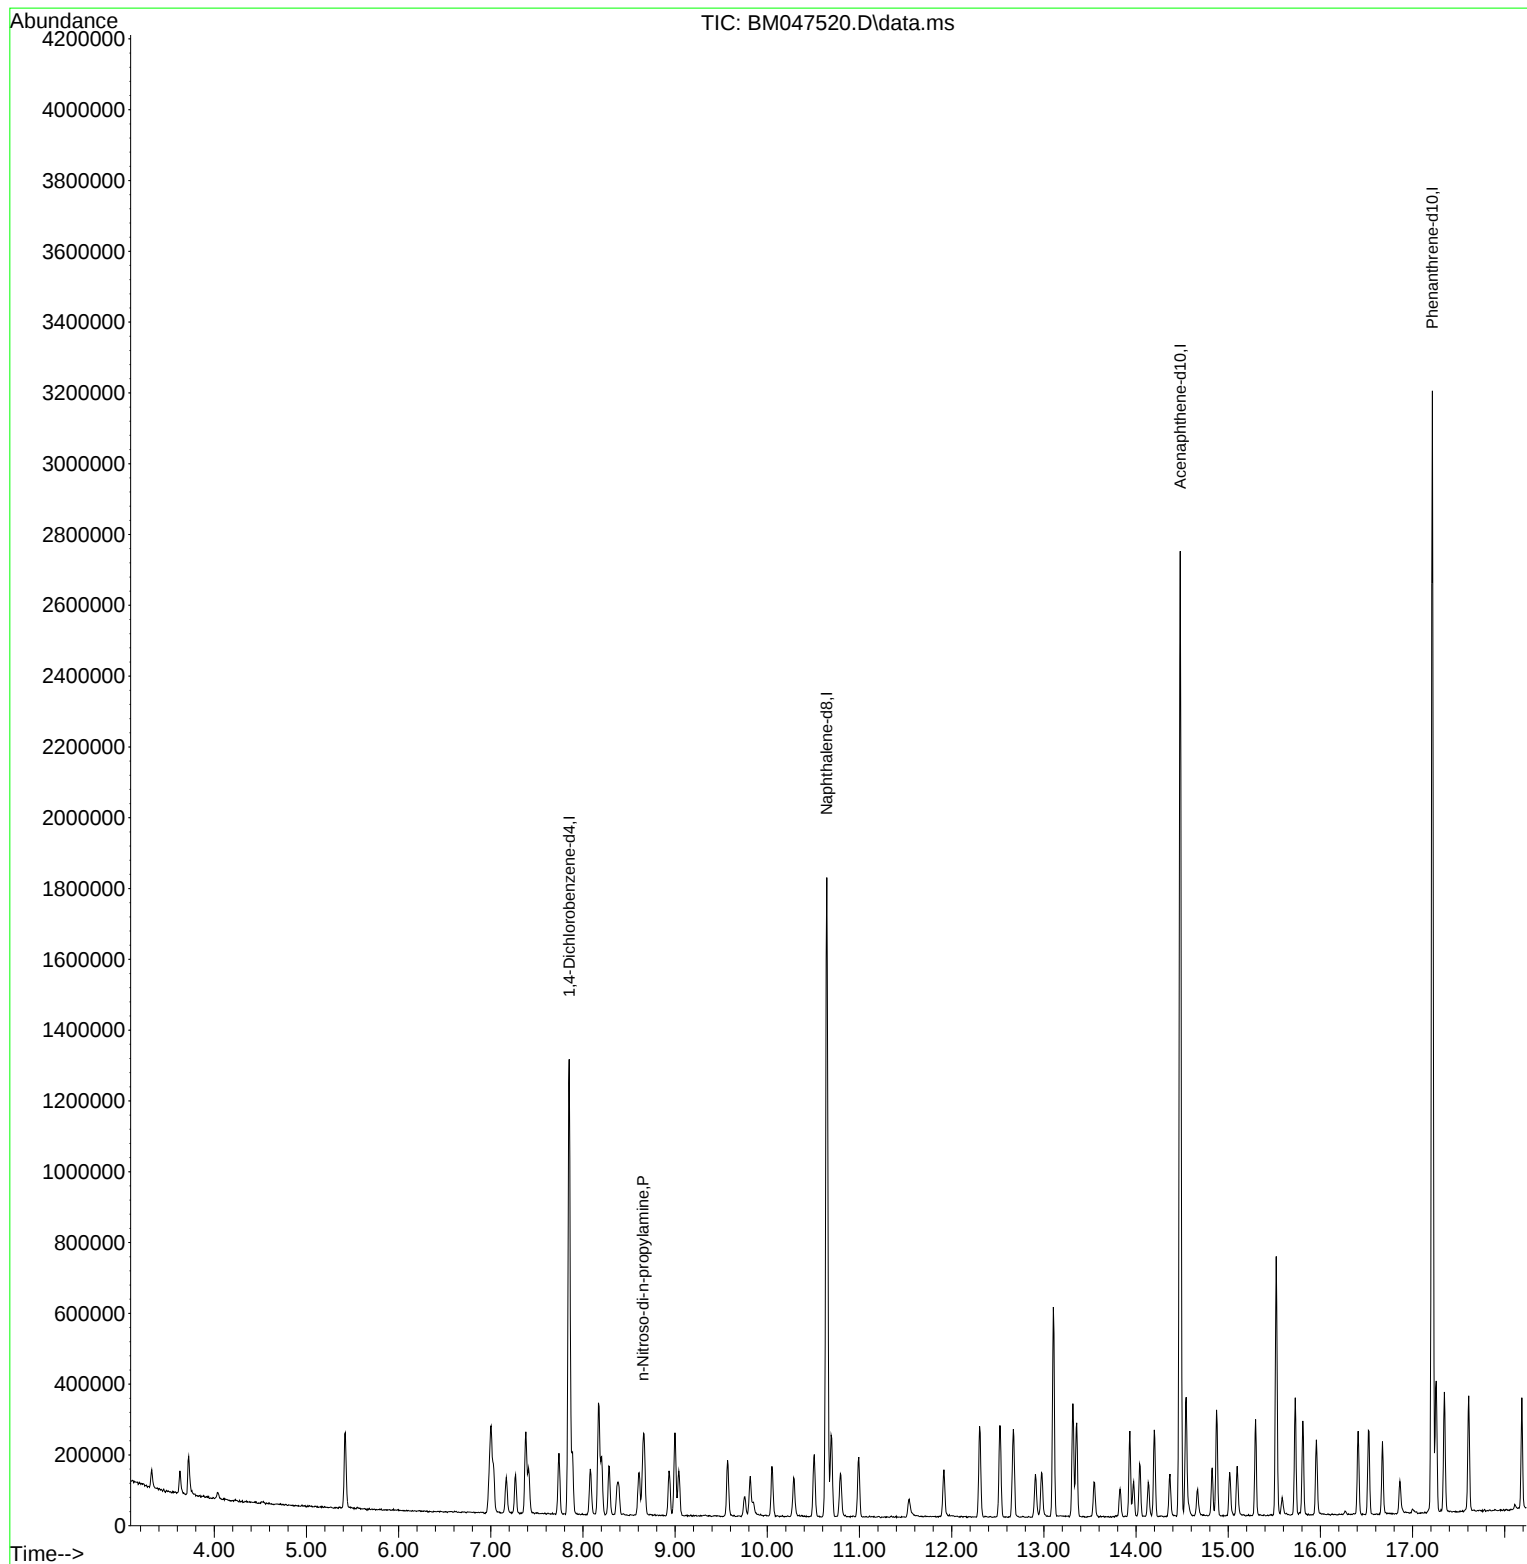

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091424\
Data File : BM047520.D
Acq On : 14 Sep 2024 11:57
Operator : RC/JU
Sample : SSTDICC2.5
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTDICC2.5

Quant Time: Sep 15 08:16:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 08:15:39 2024
Response via : Initial Calibration

