

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091424\
 Data File : BM047524.D
 Acq On : 14 Sep 2024 14:35
 Operator : RC/JU
 Sample : SSTDICCC040
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICCC040

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/16/2024
 Supervised By :mohammad ahmed 09/17/2024

Quant Time: Sep 15 08:48:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 08:43:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	365126	20.000	ng	0.00
21) Naphthalene-d8	10.645	136	1618219	20.000	ng	0.00
39) Acenaphthene-d10	14.480	164	947755	20.000	ng	0.00
64) Phenanthrene-d10	17.215	188	1792326	20.000	ng	0.00
76) Chrysene-d12	21.444	240	1627798	20.000	ng	0.00
86) Perylene-d12	24.468	264	1308860	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.422	112	1816554	79.215	ng	0.00
7) Phenol-d6	7.010	99	2621910	81.187	ng	0.00
23) Nitrobenzene-d5	9.004	82	2627381	81.256	ng	0.00
42) 2,4,6-Tribromophenol	15.962	330	767403	83.770	ng	0.00
45) 2-Fluorobiphenyl	13.110	172	5743669	83.482	ng	0.00
79) Terphenyl-d14	19.833	244	8178683	90.034	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.322	88	379485	38.636	ng	100
3) Pyridine	3.716	79	1158883m	39.648	ng	
4) n-Nitrosodimethylamine	3.628	42	533341	40.206	ng	100
6) Aniline	7.175	93	1158194	40.452	ng	100
8) 2-Chlorophenol	7.416	128	1018620	40.294	ng	100
9) Benzaldehyde	6.987	77	610922	39.784	ng	100
10) Phenol	7.034	94	1300688	40.224	ng	100
11) bis(2-Chloroethyl)ether	7.275	93	1035289	39.880	ng	100
12) 1,3-Dichlorobenzene	7.739	146	1097467	39.662	ng	100
13) 1,4-Dichlorobenzene	7.886	146	1115218	39.570	ng	100
14) 1,2-Dichlorobenzene	8.204	146	1100793	39.688	ng	100
15) Benzyl Alcohol	8.086	79	899897	41.137	ng	100
16) 2,2'-oxybis(1-Chloropr...	8.381	45	1467240	40.178	ng	100
17) 2-Methylphenol	8.286	107	847590	41.031	ng	100
18) Hexachloroethane	8.939	117	448954	39.876	ng	100
19) n-Nitroso-di-n-propyla...	8.657	70	908407	41.720	ng	100
20) 3+4-Methylphenols	8.616	107	1177936	40.867	ng	100
22) Acetophenone	8.669	105	1704805	40.072	ng	100
24) Nitrobenzene	9.045	77	1336633	40.229	ng	100
25) Isophorone	9.575	82	2301793	40.492	ng	100
26) 2-Nitrophenol	9.757	139	475675	42.013	ng	100
27) 2,4-Dimethylphenol	9.816	122	678795	39.549	ng	100
28) bis(2-Chloroethoxy)met...	10.057	93	1425885	39.933	ng	100
29) 2,4-Dichlorophenol	10.292	162	890582	40.842	ng	100
30) 1,2,4-Trichlorobenzene	10.510	180	978634	39.180	ng	100
31) Naphthalene	10.698	128	3484796	39.874	ng	100
32) Benzoic acid	9.951	122	621554	38.270	ng	100
33) 4-Chloroaniline	10.798	127	1271819	40.249	ng	100
34) Hexachlorobutadiene	10.992	225	548156	39.622	ng	100
35) Caprolactam	11.574	113	301774	42.014	ng	100
36) 4-Chloro-3-methylphenol	11.922	107	1029746	41.207	ng	100
37) 2-Methylnaphthalene	12.310	142	2350065	40.402	ng	100
38) 1-Methylnaphthalene	12.527	142	2315698	40.060	ng	100
40) 1,2,4,5-Tetrachloroben...	12.674	216	1037544	40.457	ng	100
41) Hexachlorocyclopentadiene	12.663	237	346149	41.288	ng	100
43) 2,4,6-Trichlorophenol	12.910	196	663467	41.294	ng	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091424\
 Data File : BM047524.D
 Acq On : 14 Sep 2024 14:35
 Operator : RC/JU
 Sample : SSTDICCC040
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICCC040

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/16/2024
 Supervised By :mohammad ahmed 09/17/2024

Quant Time: Sep 15 08:48:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 08:43:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 2,4,5-Trichlorophenol	12.980	196	749195	41.284	ng	100
46) 1,1'-Biphenyl	13.316	154	2977591	40.379	ng	100
47) 2-Chloronaphthalene	13.357	162	2309174	40.329	ng	100
48) 2-Nitroaniline	13.551	65	711905	42.331	ng	100
49) Acenaphthylene	14.204	152	3389381	41.020	ng	100
50) Dimethylphthalate	13.939	163	2601271	40.269	ng	100
51) 2,6-Dinitrotoluene	14.051	165	562396	41.241	ng	100
52) Acenaphthene	14.545	154	2363816	40.830	ng	100
53) 3-Nitroaniline	14.374	138	636300	41.980	ng	100
54) 2,4-Dinitrophenol	14.574	184	242408	40.526	ng	100
55) Dibenzofuran	14.880	168	3286806	40.401	ng	100
56) 4-Nitrophenol	14.674	139	533596	42.781	ng	100
57) 2,4-Dinitrotoluene	14.833	165	772430	42.471	ng	100
58) Fluorene	15.527	166	3089638	42.182	ng	100
59) 2,3,4,6-Tetrachlorophenol	15.104	232	580263	41.011	ng	100
60) Diethylphthalate	15.304	149	2809721	40.869	ng	100
61) 4-Chlorophenyl-phenyle...	15.521	204	1409661	42.091	ng	100
62) 4-Nitroaniline	15.533	138	795712	44.661	ng	100
63) Azobenzene	15.815	77	3134877	41.412	ng	100
65) 4,6-Dinitro-2-methylph...	15.592	198	327400	37.677	ng	100
66) n-Nitrosodiphenylamine	15.733	169	2266693	41.340	ng	100
67) 4-Bromophenyl-phenylether	16.409	248	705864	40.531	ng	100
68) Hexachlorobenzene	16.527	284	796111	40.352	ng	100
69) Atrazine	16.680	200	638553	42.135	ng	100
70) Pentachlorophenol	16.862	266	486319	42.523	ng	100
71) Phenanthrene	17.256	178	4065837	41.163	ng	100
72) Anthracene	17.351	178	3956786	41.695	ng	100
73) Carbazole	17.609	167	3906452	41.537	ng	100
74) Di-n-butylphthalate	18.186	149	4803649	42.689	ng	100
75) Fluoranthene	19.268	202	4593392	42.622	ng	100
77) Benzidine	19.445	184	825167	35.993	ng	100
78) Pyrene	19.627	202	4862723	40.954	ng	100
80) Butylbenzylphthalate	20.527	149	1915535	41.908	ng	100
81) Benzo(a)anthracene	21.421	228	4338226	40.888	ng	100
82) 3,3'-Dichlorobenzidine	21.344	252	1177624	41.724	ng	100
83) Chrysene	21.486	228	4082724	40.682	ng	100
84) Bis(2-ethylhexyl)phtha...	21.362	149	3022758	42.216	ng	100
85) Di-n-octyl phthalate	22.509	149	4236094	41.825	ng	100
87) Indeno(1,2,3-cd)pyrene	27.897	276	3099824	39.575	ng	100
88) Benzo(b)fluoranthene	23.515	252	3507877	41.423	ng	100
89) Benzo(k)fluoranthene	23.580	252	3570213	42.538	ng	100
90) Benzo(a)pyrene	24.332	252	2875521	41.429	ng	100
91) Dibenzo(a,h)anthracene	27.956	278	2601274	39.472	ng	100
92) Benzo(g,h,i)perylene	28.967	276	2535092	39.380	ng	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091424\
Data File : BM047524.D
Acq On : 14 Sep 2024 14:35
Operator : RC/JU
Sample : SSTDICCC040
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :

BNA_M

ClientSampleId :

SSTDICCC040

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 09/16/2024

Supervised By :mohammad ahmed 09/17/2024


Quant Time: Sep 15 08:48:03 2024

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091424.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sun Sep 15 08:43:20 2024

Response via : Initial Calibration

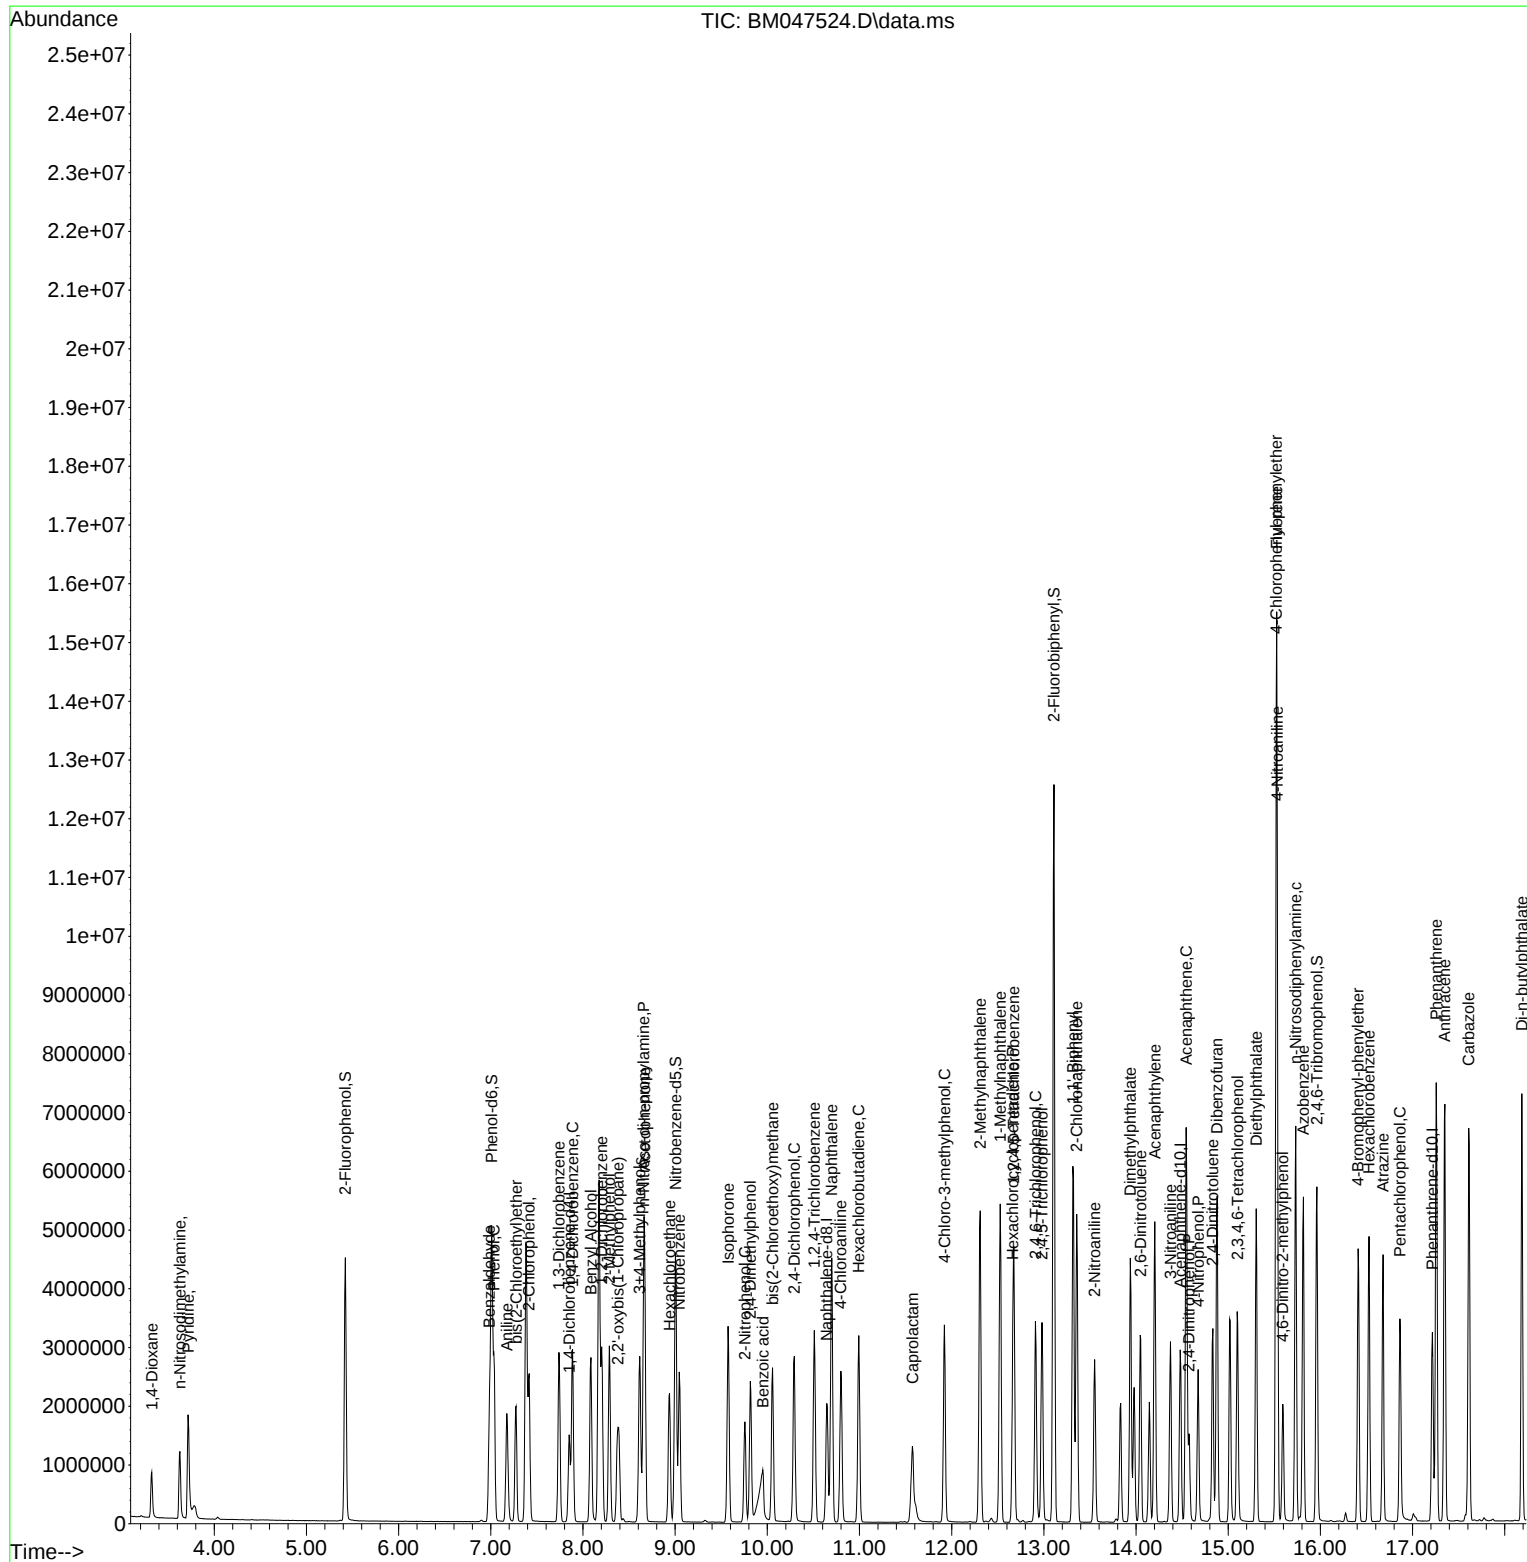

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091424\
Data File : BM047524.D
Acq On : 14 Sep 2024 14:35
Operator : RC/JU
Sample : SSTDICCC040
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTDICCC040

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/16/2024
Supervised By :mohammad ahmed 09/17/2024

Quant Time: Sep 15 08:48:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 08:43:20 2024
Response via : Initial Calibration

