
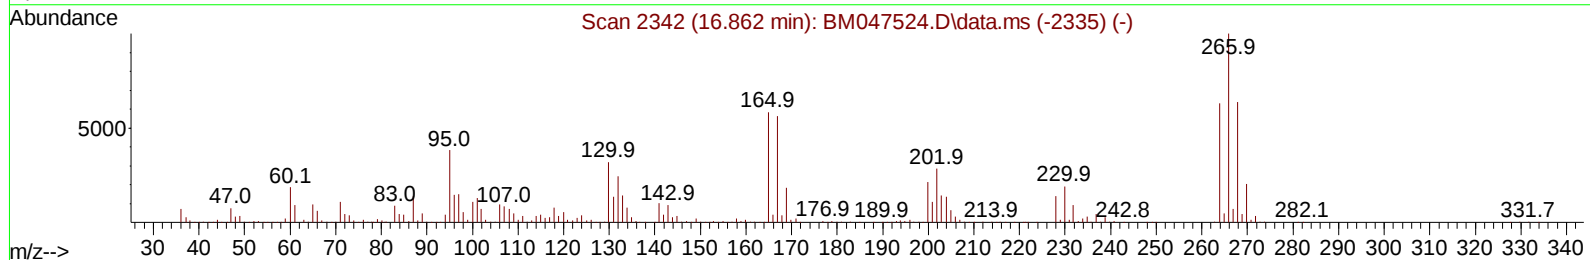
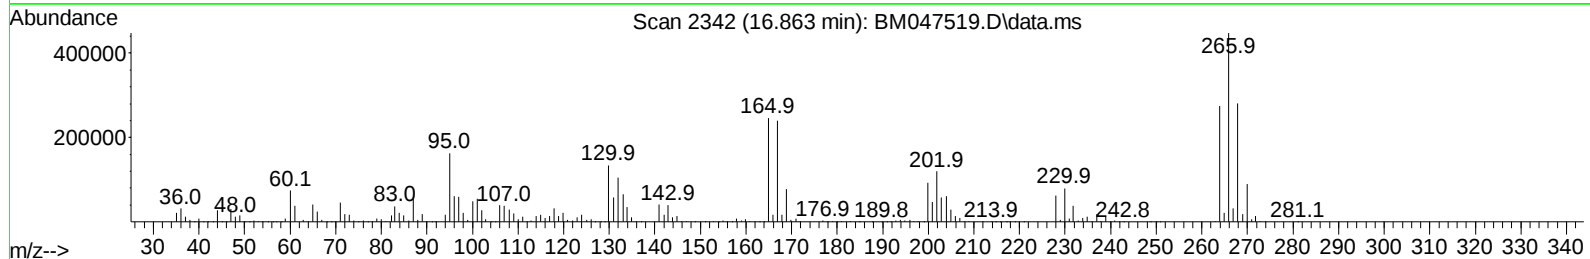


Quant Time: Sep 15 09:03:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 08:56:37 2024
Response via : Initial Calibration

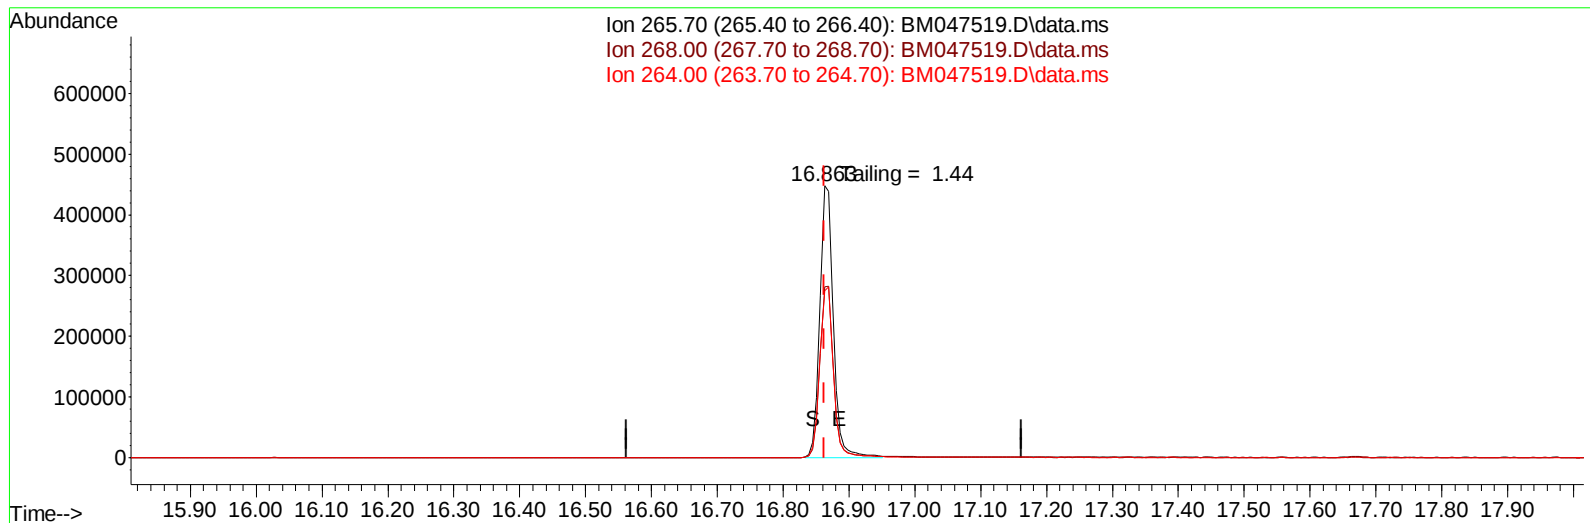

TIC: BM047519.D\data.ms

(70) Pentachlorophenol (C)




16.863min (+ 0.000) 149789.64 ng

response **629866**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.83
264.00	63.00	61.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091424\
Data File : BM047519.D
Acq On : 14 Sep 2024 11:17
Operator : RC/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 15 09:03:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 08:56:37 2024
Response via : Initial Calibration

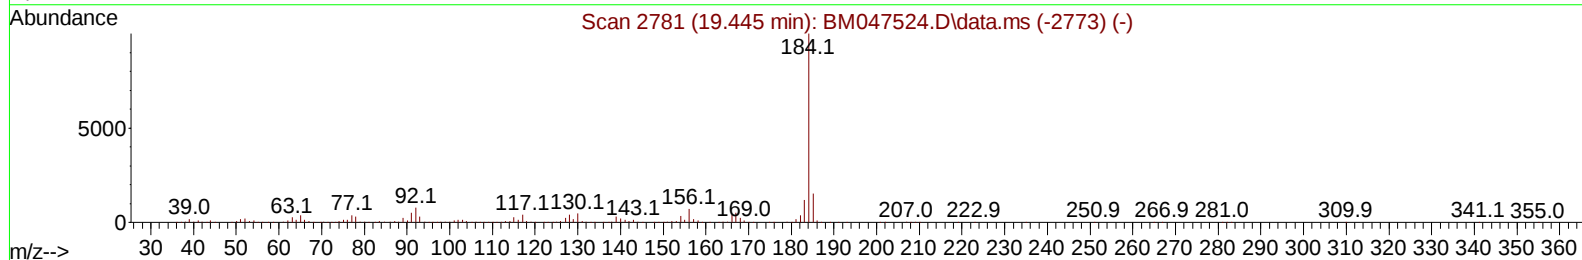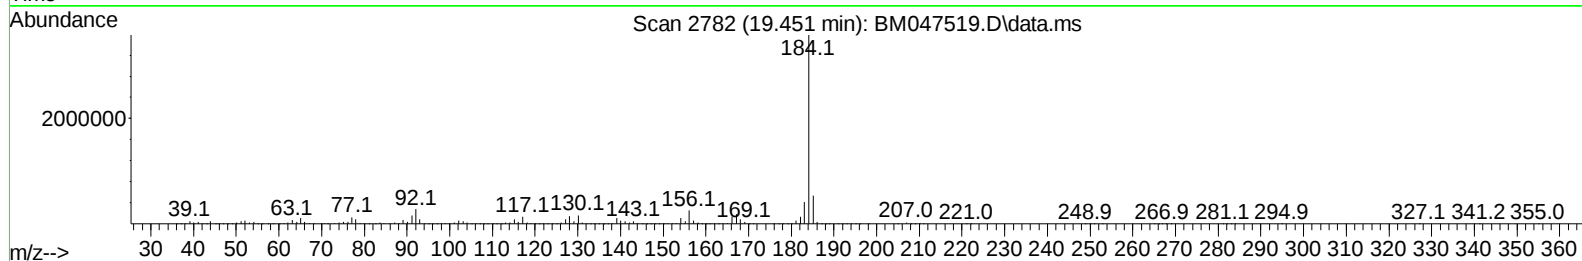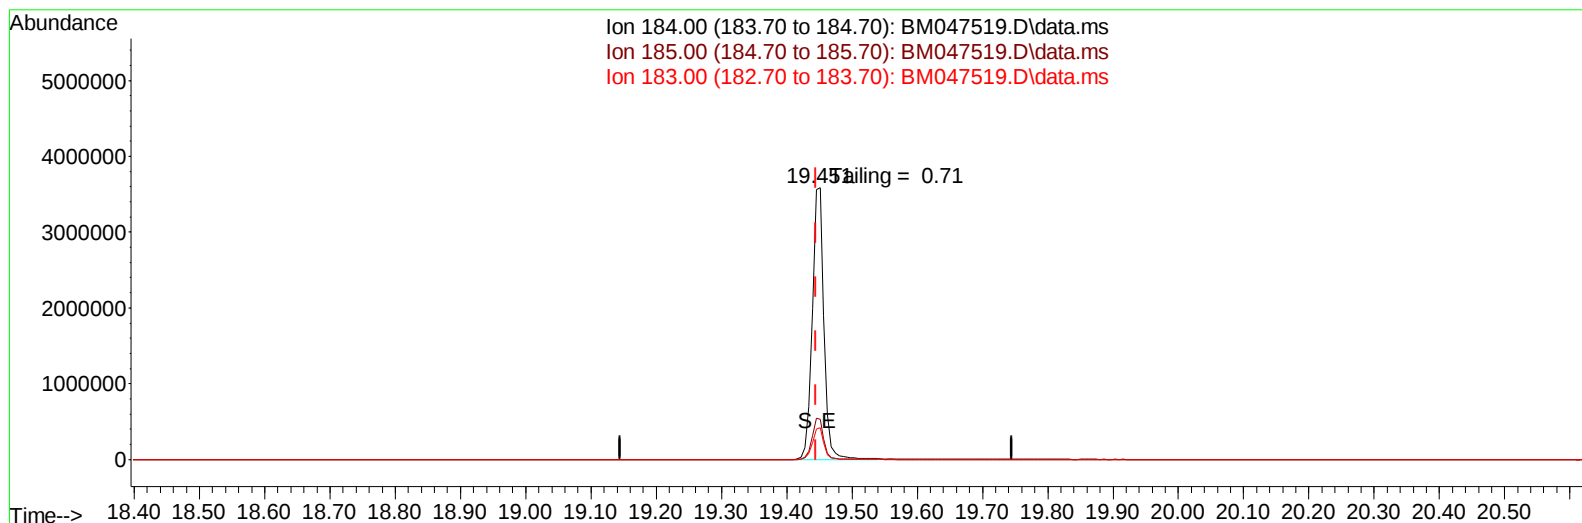

TIC: BM047519.D\data.ms

(77) Benzidine

19.451min (+ 0.006) 303907.69 ng

response 4609731

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.82
183.00	12.00	11.61
0.00	0.00	0.00