


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100521\
Data File : BM032332.D
Acq On : 05 Oct 2021 18:00
Operator : CG/JU
Sample : SSTD16051
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTD160002

Manual Integrations
APPROVED

mohammad
10/8/2021 8:33:35 AM

Quant Time: Oct 05 18:30:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 05 15:29:16 2021
Response via : Initial Calibration

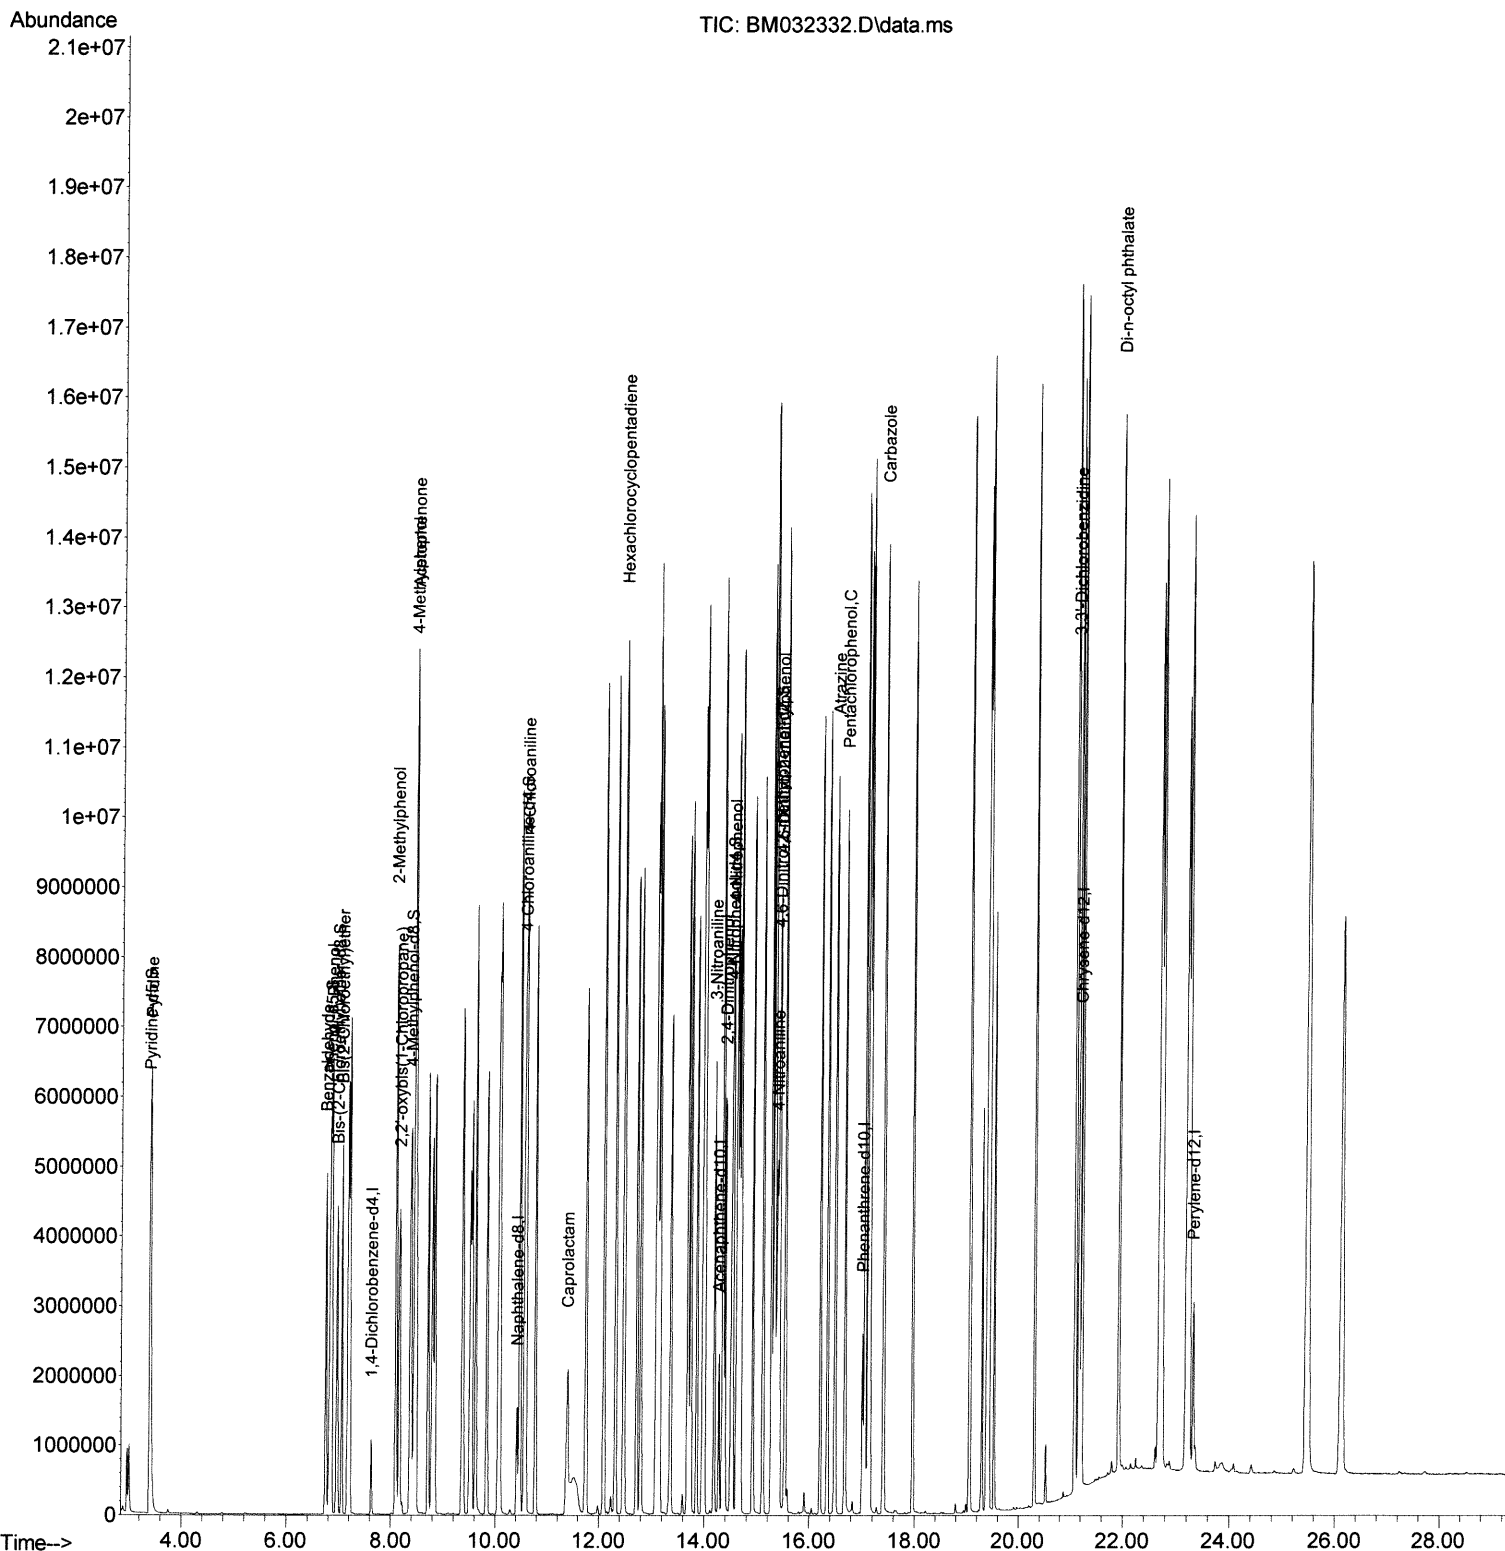



Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100521\
 Data File : BM032332.D
 Acq On : 05 Oct 2021 18:00
 Operator : CG/JU
 Sample : SSTD16051
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD160002

Manual Integrations
 APPROVED

mohammad
 10/8/2021 8:33:35 AM

Quant Time: Oct 05 18:30:22 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 05 15:29:16 2021
 Response via : Initial Calibration

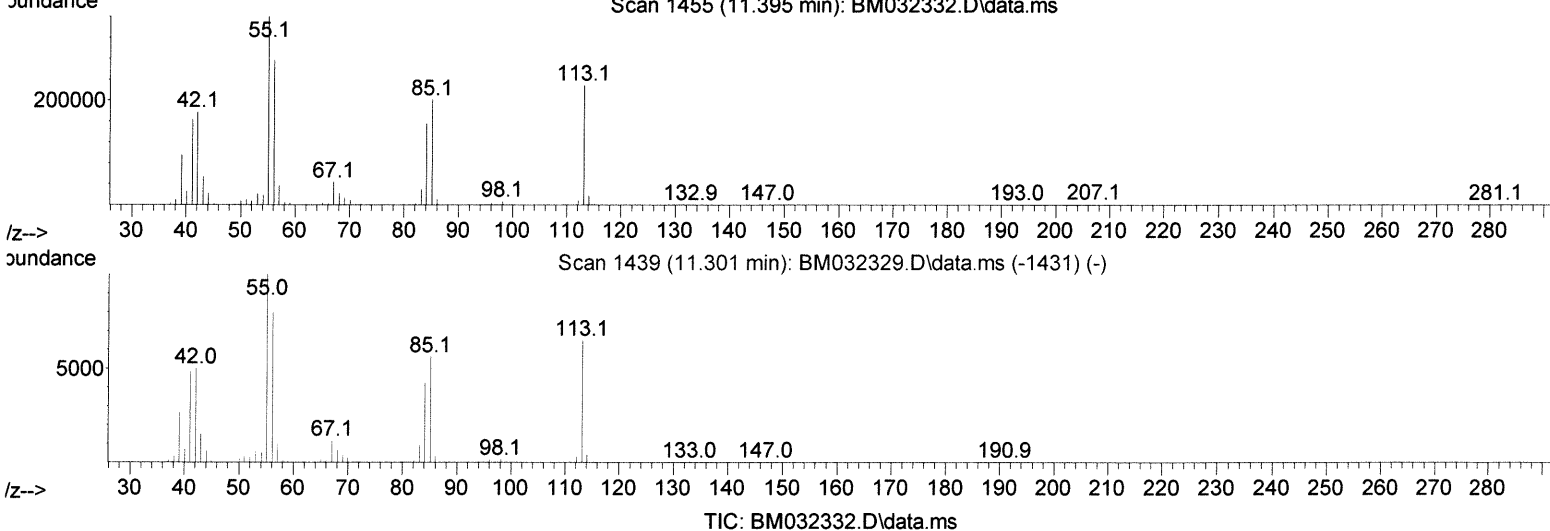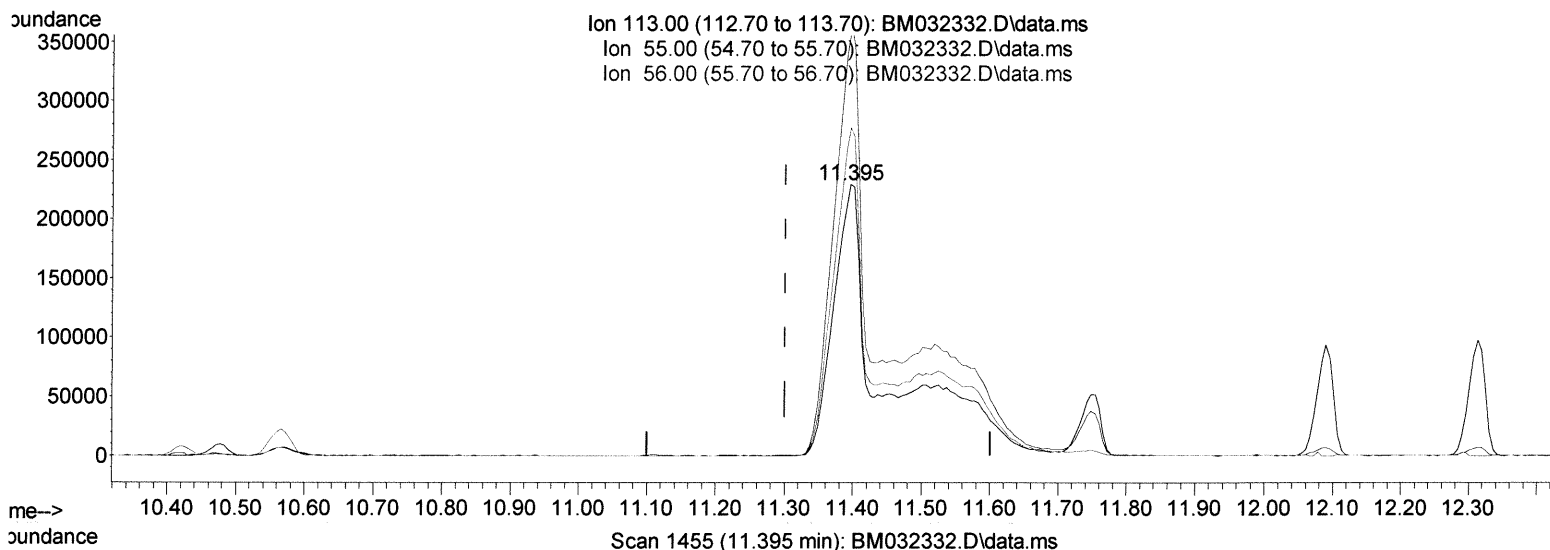

(34) Caprolactam

11.395min (+ 0.094) 99.05 ng/ul

response 648287

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	154.80	157.29
56.00	123.20	121.17
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100521\
 Data File : BM032332.D
 Acq On : 05 Oct 2021 18:00
 Operator : CG/JU
 Sample : SSTD16051
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD160002

Manual Integrations
 APPROVED

mohammad
 10/8/2021 8:33:35 AM

Quant Time: Oct 05 18:30:22 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 05 15:29:16 2021
 Response via : Initial Calibration

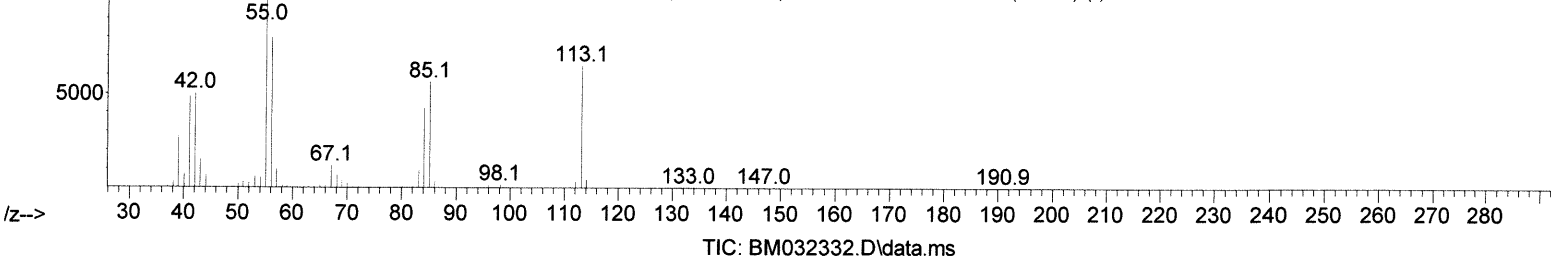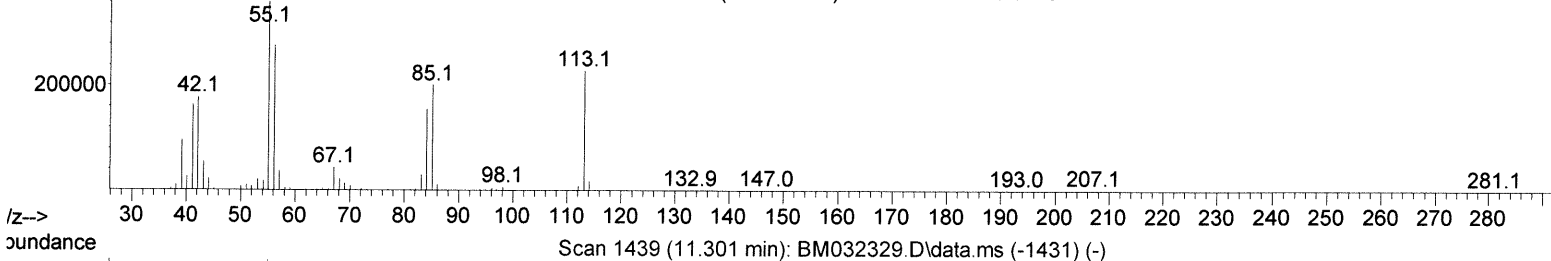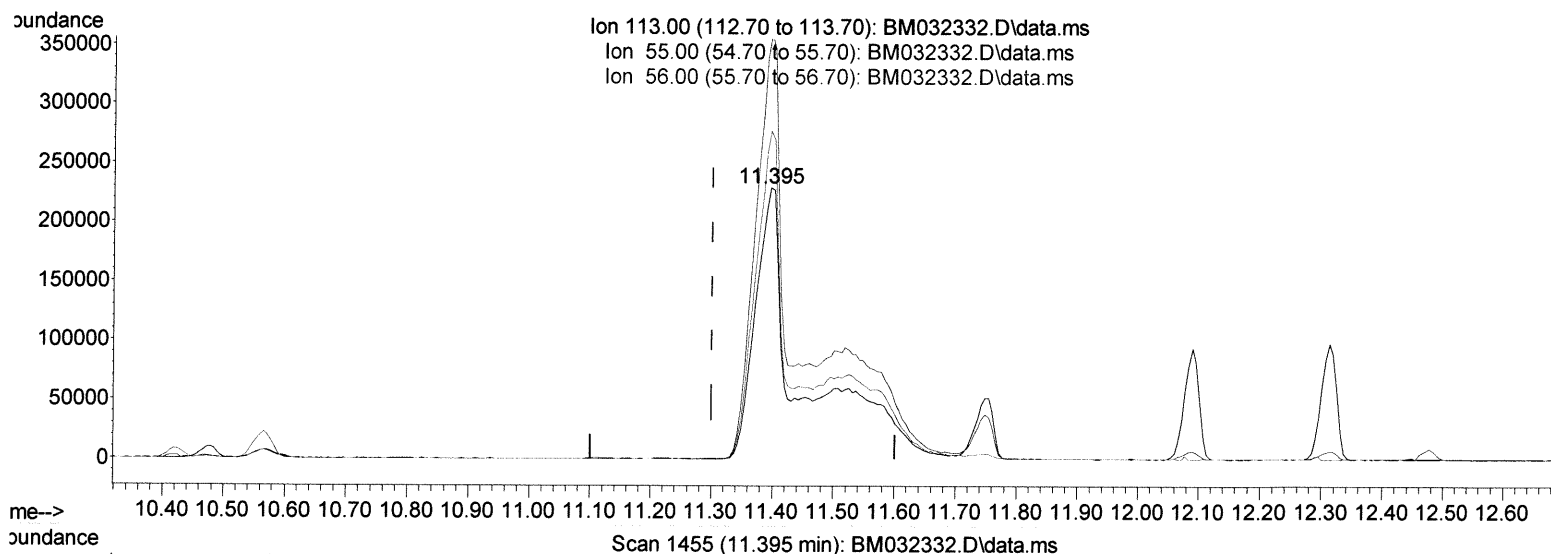

(34) Caprolactam

11.395min (+ 0.094) 187.09 ng/ul m

response 1224503

JR 10/12/21

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	154.80	157.29
56.00	123.20	121.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100521\
 Data File : BM032332.D
 Acq On : 05 Oct 2021 18:00
 Operator : CG/JU
 Sample : SSTD16051
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD160002

Manual Integrations
 APPROVED

mohammad
 10/8/2021 8:33:35 AM

Quant Time: Oct 05 18:30:22 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
 Quant Title : SVOA CALIBRATION
 Last Update : Tue Oct 05 15:29:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.625	152	280686	20.000	ng/ul	0.00
20) Naphthalene-d8	10.425	136	1230994	20.000	ng/ul	0.01
38) Acenaphthene-d10	14.277	164	790284	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.007	188	1620308	20.000	ng/ul	0.00
79) Chrysene-d12	21.177	240	1300180	20.000	ng/ul	0.01
88) Perylene-d12	23.318	264	1492175	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	3.384	84	3193240	161.460	ng/ul	0.00
7) Phenol-d5	6.831	99	4027855	168.979	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	6.966	67	2200082	160.026	ng/ul	0.02
11) 2-Chlorophenol-d4	0.000	132	0d	0.000	ng/ul	
15) 4-Methylphenol-d8	8.384	113	3277274	170.895	ng/ul	0.03
21) Nitrobenzene-d5	0.000	128	0d	0.000	ng/ul	
24) 2-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
28) 2,4-Dichlorophenol-d3	0.000	165	0d	0.000	ng/ul	
31) 4-Chloroaniline-d4	10.566	131	4305961	155.278	ng/ul	0.02
46) Dimethylphthalate-d6	0.000	166	0d	0.000	ng/ul	
49) Acenaphthylene-d8	0.000	160	0d	0.000	ng/ul	
54) 4-Nitrophenol-d4	14.518	143	1830778	170.276	ng/ul	0.04
60) Fluorene-d10	0.000	176	0d	0.000	ng/ul	
65) 4,6-Dinitro-2-methylph...	15.407	200	1652118	179.964	ng/ul	0.03
73) Anthracene-d10	0.000	188	0d	0.000	ng/ul	
81) Pyrene-d10	0.000	212	0d	0.000	ng/ul	
92) Benzo(a)pyrene-d12	0.000	264	0d	0.000	ng/ul	
Target Compounds						
					Qvalue	
5) Pyridine	3.407	79	3150192	160.715	ng/ul	97
6) Benzaldehyde	6.754	77	1762319	207.155	ng/ul	98
8) Phenol	6.866	94	3953344	163.378	ng/ul	99
10) Bis(2-Chloroethyl)ether	7.060	93	2995935	157.328	ng/ul	100
13) 2-Methylphenol	8.101	108	3054721	164.952	ng/ul	100
14) 2,2'-oxybis(1-Chloropr...	8.172	45	3727935	156.772	ng/ul	98
16) Acetophenone	8.460	105	3995029	140.927	ng/ul#	79
18) 4-Methylphenol	8.454	108	2875364	147.673	ng/ul	99
32) 4-Chloroaniline	10.595	127	4156944	149.442	ng/ul	97
34) Caprolactam	11.395	113	1224503m	187.086	ng/ul	97 10/12/21
40) Hexachlorocyclopentadiene	12.466	237	1956703	152.725	ng/ul	99
51) 3-Nitroaniline	14.195	138	1889201	177.195	ng/ul	97
53) 2,4-Dinitrophenol	14.395	184	1368500	213.001	ng/ul	96
55) 4-Nitrophenol	14.536	109	1441499	166.332	ng/ul	95
63) 4-Nitroaniline	15.377	138	1654946	165.669	ng/ul	97
66) 4,6-Dinitro-2-methylph...	15.424	198	1579379	174.799	ng/ul#	99
70) Atrazine	16.495	200	2604973	150.746	ng/ul	99
71) Pentachlorophenol	16.677	266	1831274	168.938	ng/ul	98
77) Carbazole	17.412	167	10103753	132.318	ng/ul	95
84) 3,3'-Dichlorobenzidine	21.095	252	2850415	122.819	ng/ul	98
89) Di-n-octyl phthalate	21.924	149	11958006	140.335	ng/ul	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM100521\
Data File : BM032332.D
Acq On : 05 Oct 2021 18:00
Operator : CG/JU
Sample : SSTD16051
Misc :
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Oct 05 18:30:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM100521.M
Quant Title : SVOA CALIBRATION
Last Update : Tue Oct 05 15:29:16 2021
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
SSTD160002

Manual Integrations
APPROVED

mohammad
10/8/2021 8:33:35 AM

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

(#) = qualifier out of range (m) = manual integration (+) = signals summed						