
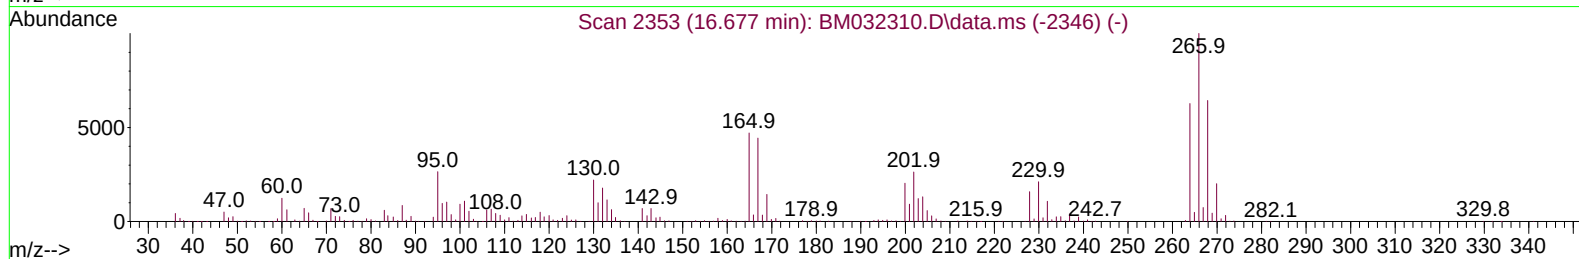
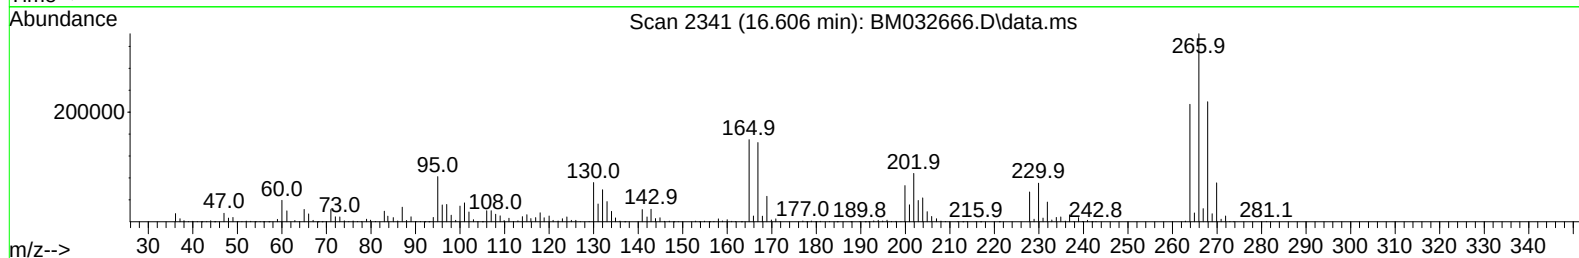


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102221\
 Data File : BM032666.D
 Acq On : 22 Oct 2021 08:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 22 11:23:14 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 22 11:23:10 2021
 Response via : Initial Calibration

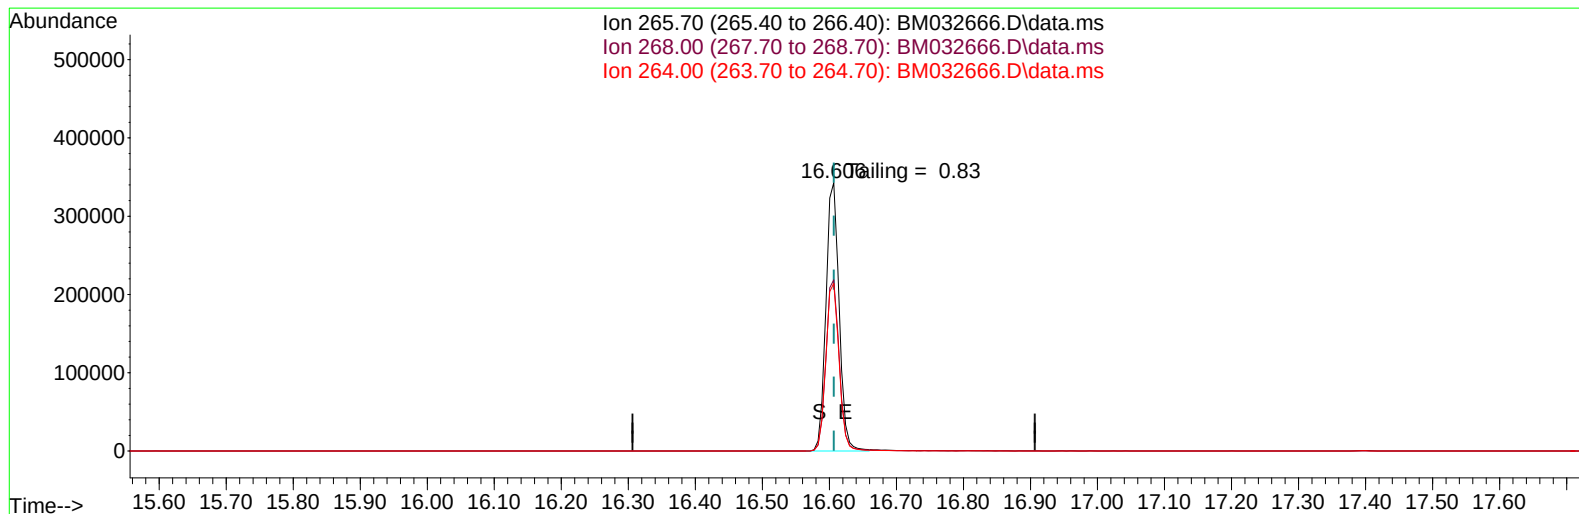

TIC: BM032666.D\data.ms

(70) Pentachlorophenol (C)




16.606min (0.000) 280555.17 ng

response 472174

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	63.83
264.00	65.10	62.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102221\
Data File : BM032666.D
Acq On : 22 Oct 2021 08:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 22 11:23:14 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 22 11:23:10 2021
Response via : Initial Calibration

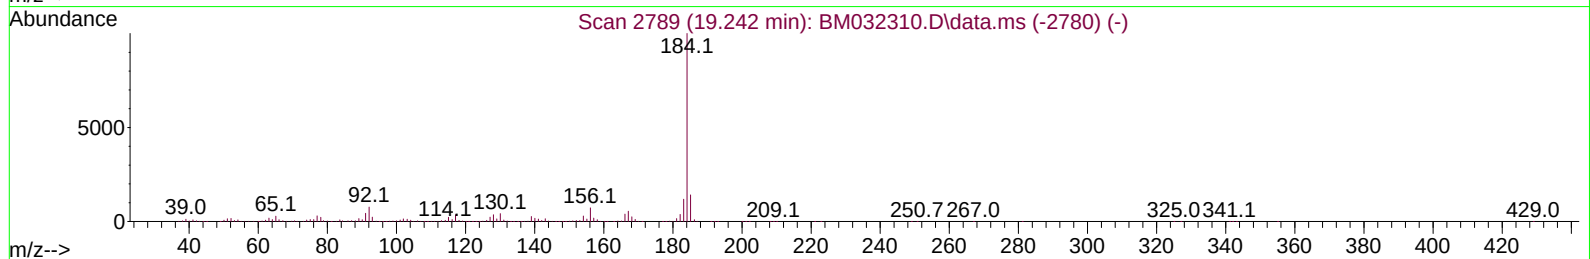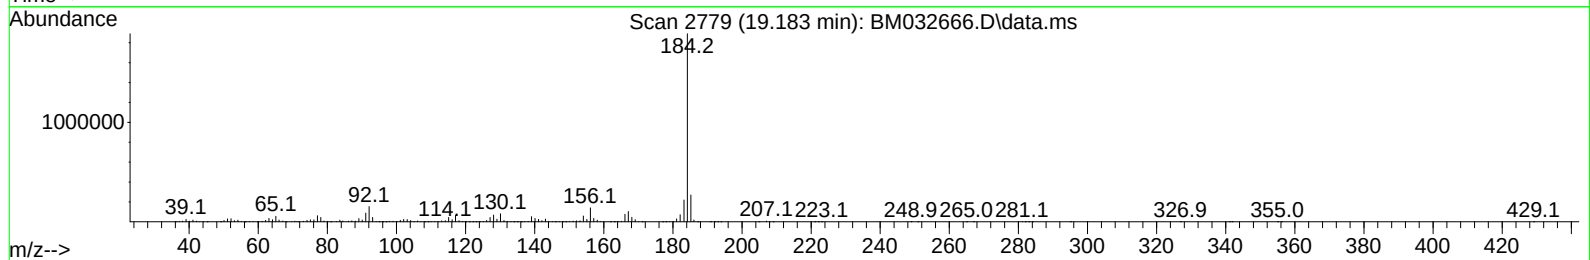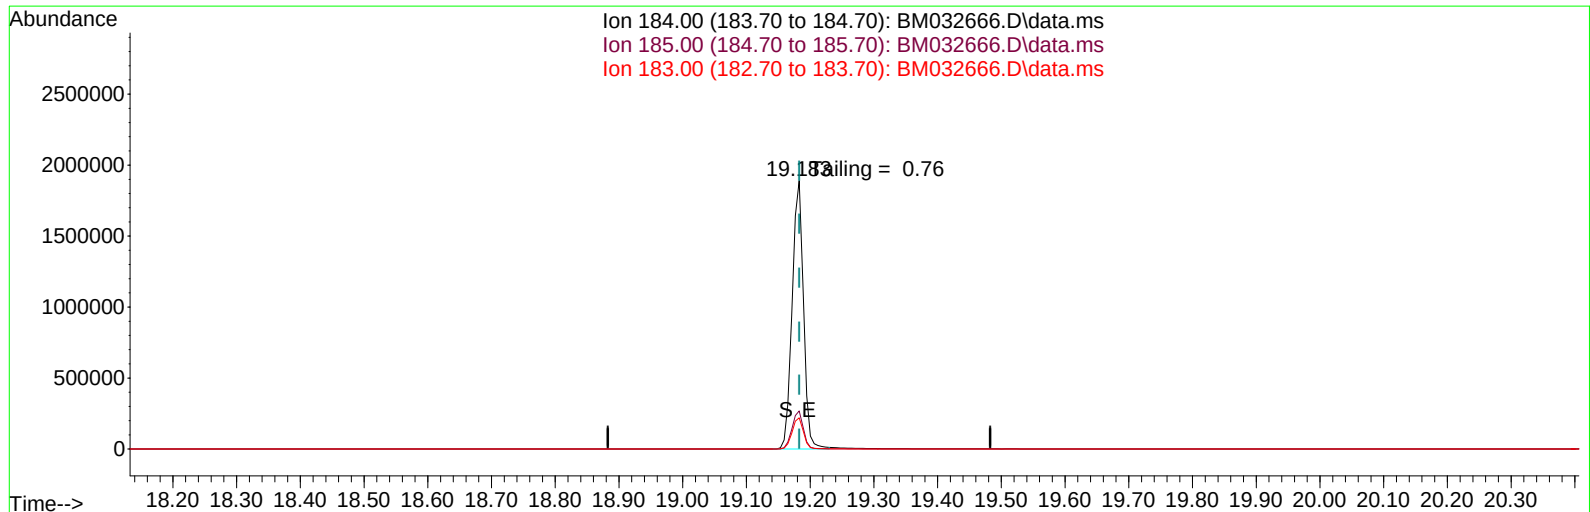

TIC: BM032666.D\data.ms

(77) Benzidine**19.183min (0.000) 102166.35 ng****response 2370416**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	14.21
183.00	11.20	11.62
0.00	0.00	0.00