
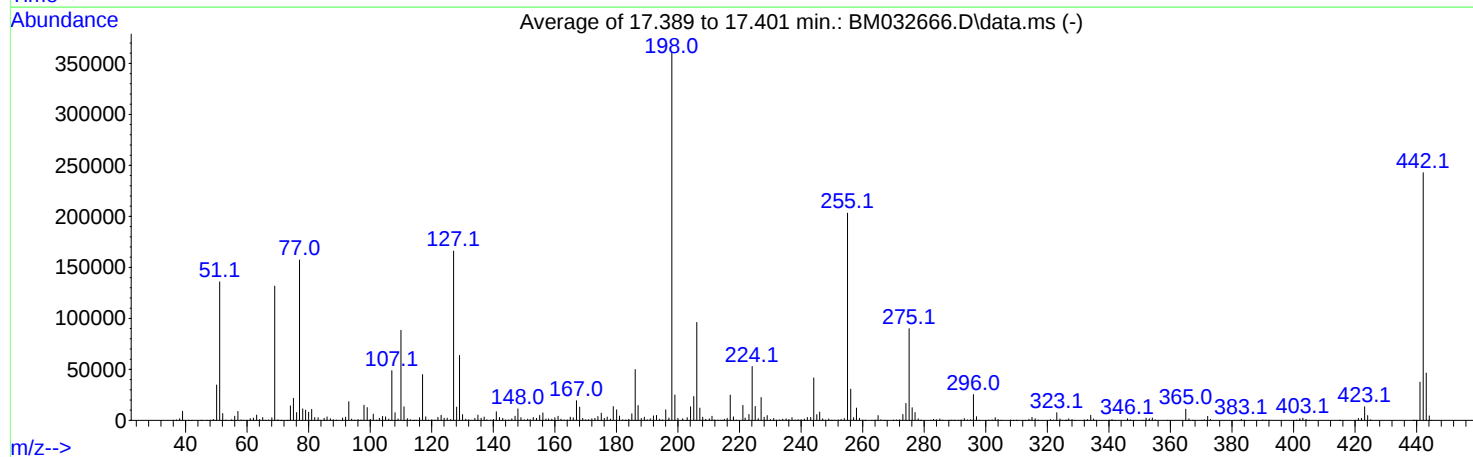


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102221\
 Data File : BM032666.D
 Acq On : 22 Oct 2021 08:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Oct 23 01:22:28 2021

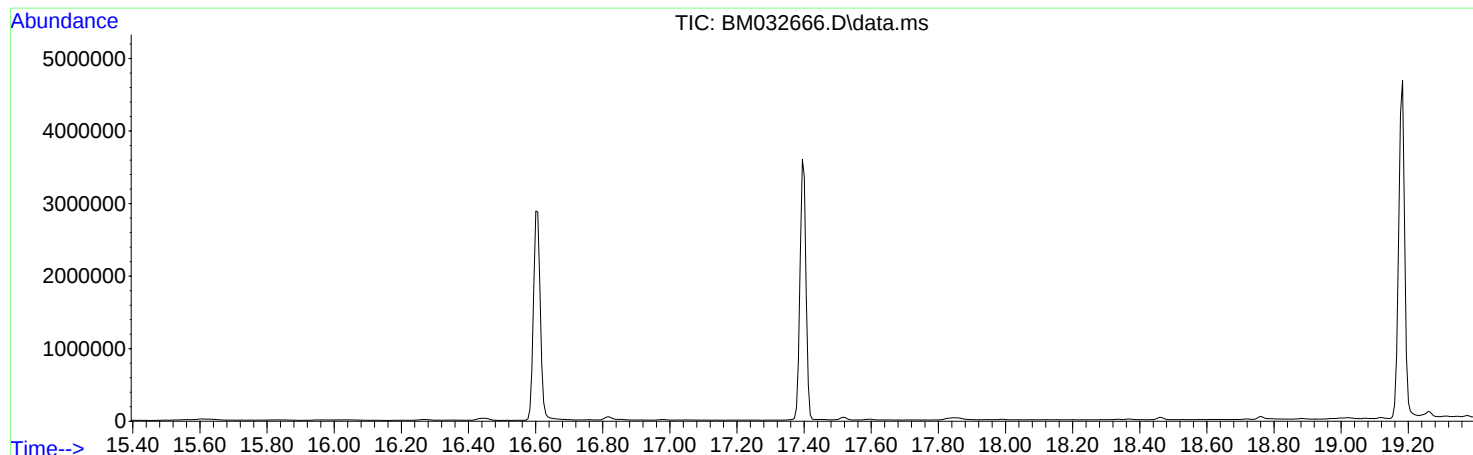




AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	135824	PASS
68	69	0.00	2	1.9	2509	PASS
69	198	0.00	100	36.5	131663	PASS
70	69	0.00	2	0.5	683	PASS
127	198	10	80	46.0	166016	PASS
197	198	0.00	2	0.6	2326	PASS
198	198	100	100	100.0	360683	PASS
199	198	5	9	6.9	24955	PASS
275	198	10	60	24.9	89957	PASS
365	198	1	100	3.0	10995	PASS
441	198	0.01	100	10.4	37464	PASS
442	442	50	100	100.0	242925	PASS
443	442	15	24	19.1	46411	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102221\
 Data File : BM032666.D
 Acq On : 22 Oct 2021 08:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Oct 22 11:23:14 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 22 11:23:10 2021
 Response via : Initial Calibration

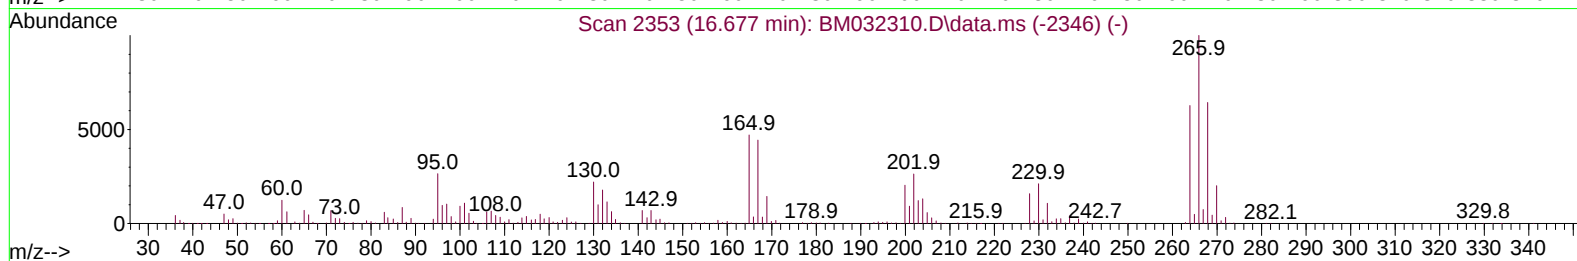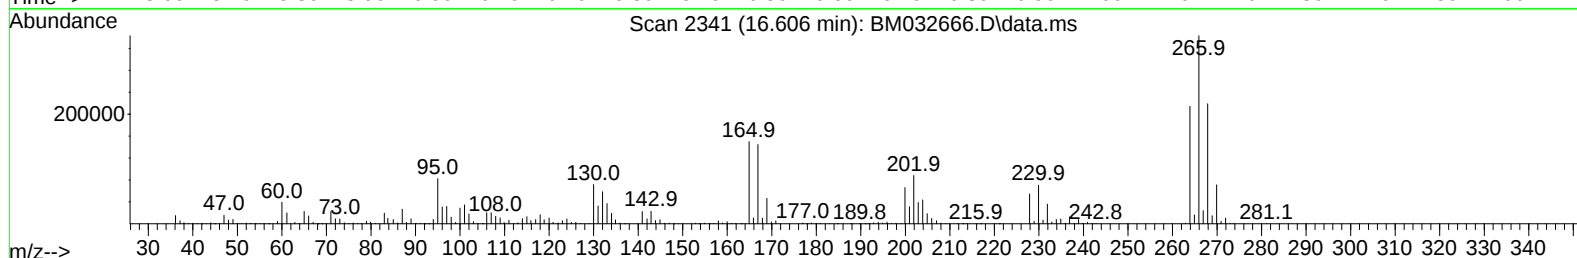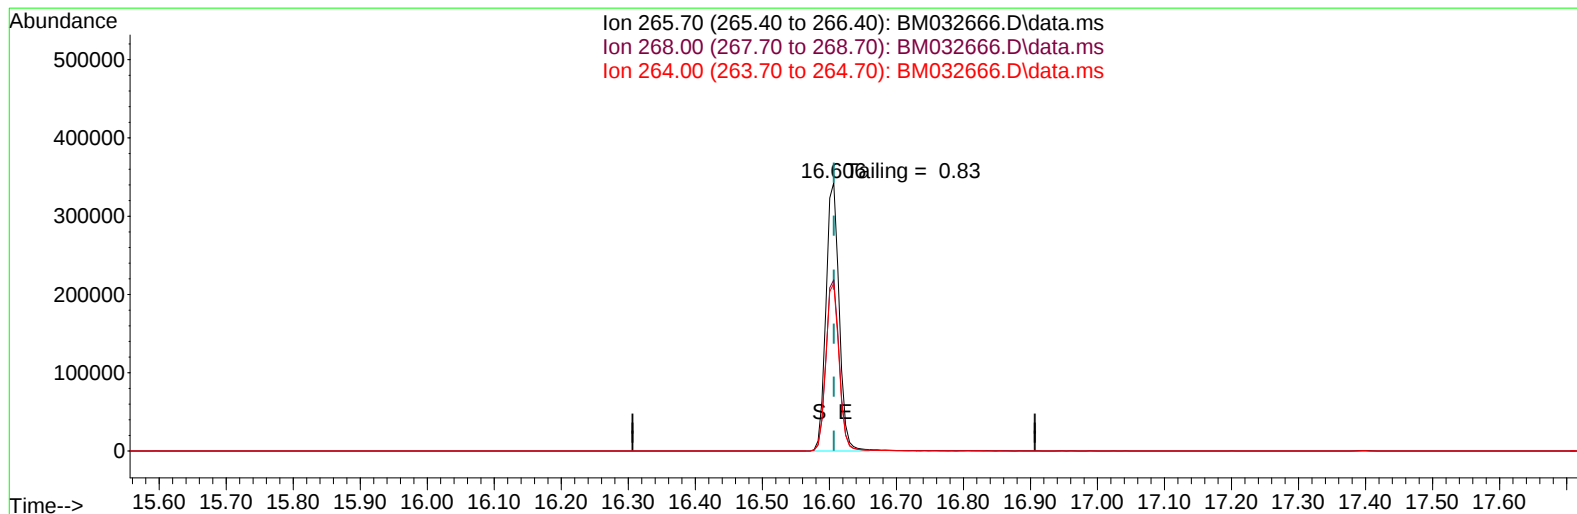

TIC: BM032666.D\data.ms

(70) Pentachlorophenol (C)

16.606min (0.000) 280555.17 ng




response 472174

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	63.83
264.00	65.10	62.47
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102221\  
Data File : BM032666.D  
Acq On    : 22 Oct 2021  08:52  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 22 11:23:14 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 22 11:23:10 2021
Response via : Initial Calibration

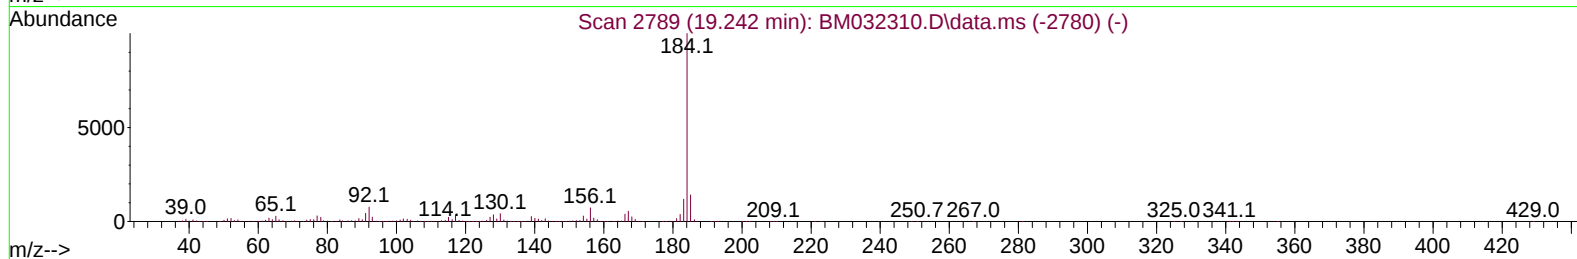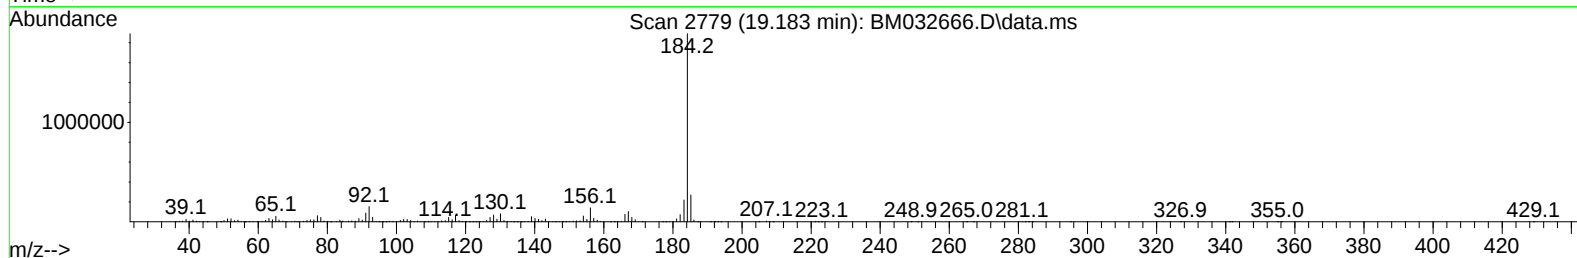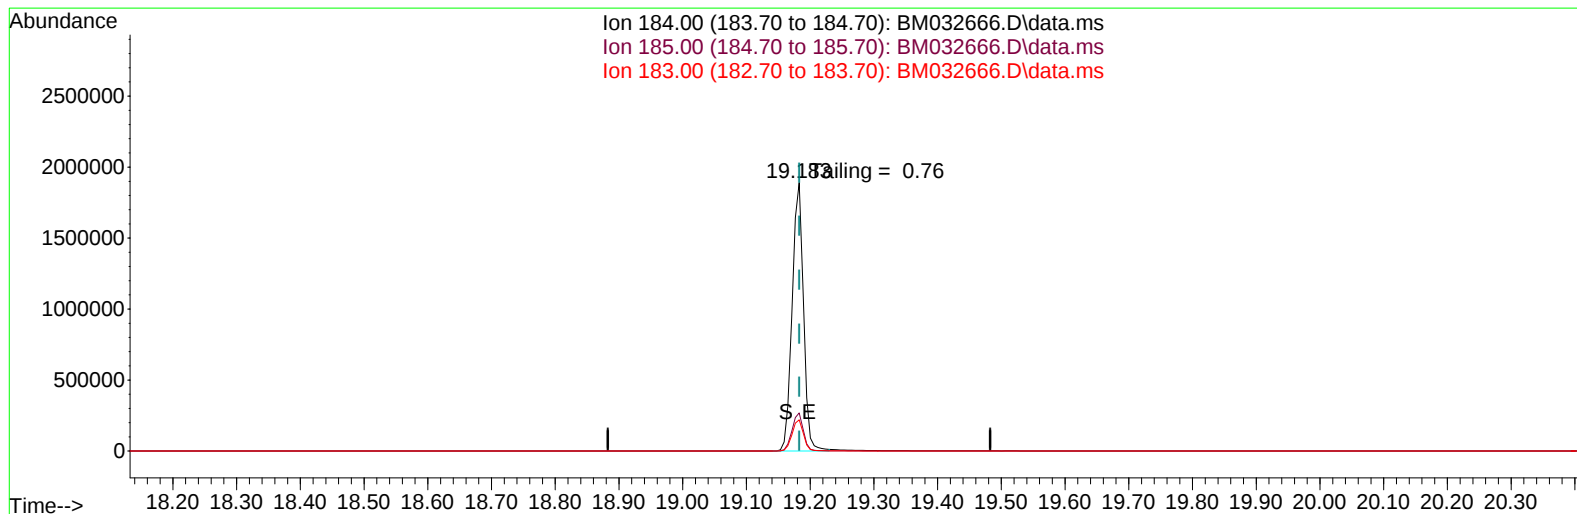

TIC: BM032666.D\data.ms

(77) Benzidine

19.183min (0.000) 102166.35 ng

response **2370416**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	14.21
183.00	11.20	11.62
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/22/2021	BNA_M	<u>BM032666.D</u>
Compound Name	Response	Retention Time
DDT	1159903	20.41
DDD	105423	19.98
DDE	3827	19.47
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
109250	1269153	8.61

Instrument :
BNA_M
ClientSampleId :
DFTPP