
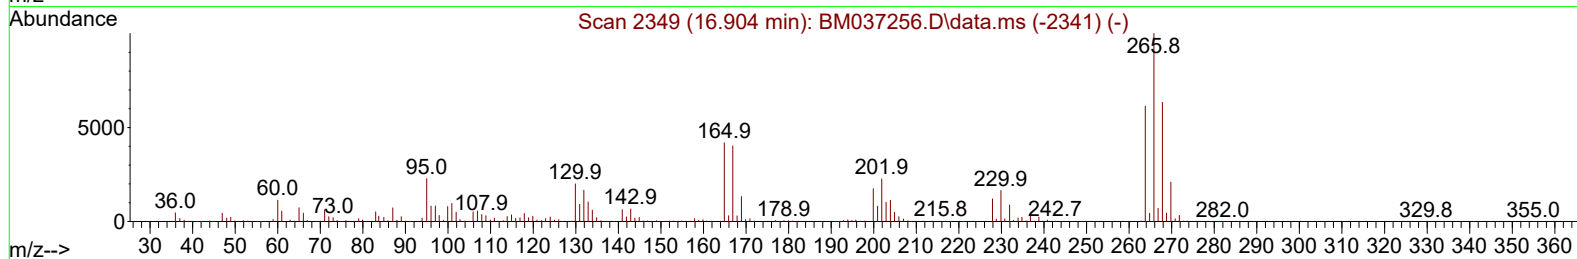
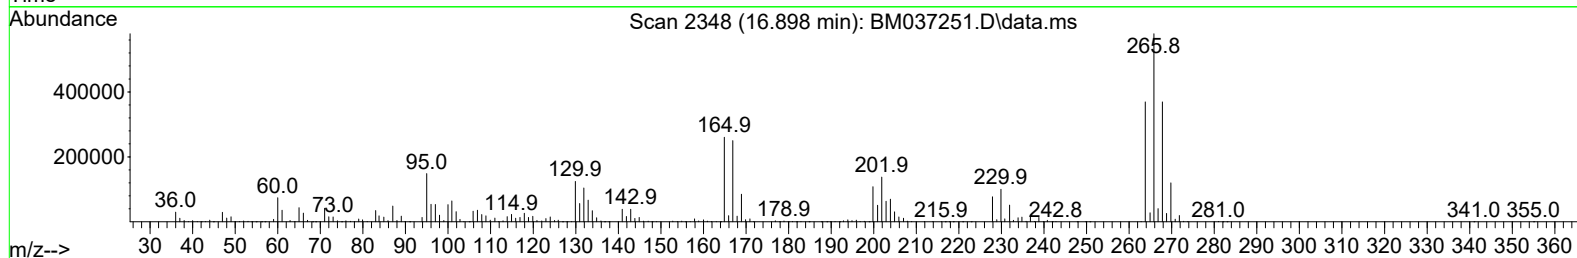


Quant Time: Oct 31 04:30:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 31 01:34:15 2022
Response via : Initial Calibration

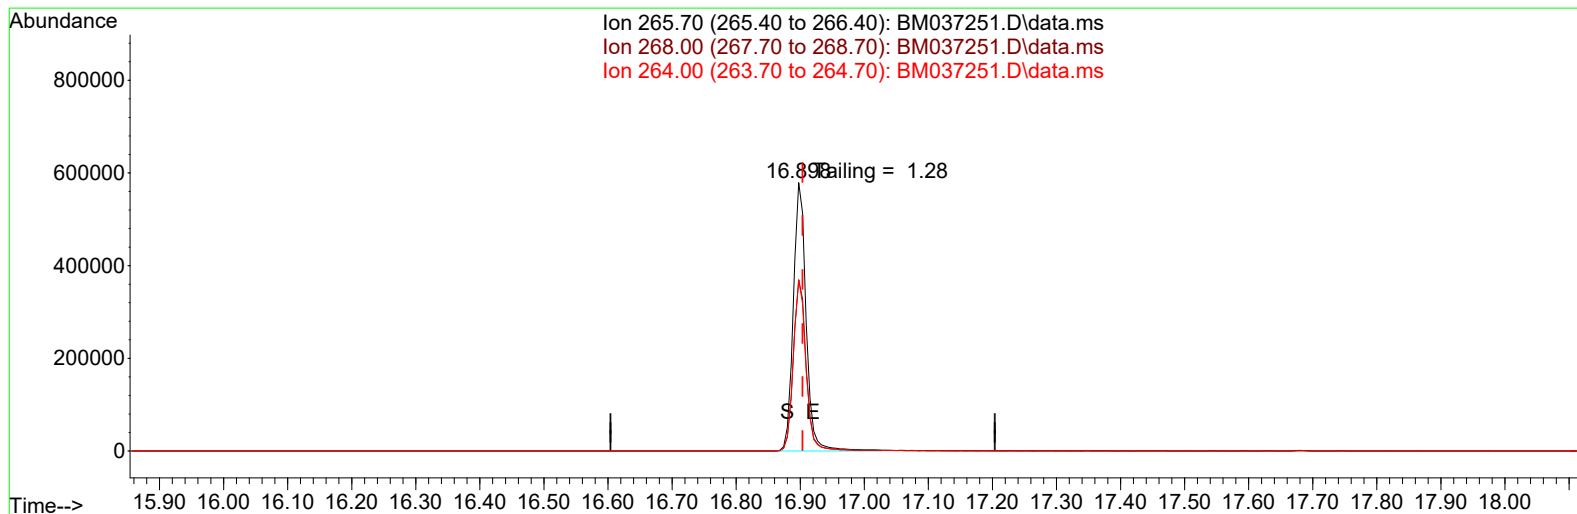

TIC: BM037251.D\data.ms

(70) Pentachlorophenol (C)




16.898min (-0.006) 178309.25 ng

response **813033**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.40	63.77
264.00	61.40	63.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102822\
Data File : BM037251.D
Acq On : 28 Oct 2022 11:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 31 04:30:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 31 01:34:15 2022
Response via : Initial Calibration

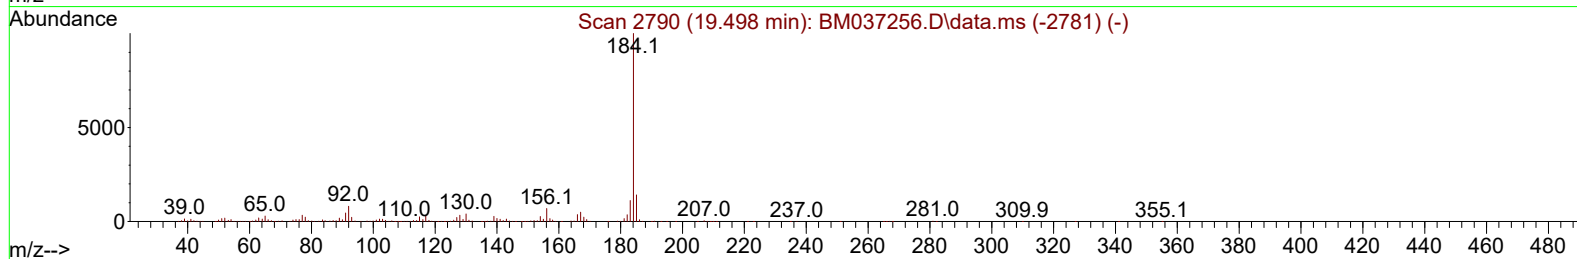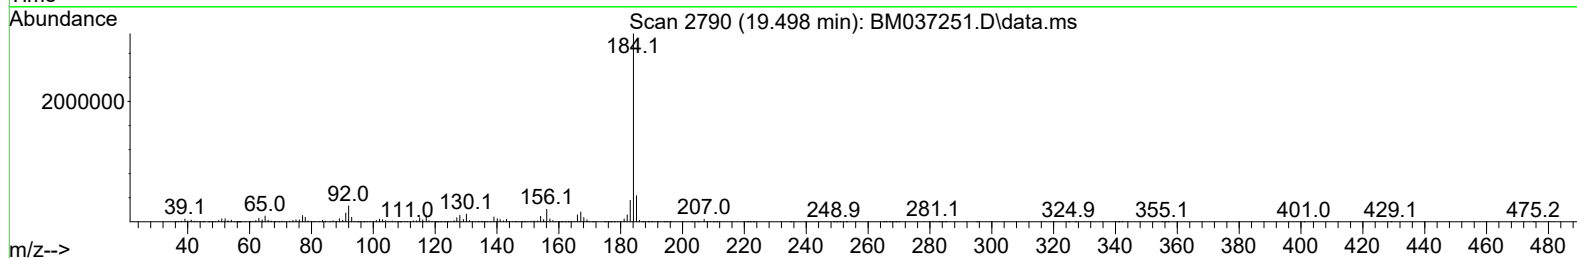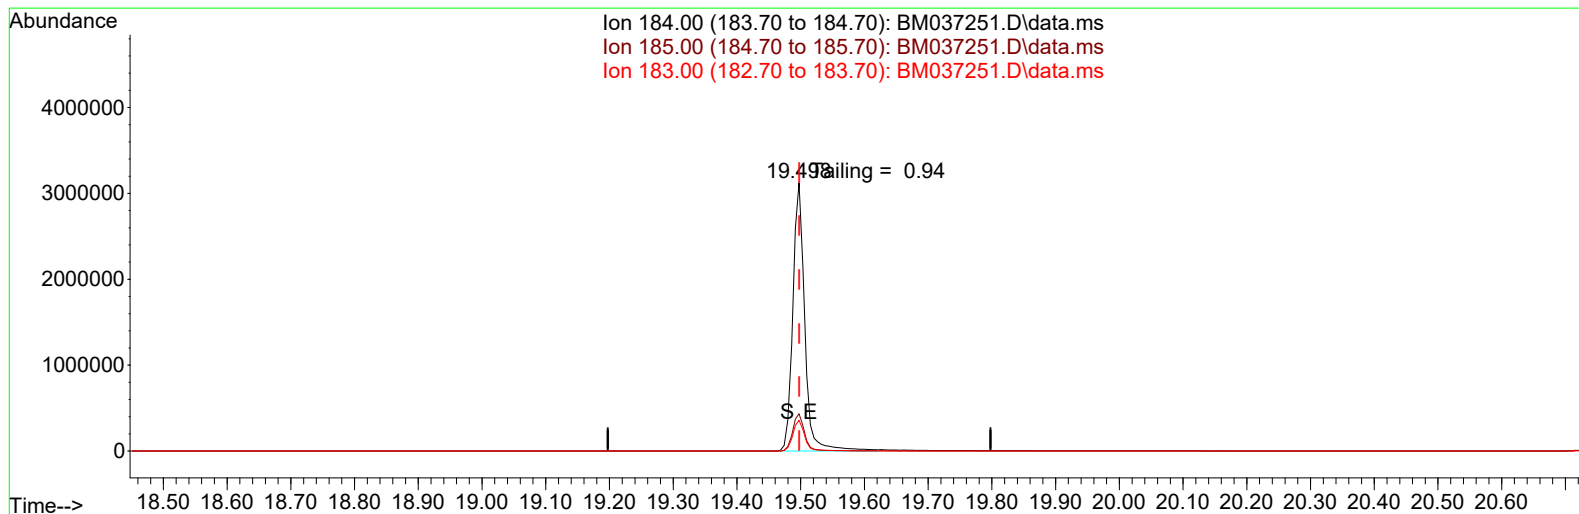

TIC: BM037251.D\data.ms

(77) Benzidine**19.498min (-0.000) 243728.32 ng****response 4124961**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.89
183.00	11.20	11.44
0.00	0.00	0.00