
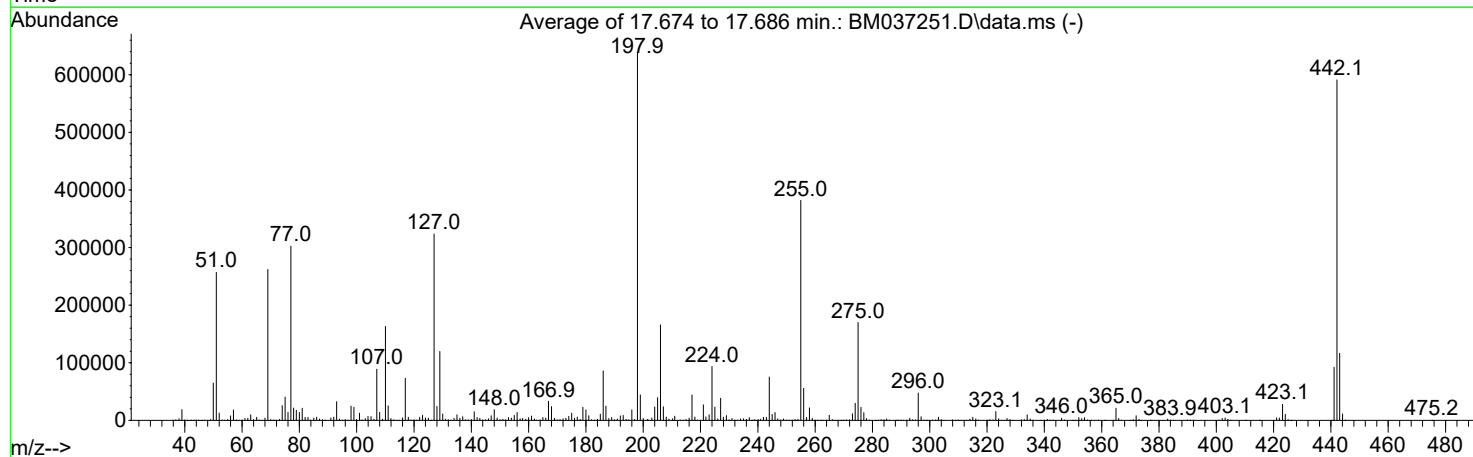


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102822\
 Data File : BM037251.D
 Acq On : 28 Oct 2022 11:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 31 01:34:15 2022

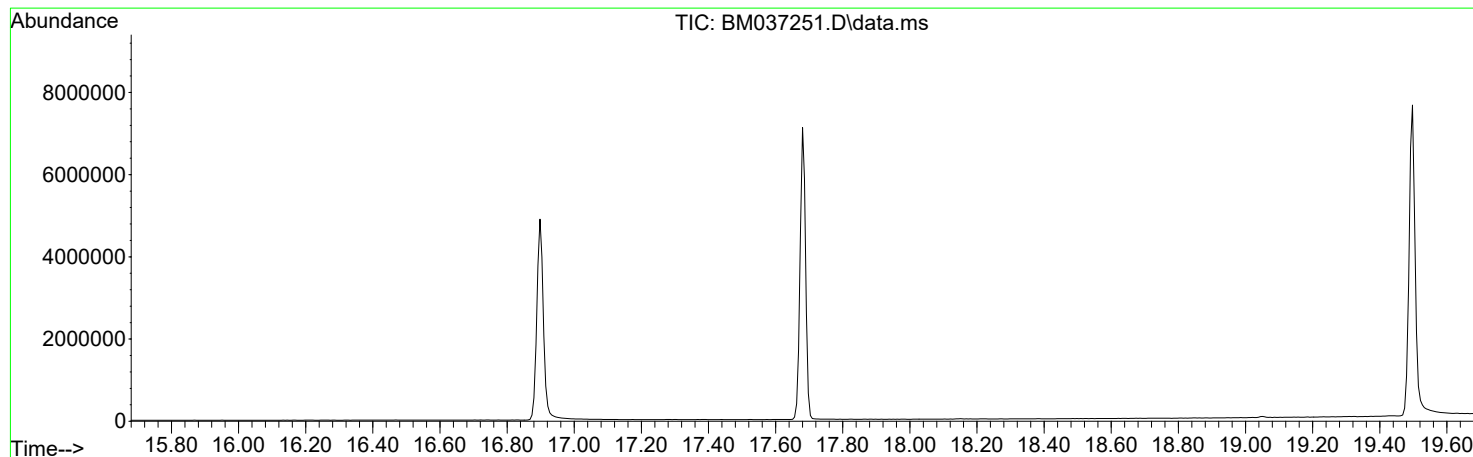




AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	257021	PASS
68	69	0.00	2	1.5	3899	PASS
69	198	0.00	100	41.0	261869	PASS
70	69	0.00	2	0.6	1475	PASS
127	198	10	80	50.7	323477	PASS
197	198	0.00	2	0.3	1751	PASS
198	198	100	100	100.0	638507	PASS
199	198	5	9	6.9	44125	PASS
275	198	10	60	26.6	169875	PASS
365	198	1	100	3.3	21147	PASS
441	198	0.01	100	14.4	92125	PASS
442	442	50	100	100.0	590891	PASS
443	442	15	24	19.7	116424	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102822\  
Data File : BM037251.D  
Acq On    : 28 Oct 2022  11:42  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 31 04:30:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 31 01:34:15 2022
Response via : Initial Calibration

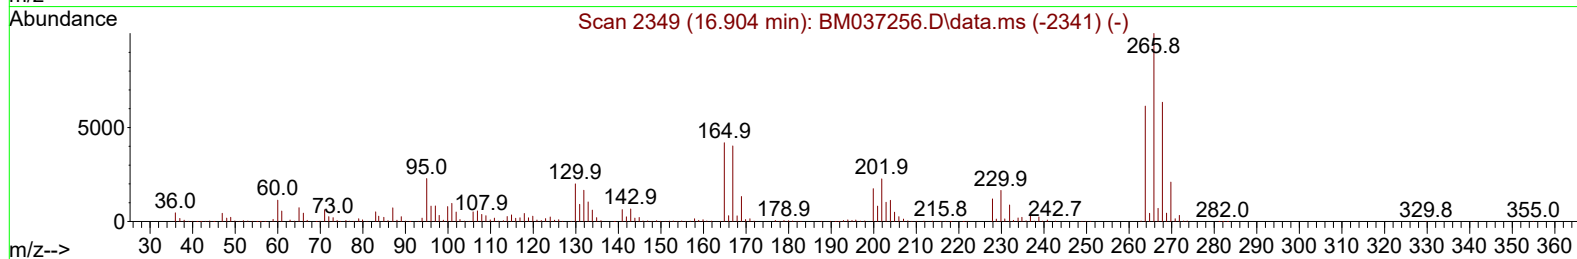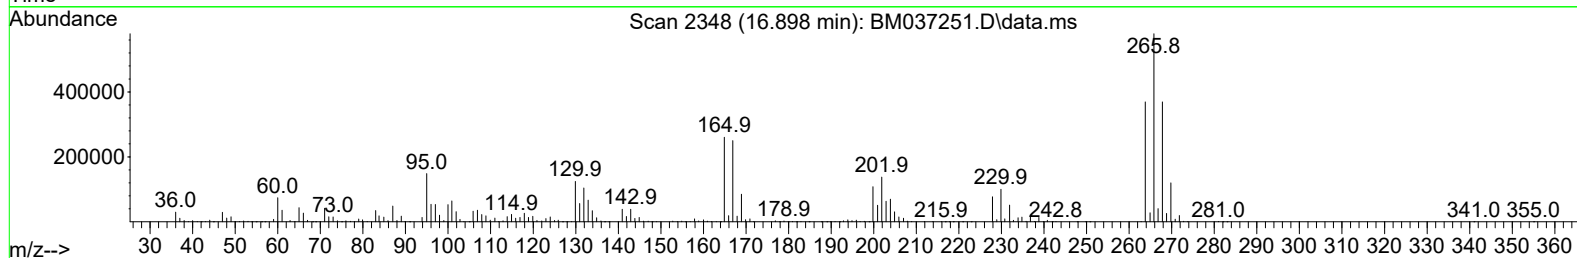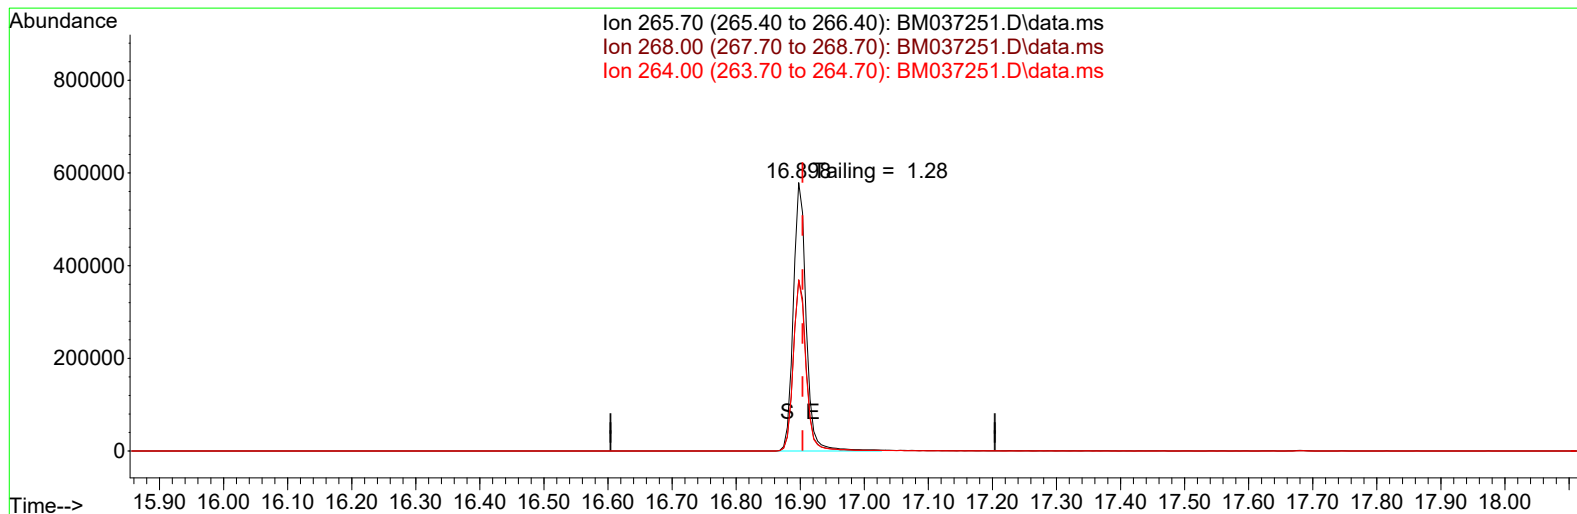

TIC: BM037251.D\data.ms

(70) Pentachlorophenol (C)

16.898min (-0.006) 178309.25 ng




response **813033**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.40	63.77
264.00	61.40	63.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102822\
Data File : BM037251.D
Acq On : 28 Oct 2022 11:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 31 04:30:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 31 01:34:15 2022
Response via : Initial Calibration

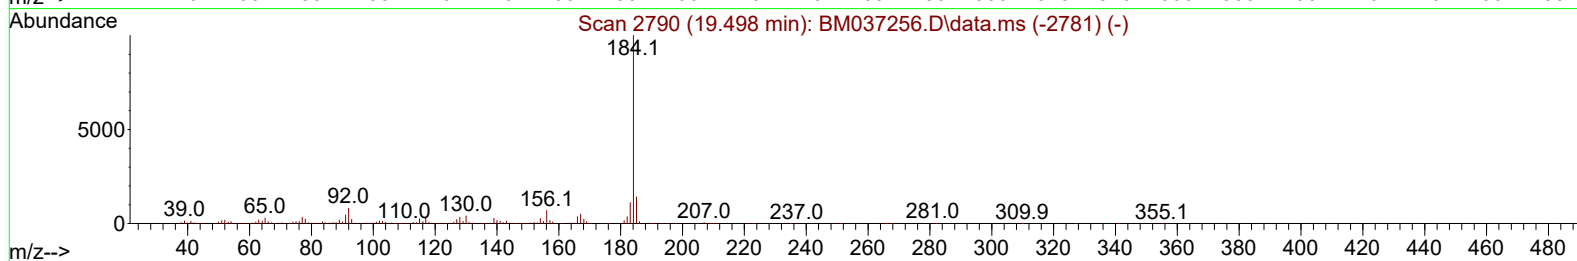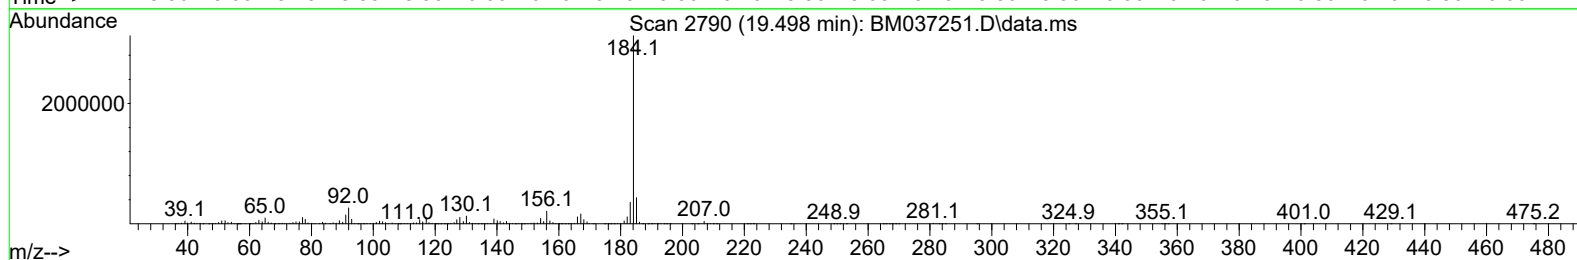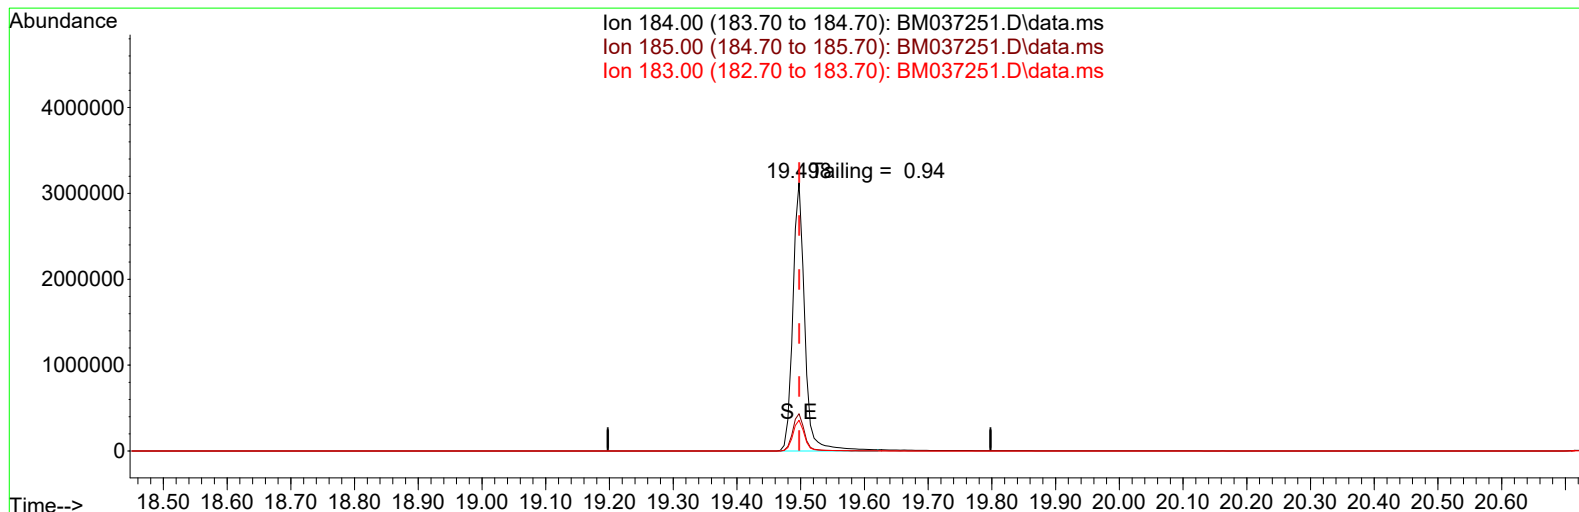

TIC: BM037251.D\data.ms

(77) Benzidine

19.498min (-0.000) 243728.32 ng

response 4124961

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.89
183.00	11.20	11.44
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/28/2022	BNA_M	<u>BM037251.D</u>
Compound Name	Response	Retention Time
DDT	1995535	20.721
DDD	42819	20.28
DDE	1185	19.774
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
44004	2039539	2.16

Instrument :
BNA_M
ClientSampleId :
DFTPP