
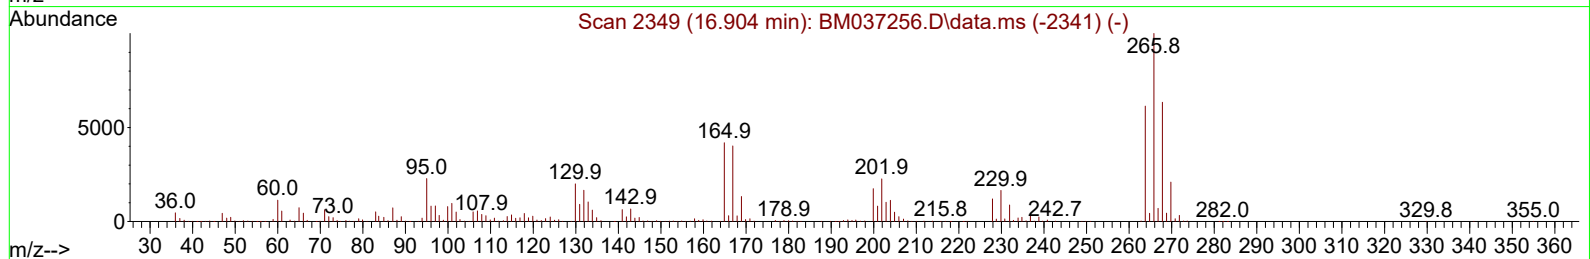
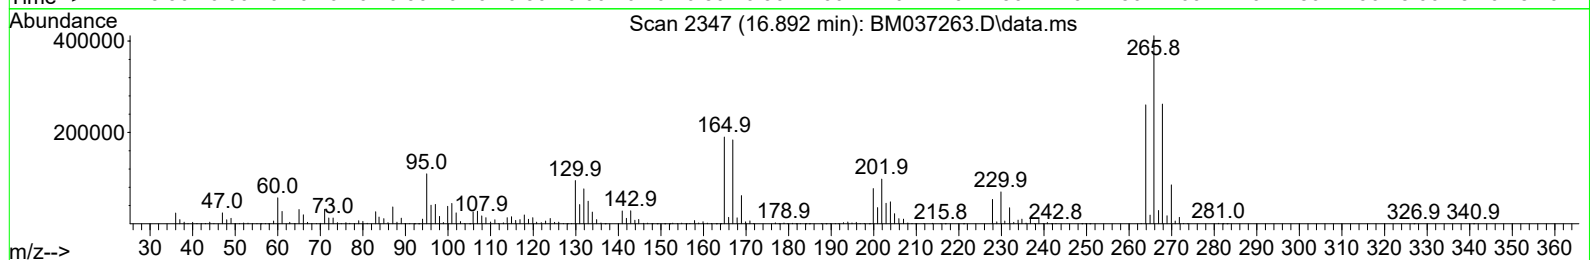


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102922\
Data File : BM037263.D
Acq On : 29 Oct 2022 10:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 31 04:41:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 31 01:34:15 2022
Response via : Initial Calibration

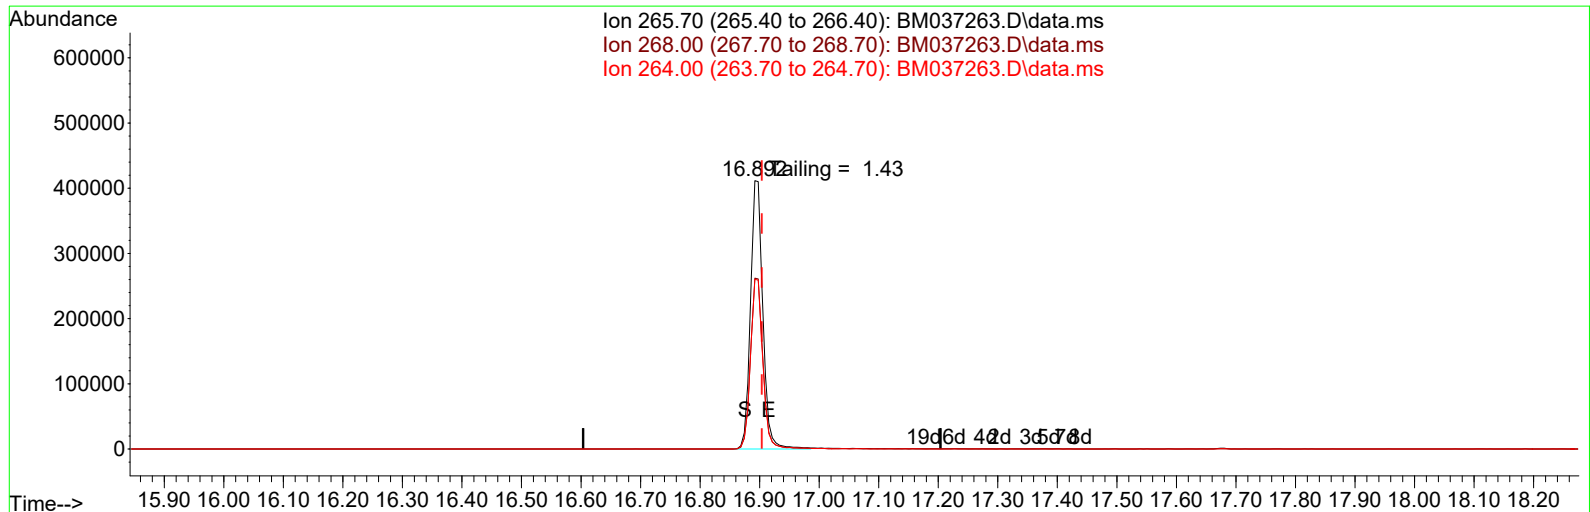

TIC: BM037263.D\data.ms

(70) Pentachlorophenol (C)




16.892min (-0.012) 24281.23 ng m

response 604997

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.40	63.69
264.00	61.40	63.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102922\
 Data File : BM037263.D
 Acq On : 29 Oct 2022 10:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 31 04:41:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 31 01:34:15 2022
 Response via : Initial Calibration

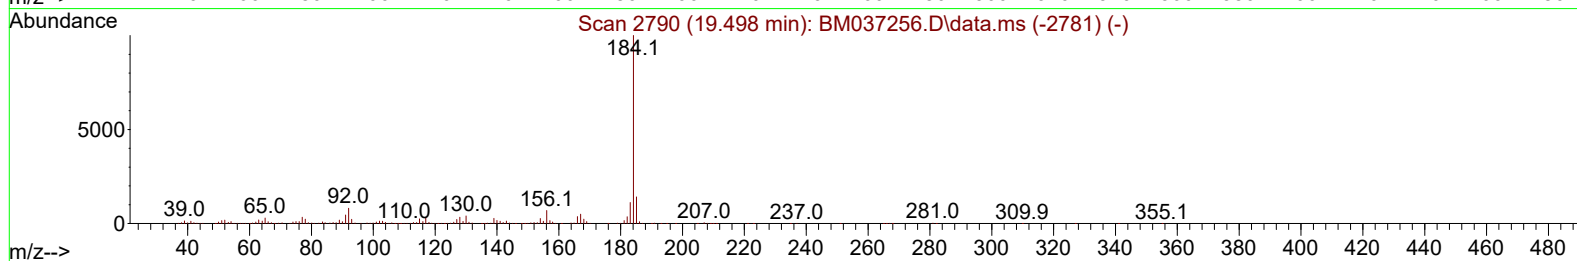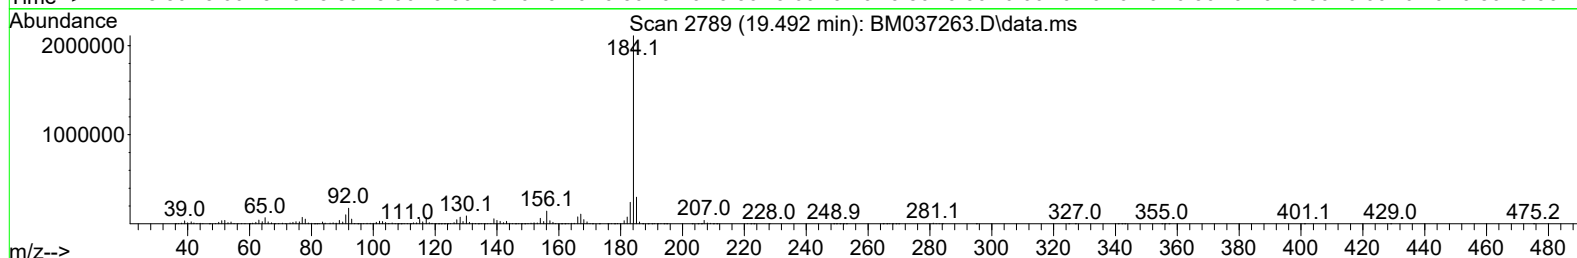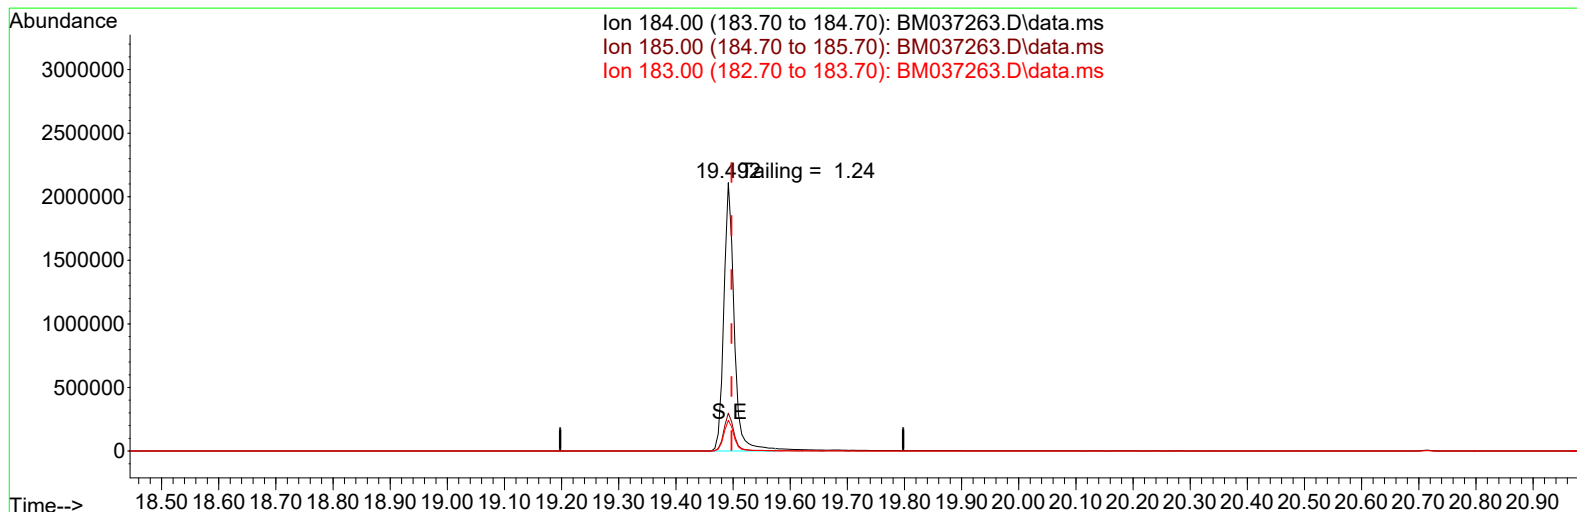

TIC: BM037263.D\data.ms

(77) Benzidine

19.492min (-0.006) 3332708.65 ng m

response 2782937

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.13
183.00	11.20	11.42
0.00	0.00	0.00